




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021250.D
Acq On : 31 Jul 2024 02:28
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Manual IntegrationsAPPROVED

Quant Time: Jul 31 03:07:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

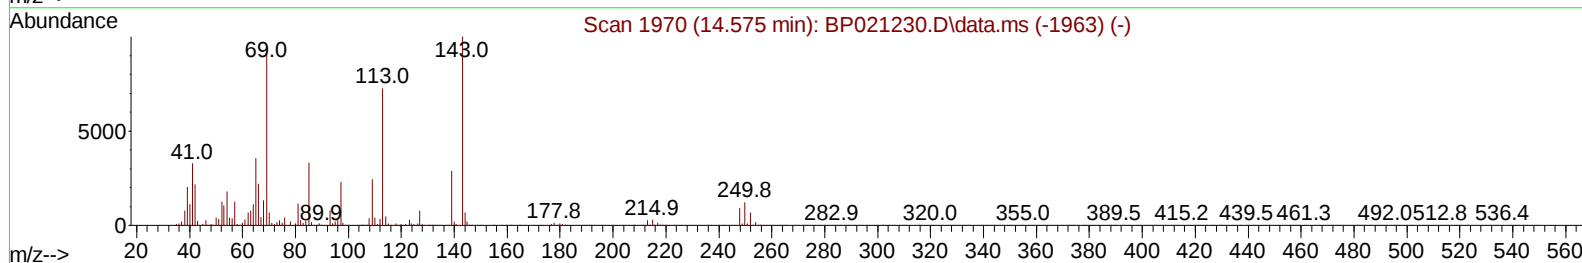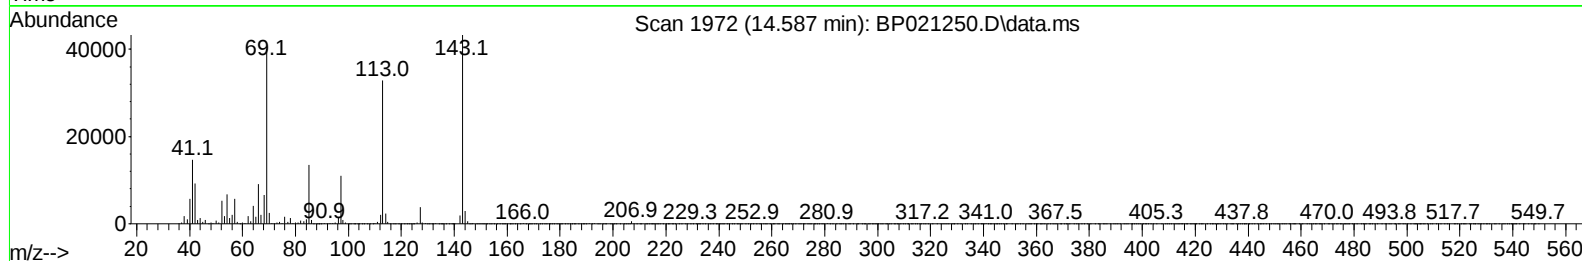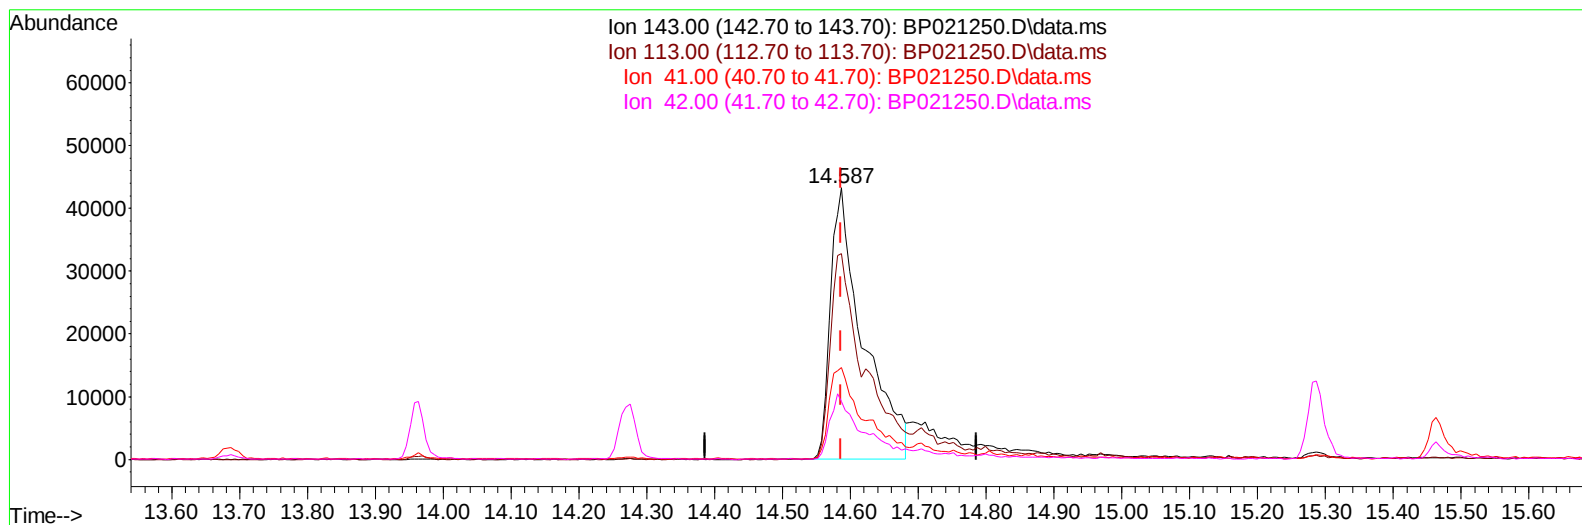

TIC: BP021250.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.001) 23.19 ng/u1

response 144103

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	75.90
41.00	37.90	33.86
42.00	27.10	21.25#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021250.D
Acq On : 31 Jul 2024 02:28
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Manual IntegrationsAPPROVED

Quant Time: Jul 31 03:07:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

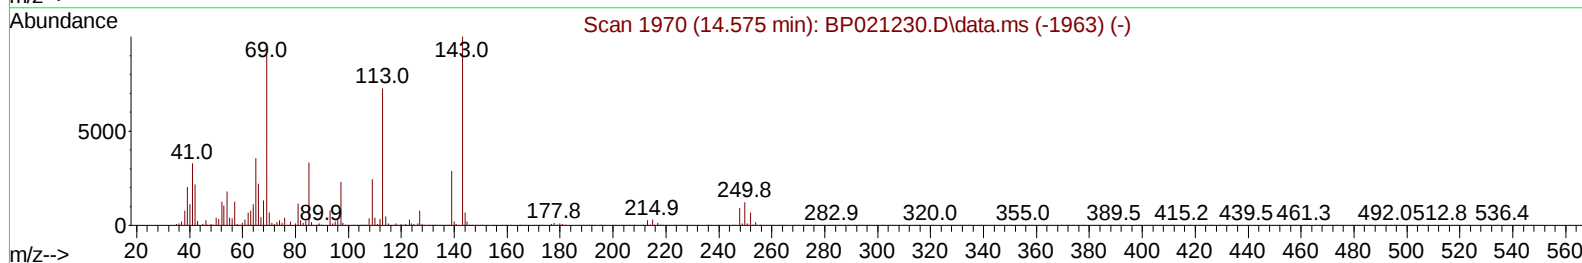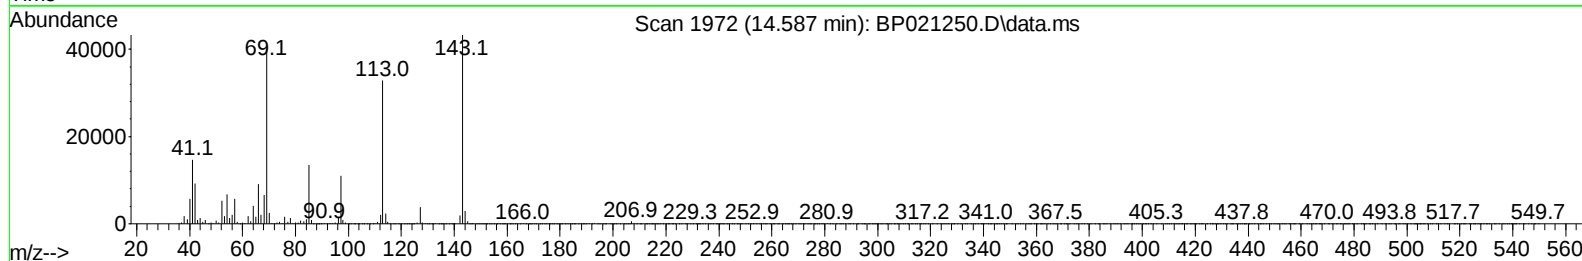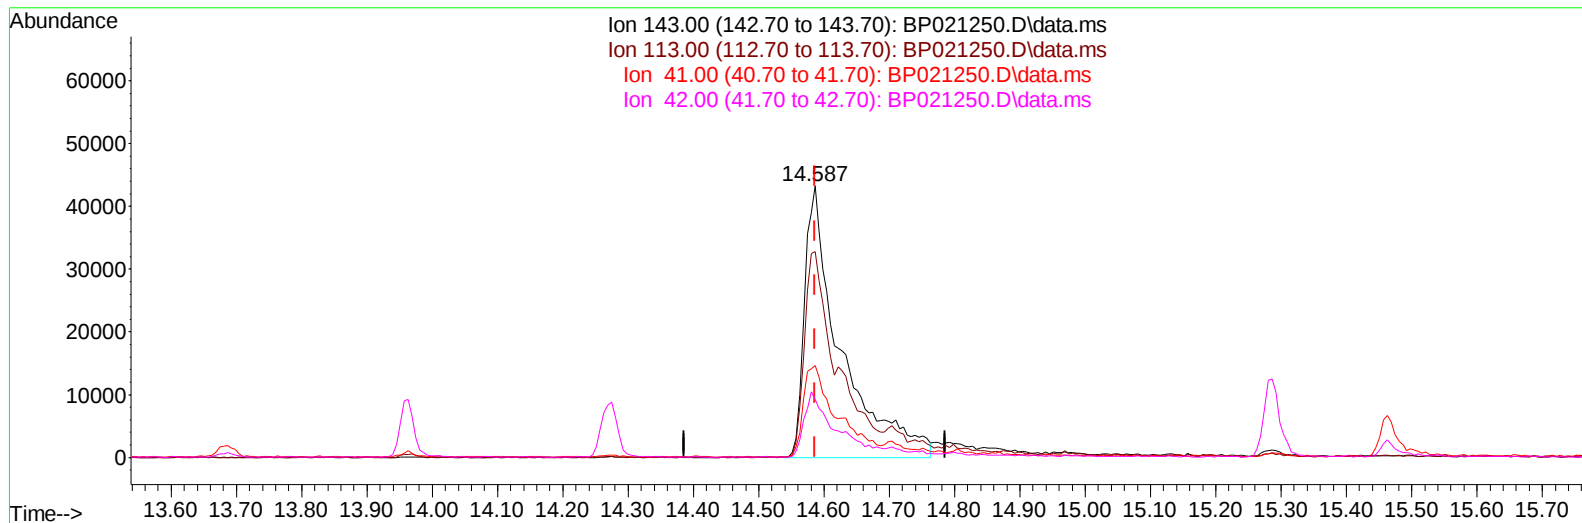

TIC: BP021250.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.001) 26.68 ng/ul m

response 165808

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	75.90
41.00	37.90	33.86
42.00	27.10	21.25#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021250.D
 Acq On : 31 Jul 2024 02:28
 Operator : MA/JU
 Sample : PB162326BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK326

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/31/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Jul 31 03:09:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	225412	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	886449	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	600904	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	1370181	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1400457	20.000	ng/ul	0.01
88) Perylene-d12	24.839	264	1446226	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	26386	5.327	ng/uL	0.00
4) Pyridine-d5	3.587	84	339805	23.695	ng/ul	0.00
7) Phenol-d5	6.846	99	447216	24.335	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	262411	23.562	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	387045	25.562	ng/ul	0.00
15) 4-Methylphenol-d8	8.364	113	376146	24.644	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	188122	27.323	ng/ul	0.00
24) 2-Nitrophenol-d4	9.511	143	220125	27.933	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.052	165	370581	26.006	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	503837	26.690	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	1265439	28.969	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	1367336	27.877	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	165808m	26.678	ng/ul	0.00
60) Fluorene-d10	15.287	176	1076465	30.038	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	199343	24.045	ng/ul	0.00
73) Anthracene-d10	17.204	188	1763162	28.972	ng/ul	0.01
81) Pyrene-d10	19.586	212	2242029	25.895	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.627	264	2119969	29.722	ng/ul	0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021250.D
Acq On : 31 Jul 2024 02:28
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

Quant Time: Jul 31 03:09:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

