




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021277.D
Acq On : 01 Aug 2024 02:35
Operator : CG/JU
Sample : P3264-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BE1

Manual IntegrationsAPPROVED

Quant Time: Aug 01 04:22:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :mohammad ahmed 09/04/2024

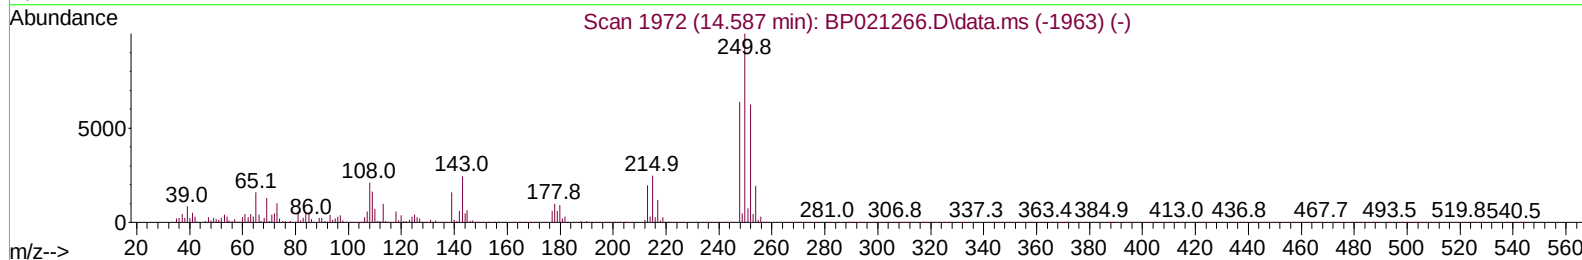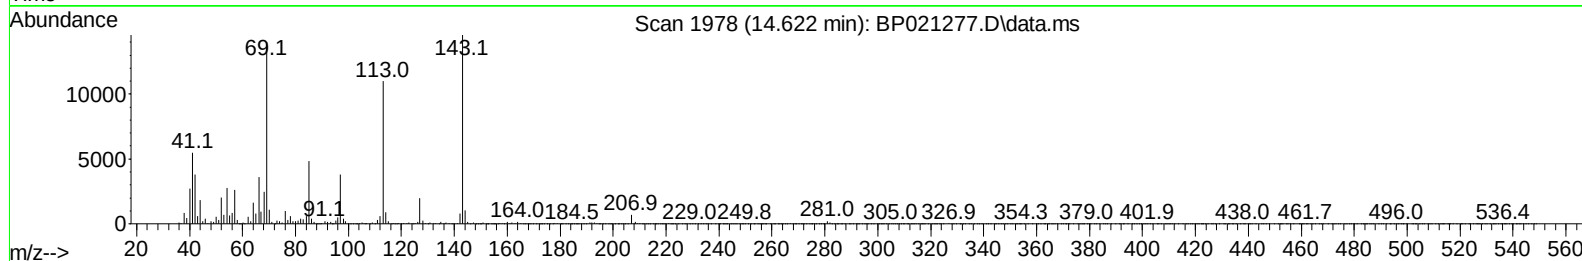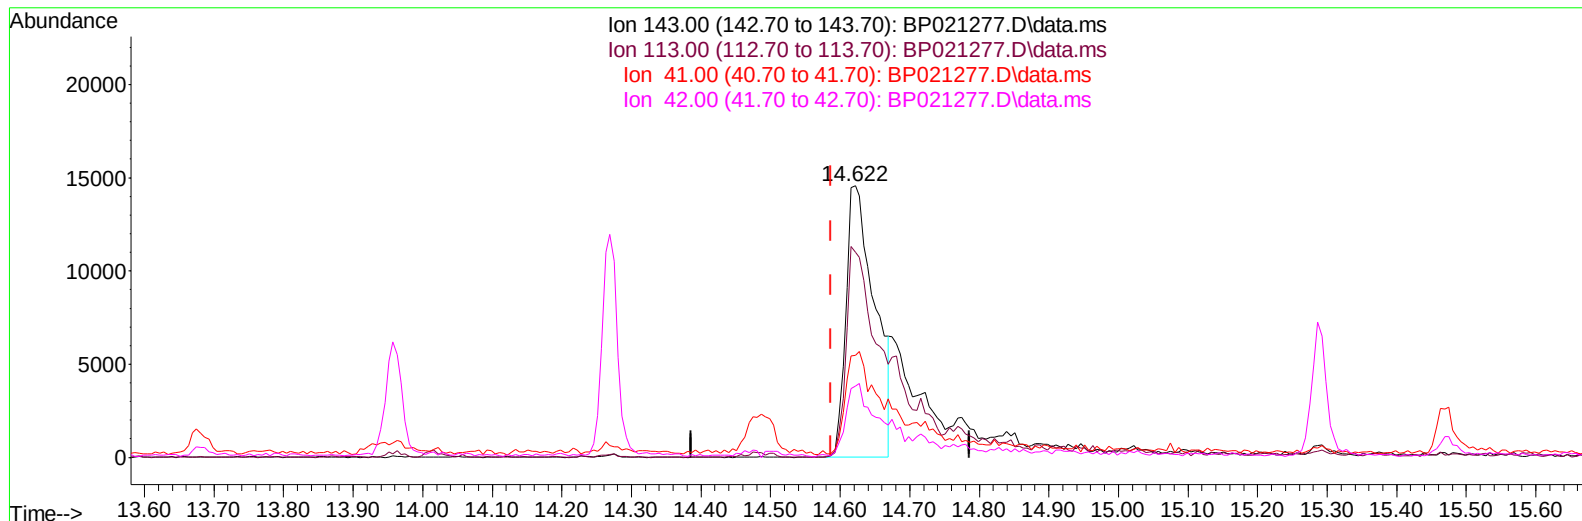

TIC: BP021277.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (+ 0.036) 6.46 ng/ul

response 41813

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	75.56
41.00	37.90	37.65
42.00	27.10	26.22




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021277.D
Acq On : 01 Aug 2024 02:35
Operator : CG/JU
Sample : P3264-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BE1

Manual IntegrationsAPPROVED

Quant Time: Aug 01 04:22:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :mohammad ahmed 09/04/2024

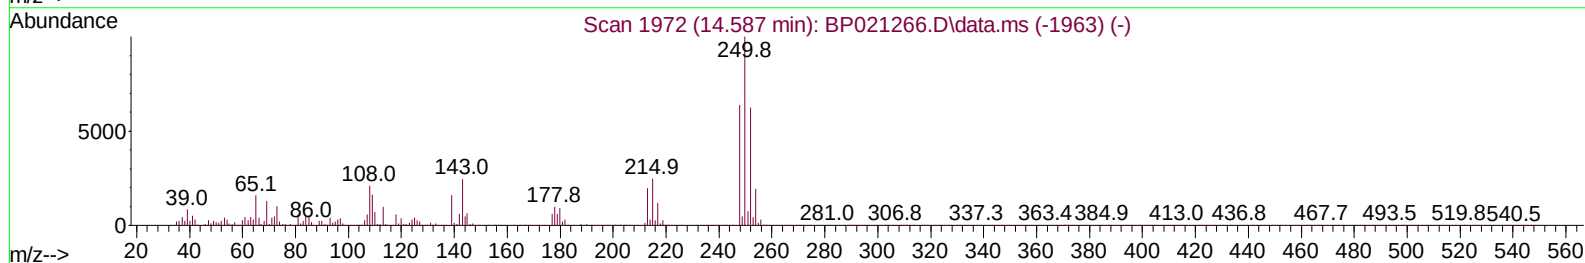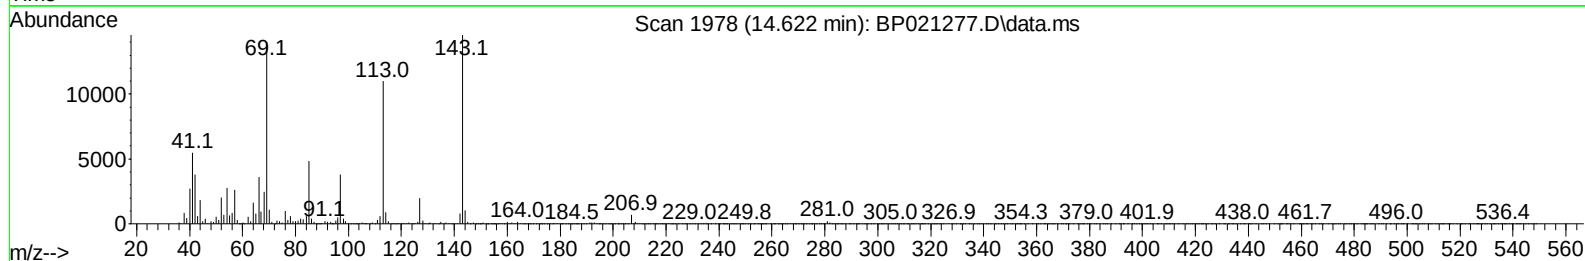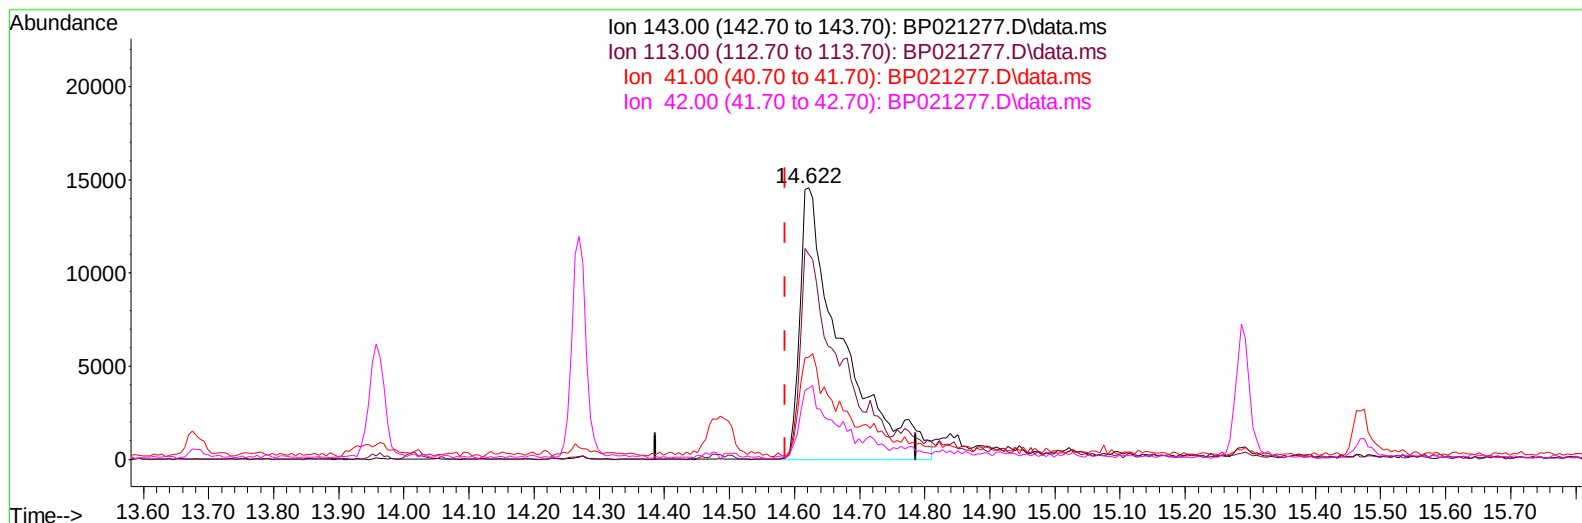

TIC: BP021277.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (+ 0.036) 10.07 ng/ul m

response 65143

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	75.56
41.00	37.90	37.65
42.00	27.10	26.22

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021277.D
 Acq On : 01 Aug 2024 02:35
 Operator : CG/JU
 Sample : P3264-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BE1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/01/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Aug 01 04:25:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	232423	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	965435	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	625335	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188	1132797	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	1033330	20.000	ng/ul	0.00
88) Perylene-d12	24.827	264	1189387	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	13611	2.665	ng/uL	0.00
4) Pyridine-d5	3.599	84	178176	12.050	ng/ul	0.00
7) Phenol-d5	6.863	99	262317	13.843	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.981	67	166474	14.497	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	203809	13.054	ng/ul	0.01
15) 4-Methylphenol-d8	8.369	113	230718	14.660	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	103112	13.751	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	117134	13.648	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	211001	13.596	ng/ul	0.02
31) 4-Chloroaniline-d4	10.569	131	230523	11.212	ng/ul	0.01
46) Dimethylphthalate-d6	13.681	166	726753	15.987	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	793514	15.546	ng/ul	0.00
54) 4-Nitrophenol-d4	14.622	143	65143m	10.072	ng/ul	0.04
60) Fluorene-d10	15.286	176	513615	13.772	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	66788	9.744	ng/ul	0.00
73) Anthracene-d10	17.192	188	832923	16.555	ng/ul	0.00
81) Pyrene-d10	19.575	212	1128923	17.671	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.598	264	1005784	17.146	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021277.D
Acq On : 01 Aug 2024 02:35
Operator : CG/JU
Sample : P3264-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BE1

Manual IntegrationsAPPROVED

Quant Time: Aug 01 04:25:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :mohammad ahmed 09/04/2024

