




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021281.D
Acq On : 01 Aug 2024 06:12
Operator : CG/JU
Sample : PB162151BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Manual IntegrationsAPPROVED

Quant Time: Aug 01 07:20:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :mohammad ahmed 09/04/2024

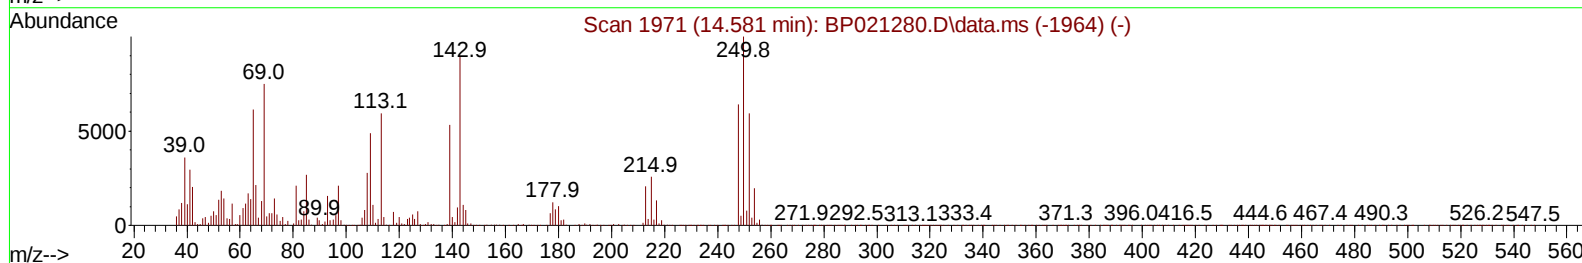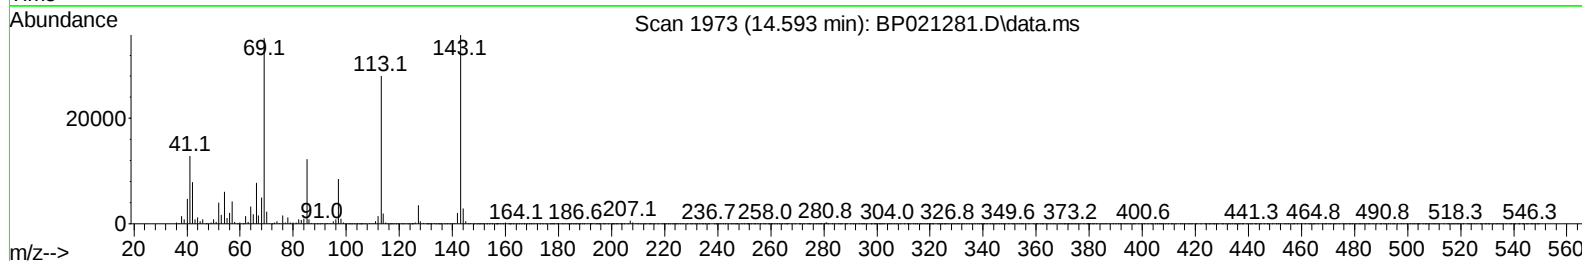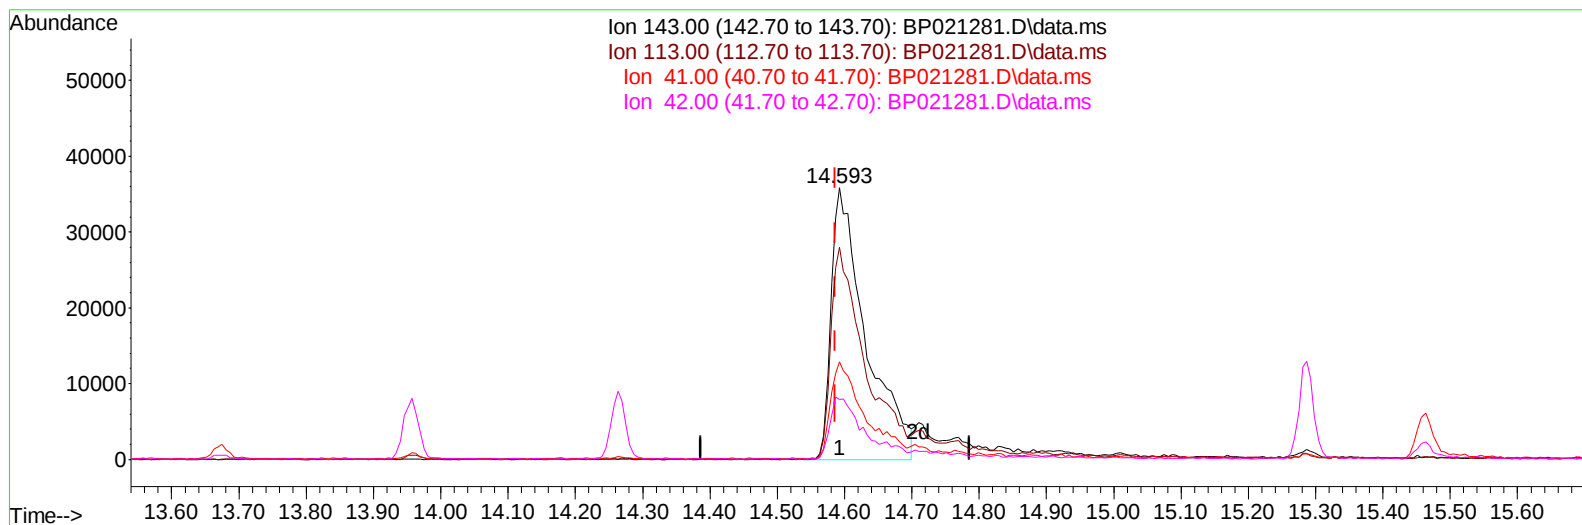

TIC: BP021281.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.593min (+ 0.006) 23.48 ng/ul

response 127870

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	78.16
41.00	37.90	36.03
42.00	27.10	22.05




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021281.D
Acq On : 01 Aug 2024 06:12
Operator : CG/JU
Sample : PB162151BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Manual IntegrationsAPPROVED

Quant Time: Aug 01 07:20:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :mohammad ahmed 09/04/2024

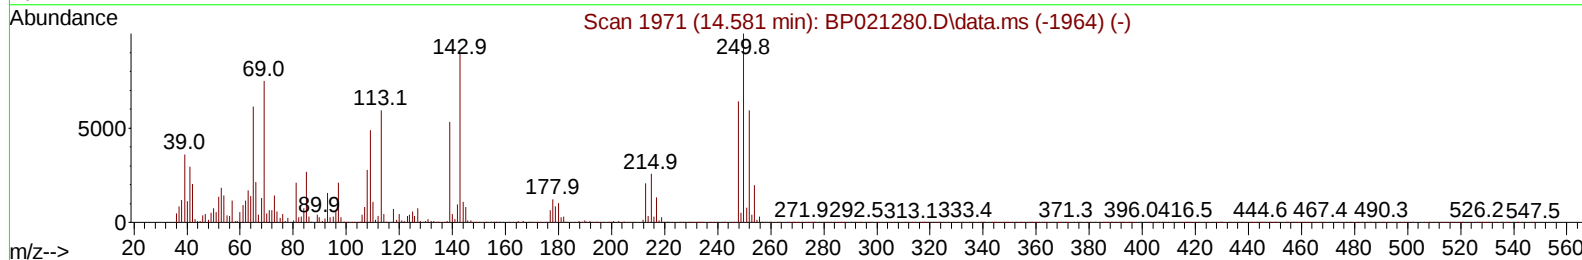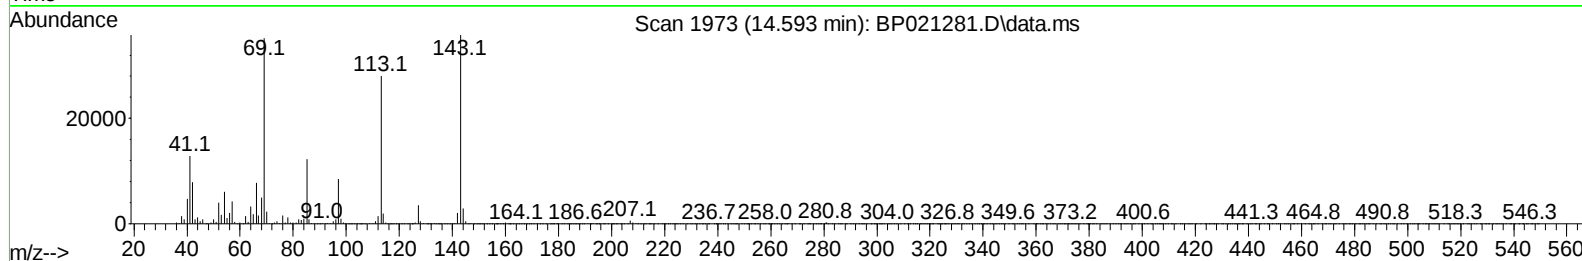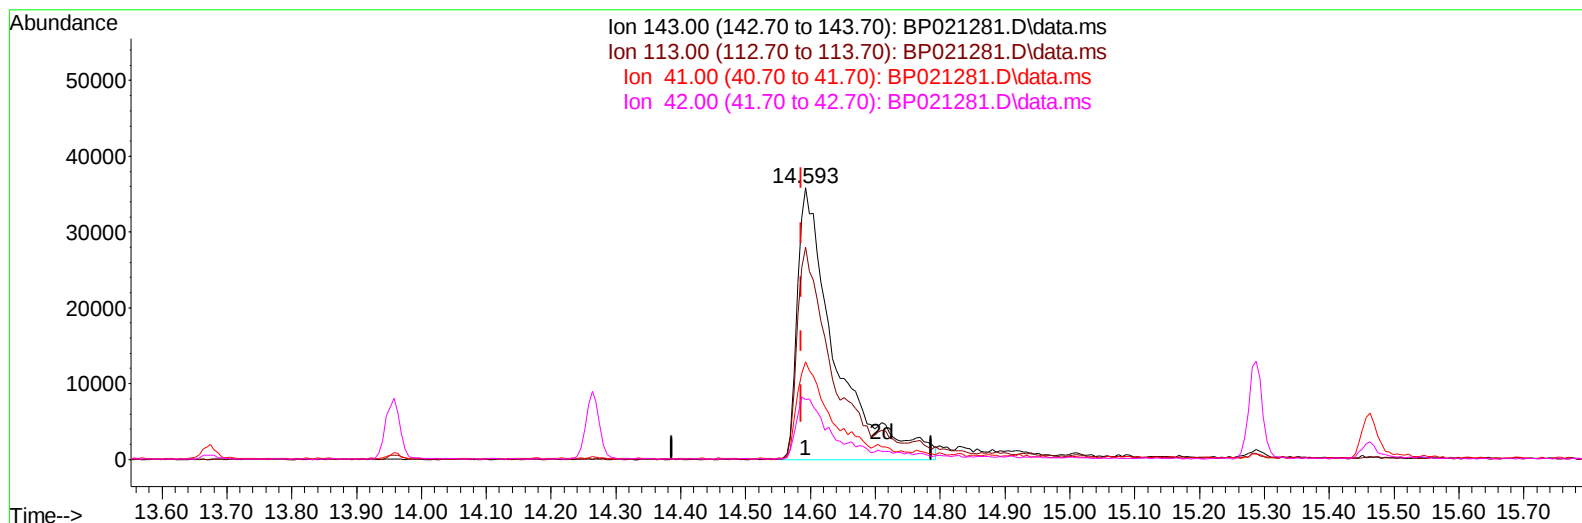

TIC: BP021281.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.593min (+ 0.006) 26.51 ng/ul m

response 144394

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	78.16
41.00	37.90	36.03
42.00	27.10	22.05

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021281.D
 Acq On : 01 Aug 2024 06:12
 Operator : CG/JU
 Sample : PB162151BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK151

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/01/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Aug 01 08:02:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	205173	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	801115	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	526625	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	1172546	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	1018333	20.000	ng/ul	# 0.00
88) Perylene-d12	24.839	264	1095167	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	24594	5.455	ng/uL	0.00
4) Pyridine-d5	3.587	84	322527	24.709	ng/ul	0.00
7) Phenol-d5	6.846	99	419093	25.055	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	246909	24.357	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	373113	27.073	ng/ul	0.00
15) 4-Methylphenol-d8	8.364	113	362373	26.084	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	178971	28.763	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	208000	29.206	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.058	165	352147	27.345	ng/ul	0.00
31) 4-Chloroaniline-d4	10.558	131	485799	28.475	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	1200137	31.349	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	1274816	29.656	ng/ul	0.00
54) 4-Nitrophenol-d4	14.593	143	144394m	26.510	ng/ul	0.00
60) Fluorene-d10	15.287	176	1009905	32.156	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	168104	23.695	ng/ul	0.00
73) Anthracene-d10	17.192	188	1645407	31.595	ng/ul	0.00
81) Pyrene-d10	19.575	212	1942420	30.853	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.604	264	1721909	31.879	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021281.D
Acq On : 01 Aug 2024 06:12
Operator : CG/JU
Sample : PB162151BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :mohammad ahmed 09/04/2024

Quant Time: Aug 01 08:02:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

