

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021225.D
 Acq On : 30 Jul 2024 02:34
 Operator : MA/JU
 Sample : P3300-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1G92

Quant Time: Jul 30 03:46:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 09/04/2024

07/30/2024
 Supervised By :mohammad
 ahmed

08/03/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	186984	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	709843	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.269	164	443131	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.087	188	946157	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1022253	20.000	ng/u1	0.00
88) Perylene-d12	24.821	264	1224145	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	18015	4.384	ng/uL	0.00
4) Pyridine-d5	3.605	84	78951	6.637	ng/u1	0.01
7) Phenol-d5	6.864	99	109882	7.208	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.987	67	229909	24.886	ng/u1	0.00
11) 2-Chlorophenol-d4	7.187	132	289487	23.048	ng/u1	0.00
15) 4-Methylphenol-d8	8.369	113	203123	16.043	ng/u1	0.00
21) Nitrobenzene-d5	8.799	128	139216	25.250	ng/u1	0.00
24) 2-Nitrophenol-d4	9.510	143	158059	25.047	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.052	165	286706	25.126	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	366281	24.230	ng/u1	0.00
46) Dimethylphthalate-d6	13.687	166	951331	29.532	ng/u1	0.00
49) Acenaphthylene-d8	13.957	160	1012981	28.005	ng/u1	0.00
54) 4-Nitrophenol-d4	14.634	143	34028m	7.424	ng/u1	0.05
60) Fluorene-d10	15.287	176	725368	27.447	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	138503	24.194	ng/u1	0.00
73) Anthracene-d10	17.192	188	1352879	32.193	ng/u1	0.00
81) Pyrene-d10	19.575	212	1687464	26.700	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.598	264	2020576	33.467	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.422	149	126583	2.718	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021225.D
Acq On : 30 Jul 2024 02:34
Operator : MA/JU
Sample : P3300-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G92


Quant Time: Jul 30 03:46:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 09/04/2024

07/30/2024
Supervised By :mohammad
ahmed


08/03/2024

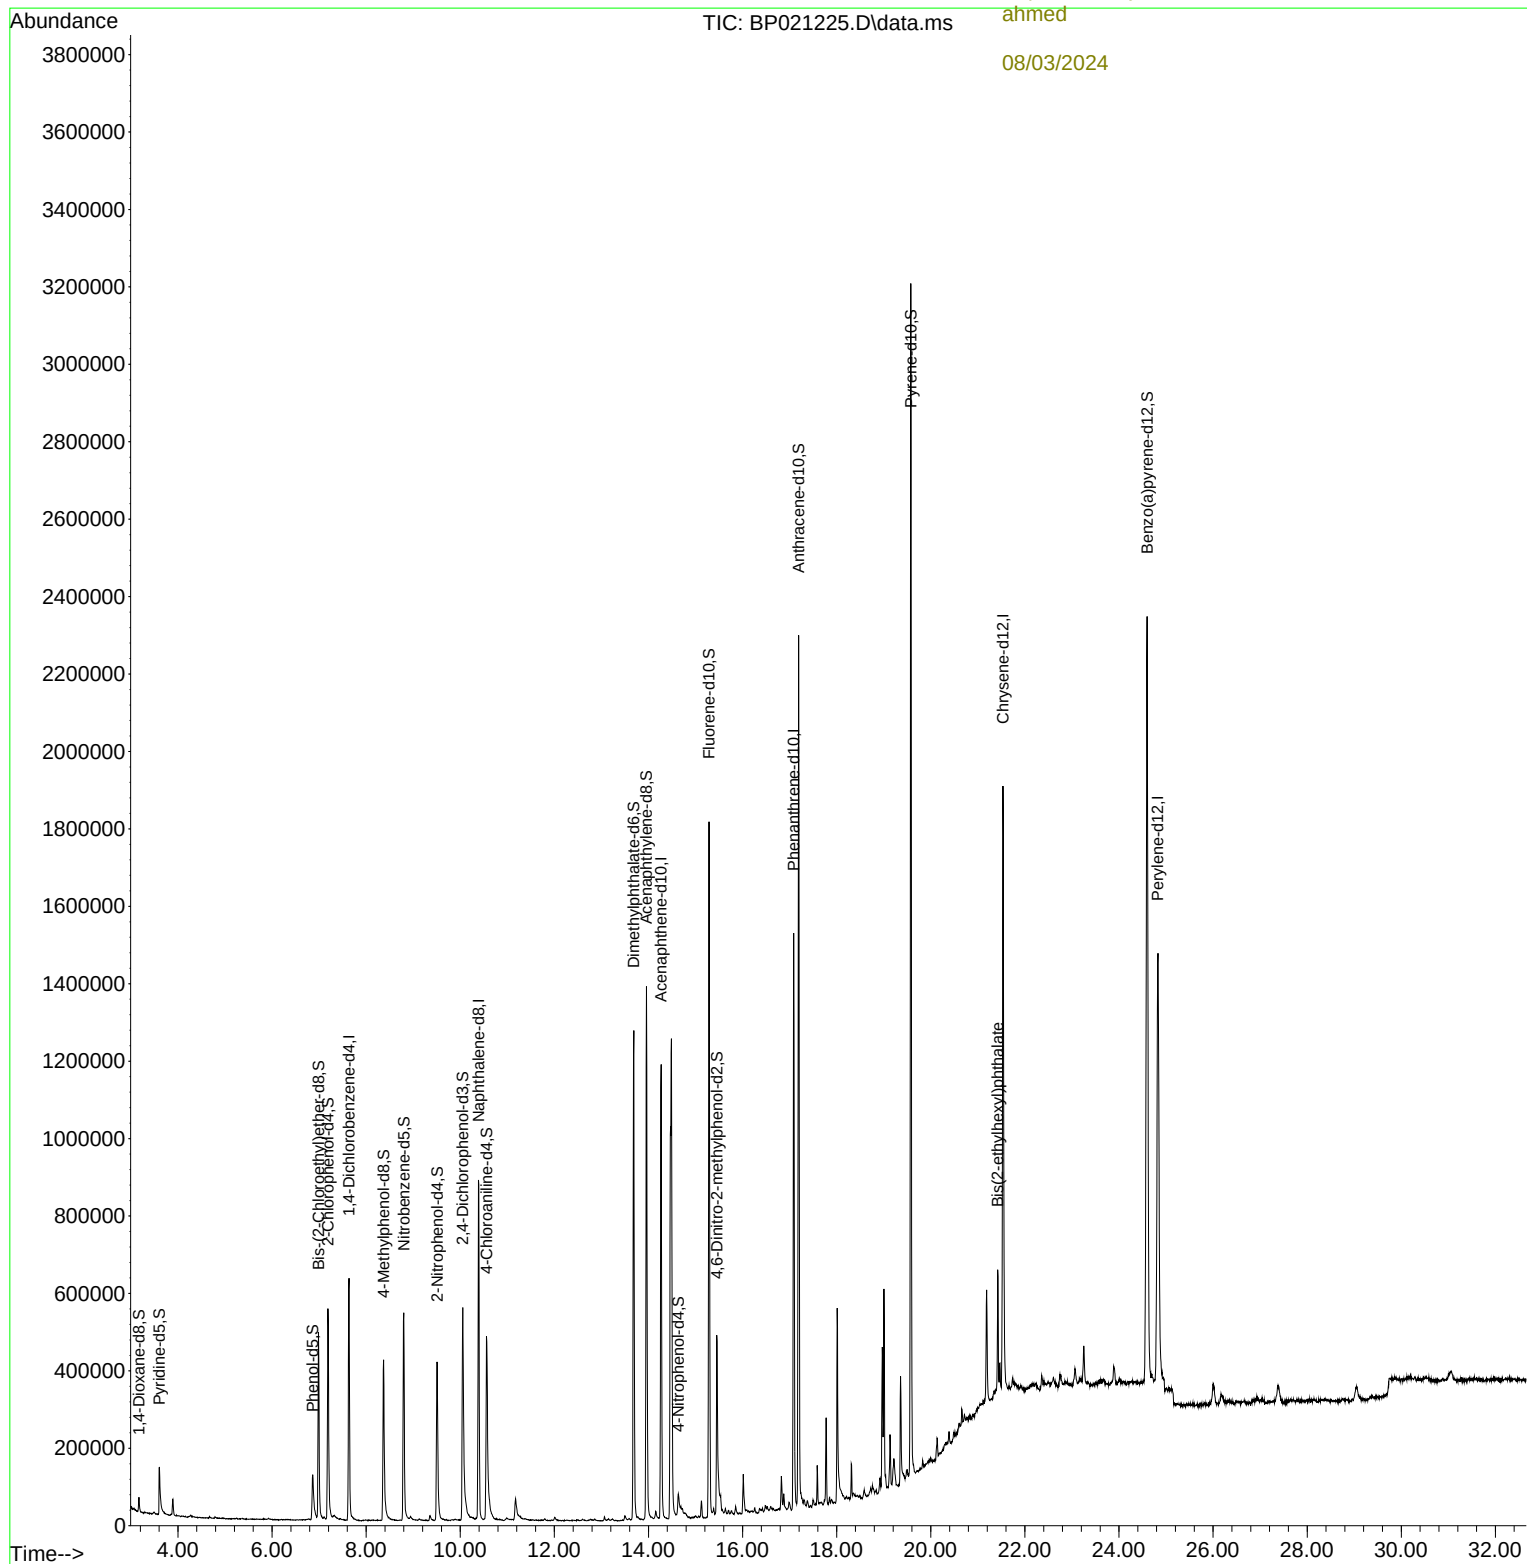

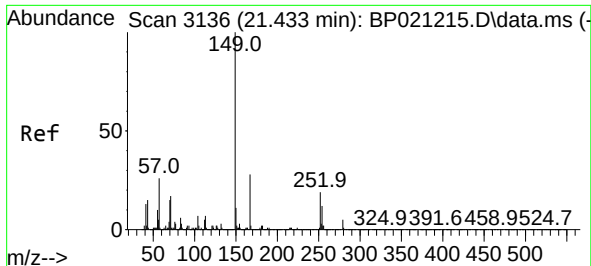

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.718 ng/ul
 RT: 21.422 min Scan# 3136
 Delta R.T. 0.000 min
 Lab File: BP021225.D
 Acq: 30 Jul 2024 02:34



Instrument :
 BNA_P
 ClientSampleId :
 E1G92

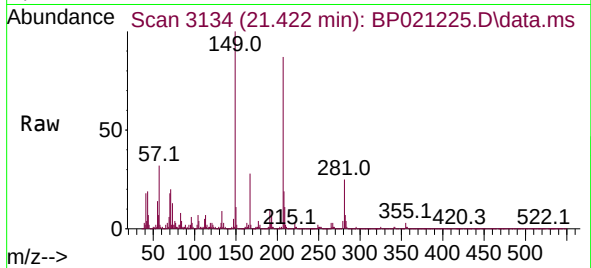

Tgt Ion:149 Resp: 126583
 Ion Ratio Lower Upper
 149 100
 167 27.9 22.1 33.1
 279 4.0 3.7 5.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 09/04/2024

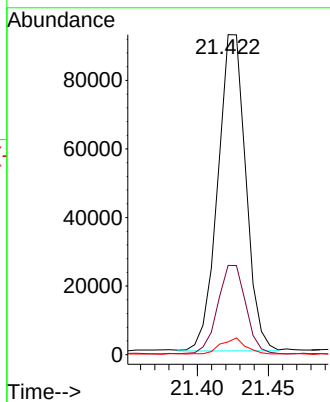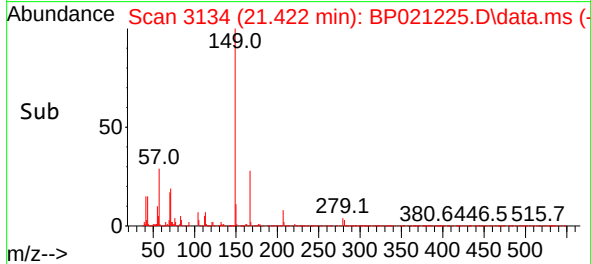

07/30/2024
 Supervised By :mohammad
 ahmed

08/03/2024