

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021240.D
 Acq On : 30 Jul 2024 18:31
 Operator : MA/JU
 Sample : P3359-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1G78

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/31/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Jul 30 23:25:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	151466	20.000	ng/u1	0.00
20) Naphthalene-d8	10.404	136	602164	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.275	164	406455	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.104	188	903345	20.000	ng/u1	0.01
79) Chrysene-d12	21.545	240	996491	20.000	ng/u1	# 0.01
88) Perylene-d12	24.845	264	1074408	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	14174	4.258	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.864	99	104537	8.466	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.981	67	123623	16.519	ng/u1	0.00
11) 2-Chlorophenol-d4	7.187	132	174246	17.126	ng/u1	0.00
15) 4-Methylphenol-d8	8.369	113	161971	15.793	ng/u1	0.00
21) Nitrobenzene-d5	8.793	128	83918	17.942	ng/u1	0.00
24) 2-Nitrophenol-d4	9.505	143	94133	17.584	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	170637m	17.628	ng/u1	0.02
31) 4-Chloroaniline-d4	10.575	131	115835	9.033	ng/u1	0.02
46) Dimethylphthalate-d6	13.687	166	611279	20.688	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	649698	19.583	ng/u1	0.00
54) 4-Nitrophenol-d4	14.657	143	19259m	4.581	ng/u1	0.07
60) Fluorene-d10	15.298	176	538543	22.217	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.481	200	77719	14.219	ng/u1	0.02
73) Anthracene-d10	17.204	188	916184	22.835	ng/u1	0.01
81) Pyrene-d10	19.580	212	1226587	19.910	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.610	264	1293817	24.416	ng/u1	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.433	149	192007	4.230	ng/u1	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021240.D
Acq On : 30 Jul 2024 18:31
Operator : MA/JU
Sample : P3359-14
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
E1G78

Quant Time: Jul 30 23:25:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

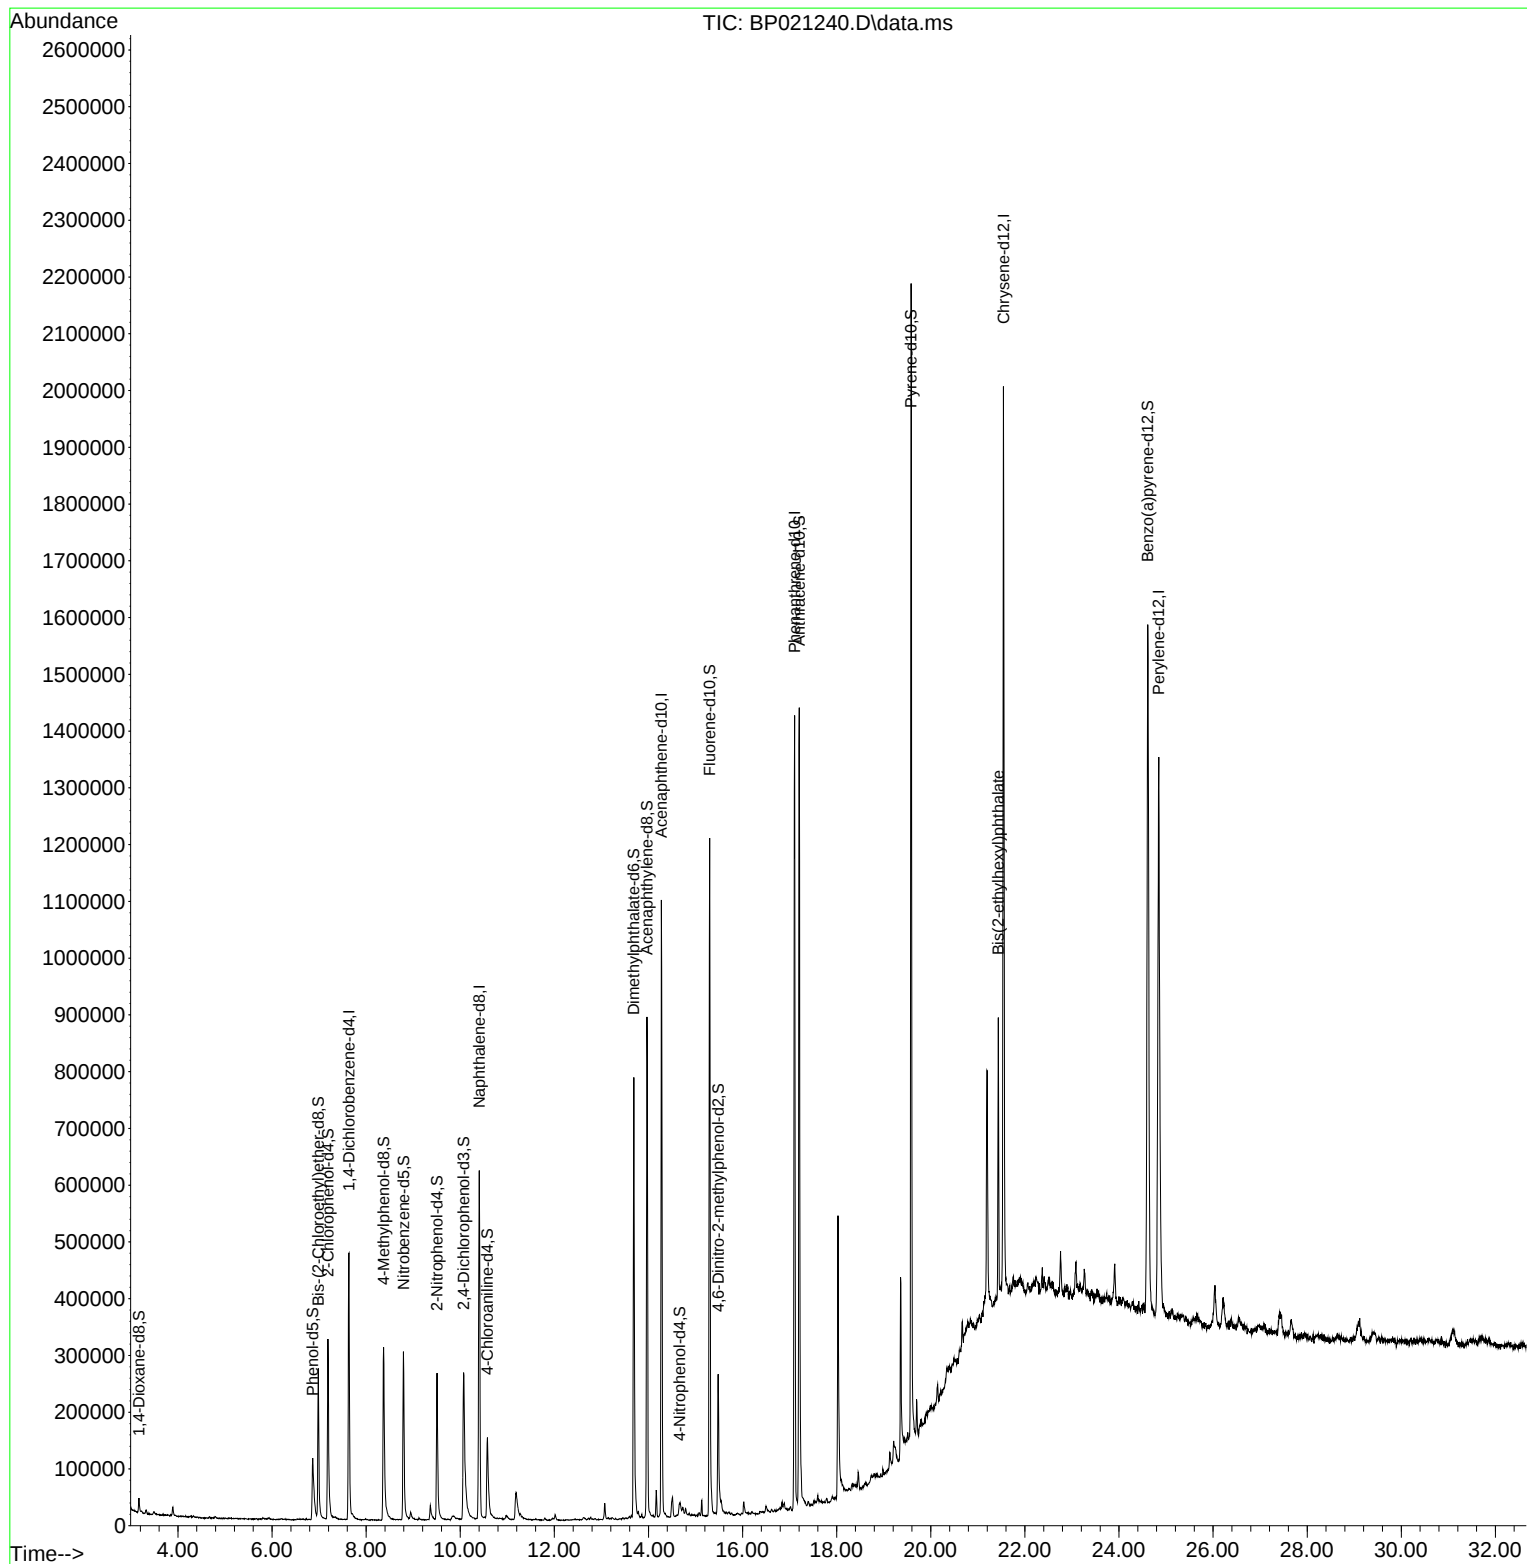

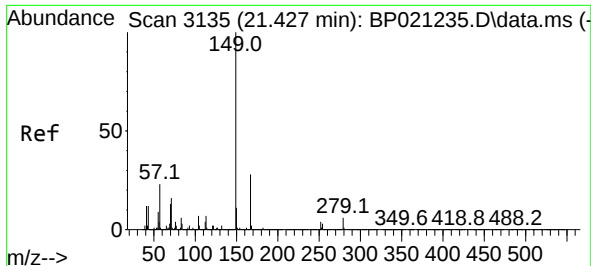

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.230 ng/ul
 RT: 21.433 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BP021240.D
 Acq: 30 Jul 2024 18:31

Instrument :
 BNA_P
 ClientSampleId :
 E1G78

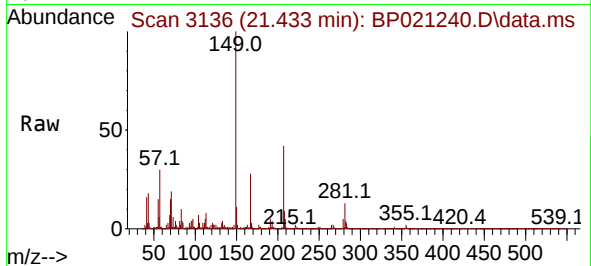

Tgt Ion:149 Resp: 19200
 Ion Ratio Lower Upper
 149 100
 167 27.6 22.1 33.1
 279 5.0 3.7 5.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/31/2024
 Supervised By :mohammad ahmed 09/04/2024

