

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021269.D
 Acq On : 31 Jul 2024 20:47
 Operator : CG/JU
 Sample : P3347-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX4

Quant Time: Aug 01 01:24:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	212014	20.000	ng/u1	0.00
20) Naphthalene-d8	10.398	136	861664	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.263	164	565152	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.092	188	1174546	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	884622	20.000	ng/u1	# 0.00
88) Perylene-d12	24.851	264	1123158	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	15995	3.433	ng/uL	-0.01
4) Pyridine-d5	3.593	84	104343	7.736	ng/u1	0.00
7) Phenol-d5	6.857	99	186961	10.816	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	6.981	67	256097	24.448	ng/u1	0.00
11) 2-Chlorophenol-d4	7.181	132	410827	28.848	ng/u1	0.00
15) 4-Methylphenol-d8	8.363	113	331846	23.116	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	199626	29.828	ng/u1	0.00
24) 2-Nitrophenol-d4	9.498	143	240546	31.402	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.051	165	436603	31.521	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	334614	18.235	ng/u1	0.00
46) Dimethylphthalate-d6	13.681	166	1378886	33.563	ng/u1	0.00
49) Acenaphthylene-d8	13.957	160	1511252	32.760	ng/u1	0.00
54) 4-Nitrophenol-d4	14.598	143	45827	7.840	ng/u1	0.01
60) Fluorene-d10	15.286	176	1160416	34.429	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	423365	59.573	ng/u1	0.00
73) Anthracene-d10	17.192	188	1740197	33.358	ng/u1	0.00
81) Pyrene-d10	19.574	212	1820835	33.293	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.615	264	1931771	34.873	ng/u1	0.02
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	14.945	232	22773	2.167	ng/u1	95
71) Pentachlorophenol	16.745	266	1012240	118.068	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021269.D
Acq On : 31 Jul 2024 20:47
Operator : CG/JU
Sample : P3347-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX4

Quant Time: Aug 01 01:24:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration




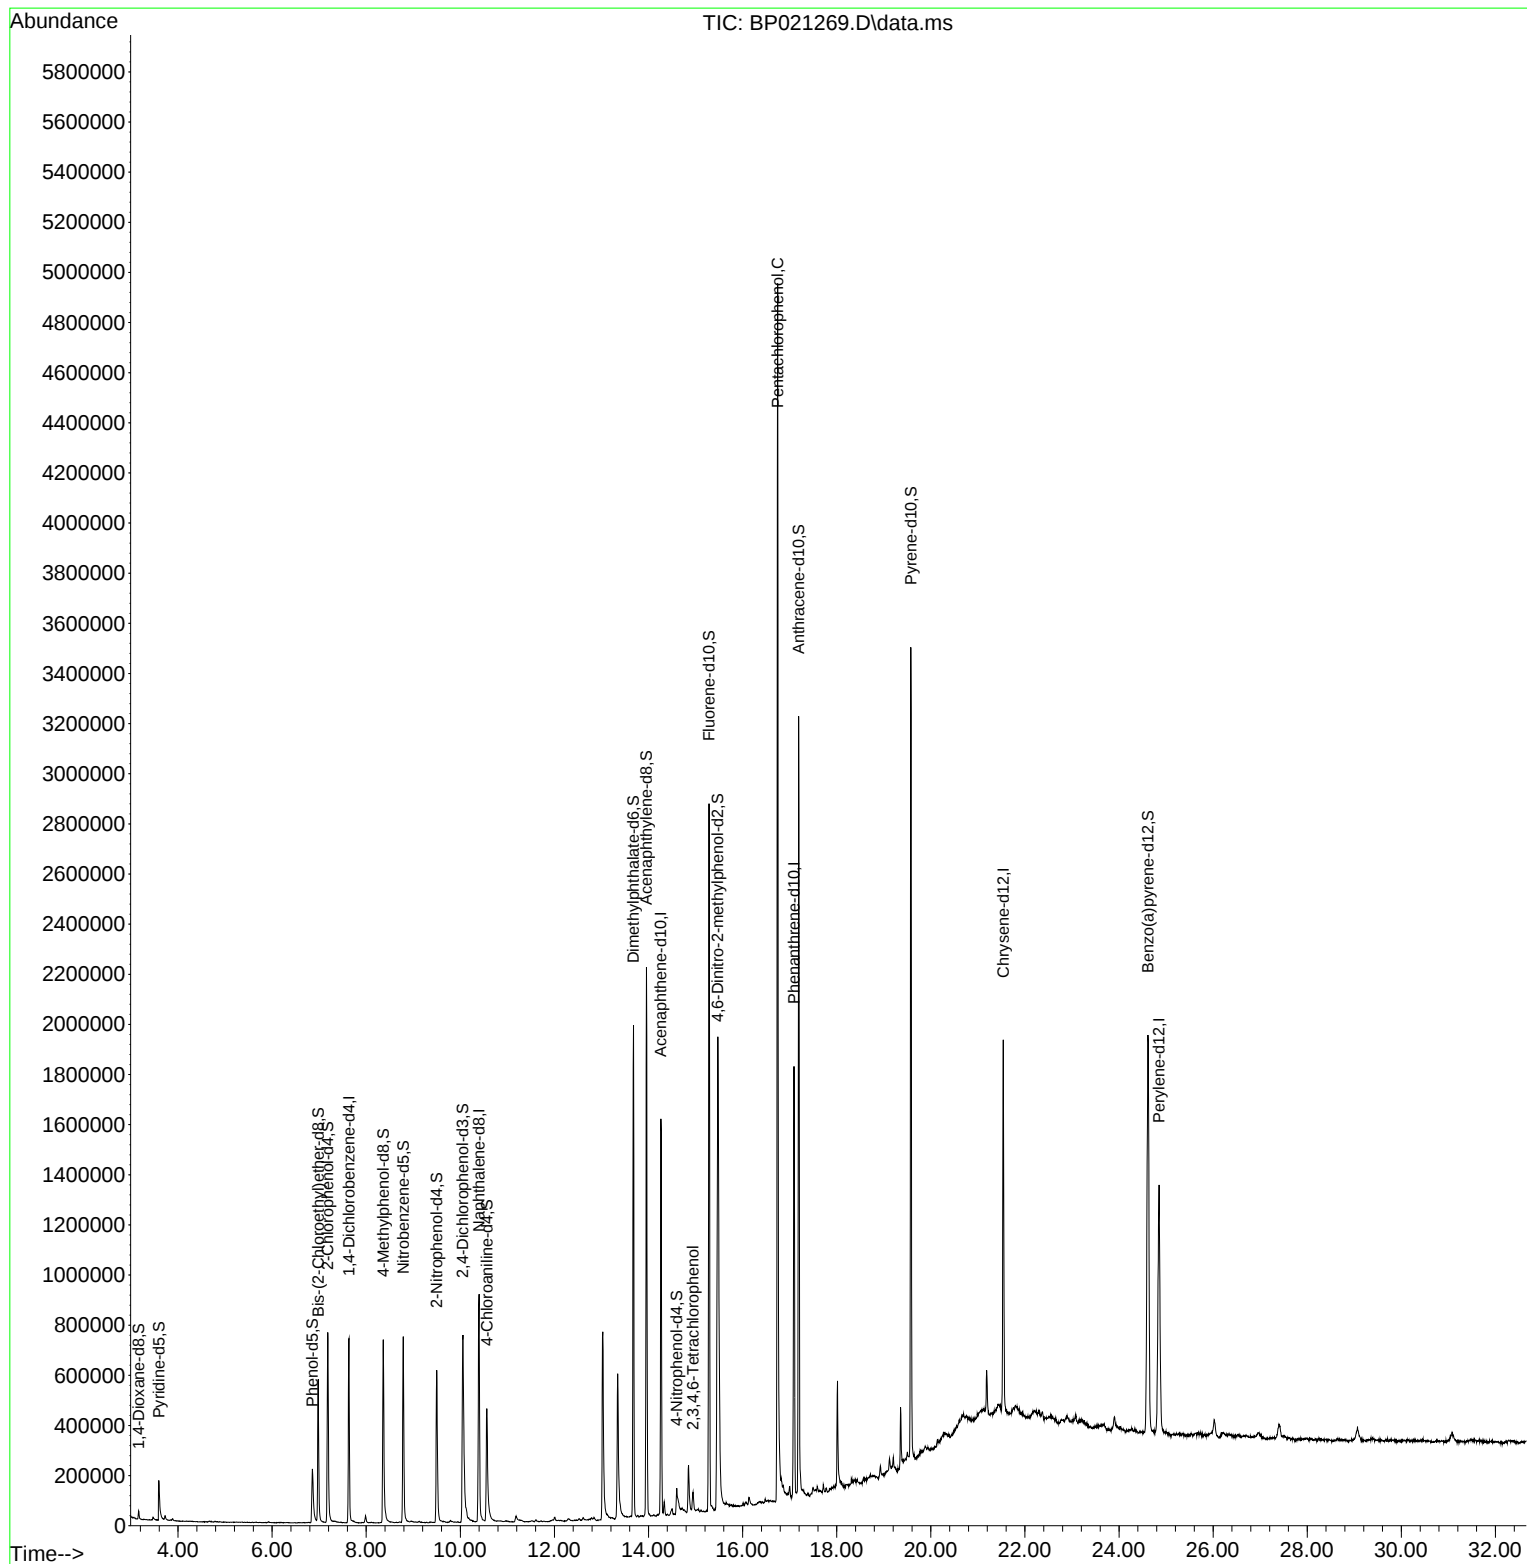


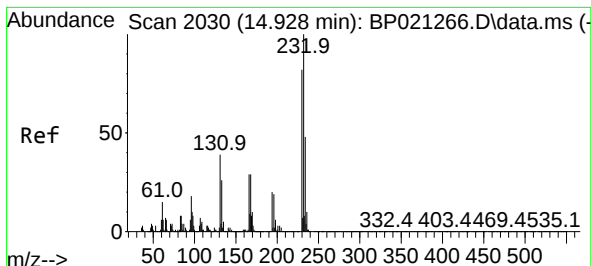

#58
2,3,4,6-Tetrachlorophenol
Concen: 2.167 ng/ul
RT: 14.945 min Scan# 2030
Delta R.T. 0.012 min
Lab File: BP021269.D
Acq: 31 Jul 2024 20:47

Instrument :
BNA_P
ClientSampleId :
C0AX4

Tgt Ion:	232	Resp:	22773
Ion	Ratio	Lower	Upper
232	100		
131	39.6	34.4	51.6
130	2.9	2.0	3.0
166	27.7	24.4	36.6

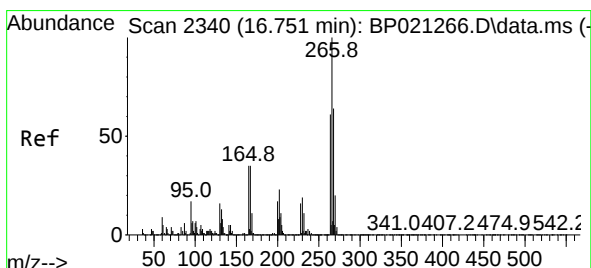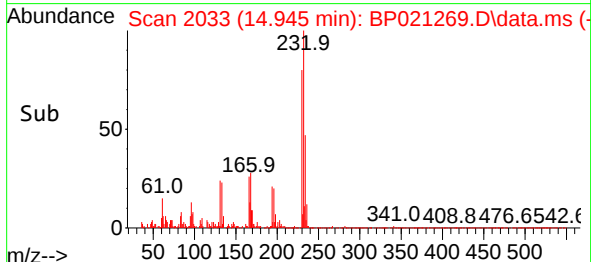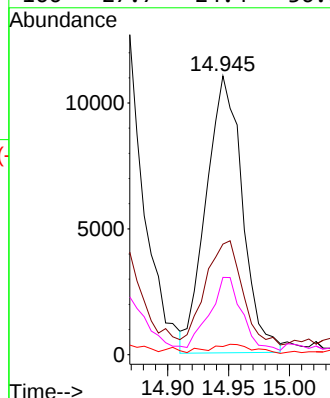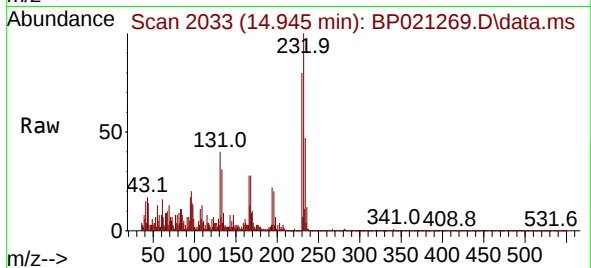

#71
Pentachlorophenol
Concen: 118.068 ng/ul
RT: 16.745 min Scan# 2339
Delta R.T. -0.006 min
Lab File: BP021269.D
Acq: 31 Jul 2024 20:47

Tgt Ion:	266	Resp:	1012240
Ion	Ratio	Lower	Upper
266	100		
264	63.6	52.3	78.5
268	65.0	52.3	78.5

