

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021224.D
 Acq On : 30 Jul 2024 01:51
 Operator : MA/JU
 Sample : P3280-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	28	rBV2	11698	15213	0.28%	0.032%
2	3.170	28	31	35	rVV	37876	42544	0.78%	0.089%
3	3.605	103	105	118	rBV	122324	243019	4.46%	0.509%
4	3.893	150	154	162	rVB	28135	42876	0.79%	0.090%
5	4.299	220	223	228	rVB	8117	12625	0.23%	0.026%
6	4.411	236	242	247	rBV	28444	46507	0.85%	0.098%
7	4.675	285	287	293	rVB6	4339	6091	0.11%	0.013%
8	4.793	304	307	312	rBV	11716	17305	0.32%	0.036%
9	5.005	339	343	350	rVB2	10315	16008	0.29%	0.034%
10	6.740	635	638	643	rVB6	5773	7504	0.14%	0.016%
11	6.869	653	660	674	rBV	139655	351902	6.46%	0.738%
12	6.987	674	680	698	rVB	566067	989676	18.17%	2.075%
13	7.193	708	715	733	rBV	631633	1210903	22.23%	2.539%
14	7.640	784	791	805	rBV	733613	1237207	22.72%	2.594%
15	7.987	844	850	861	rBV5	13602	34328	0.63%	0.072%
16	8.369	908	915	933	rBV	496062	1014968	18.64%	2.128%
17	8.793	981	987	1006	rBV	670832	1219399	22.39%	2.557%
18	9.128	1041	1044	1049	rVB4	4730	7309	0.13%	0.015%
19	9.505	1100	1108	1127	rBV	510157	1049419	19.27%	2.200%
20	10.057	1193	1202	1229	rBV	596711	1586755	29.13%	3.327%
21	10.393	1250	1259	1273	rBV	883705	1683781	30.92%	3.530%
22	10.563	1280	1288	1314	rBV	511479	1280877	23.52%	2.685%
23	11.063	1371	1373	1381	rVB9	2554	5641	0.10%	0.012%
24	12.022	1532	1536	1545	rVB4	8972	20632	0.38%	0.043%
25	13.228	1736	1741	1747	rBV8	3319	7756	0.14%	0.016%
26	13.675	1811	1817	1836	rBV	1630530	2417645	44.39%	5.069%
27	13.963	1858	1866	1887	rBV	1779999	2794472	51.31%	5.859%
28	14.269	1911	1918	1930	rBV	1449618	2222261	40.80%	4.659%
29	14.628	1974	1979	1984	rBV2	52901	122178	2.24%	0.256%
30	14.769	1999	2003	2011	rVB5	18168	34534	0.63%	0.072%
31	15.287	2083	2091	2104	rBV	2390993	3544215	65.07%	7.431%
32	15.463	2114	2121	2150	rVB	458122	1168572	21.46%	2.450%
33	17.092	2391	2398	2409	rBV	1464412	2344367	43.04%	4.915%
34	17.192	2409	2415	2428	rBV	2401298	3441713	63.19%	7.216%
35	17.775	2511	2514	2518	rBV5	7834	11736	0.22%	0.025%
36	18.016	2551	2555	2565	rBV2	55634	100832	1.85%	0.211%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021224.D
Acq On : 30 Jul 2024 01:51
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	19.122	2740	2743	2748	rVB2	36409	44047	0.81%	0.092%
38	19.204	2753	2757	2762	rBV	32527	47264	0.87%	0.099%
39	19.351	2779	2782	2789	rBV3	68700	115946	2.13%	0.243%
40	19.575	2814	2820	2832	rBV2	3462223	5049940	92.72%	10.587%
41	21.527	3147	3152	3165	rVB	1846009	3095856	56.84%	6.491%
42	24.598	3664	3674	3694	rVB	2018039	5446420	100.00%	11.419%
43	24.821	3704	3712	3730	rVB	1155210	3545580	65.10%	7.433%




Sum of corrected areas: 47697823

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021224.D
Acq On : 30 Jul 2024 01:51
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

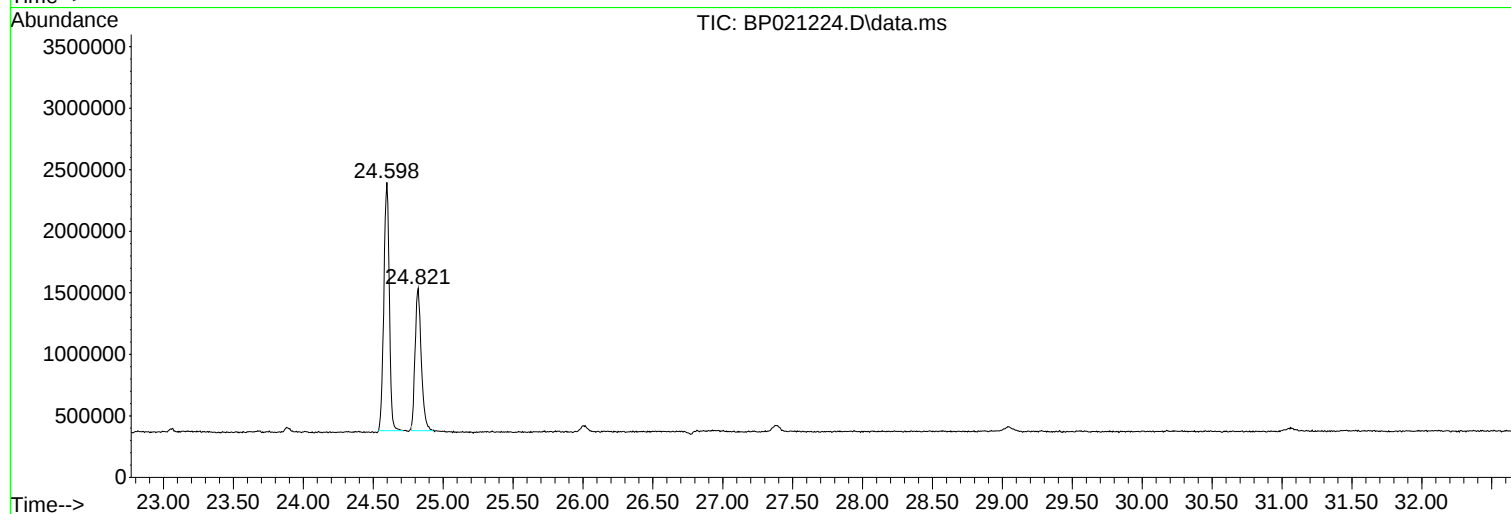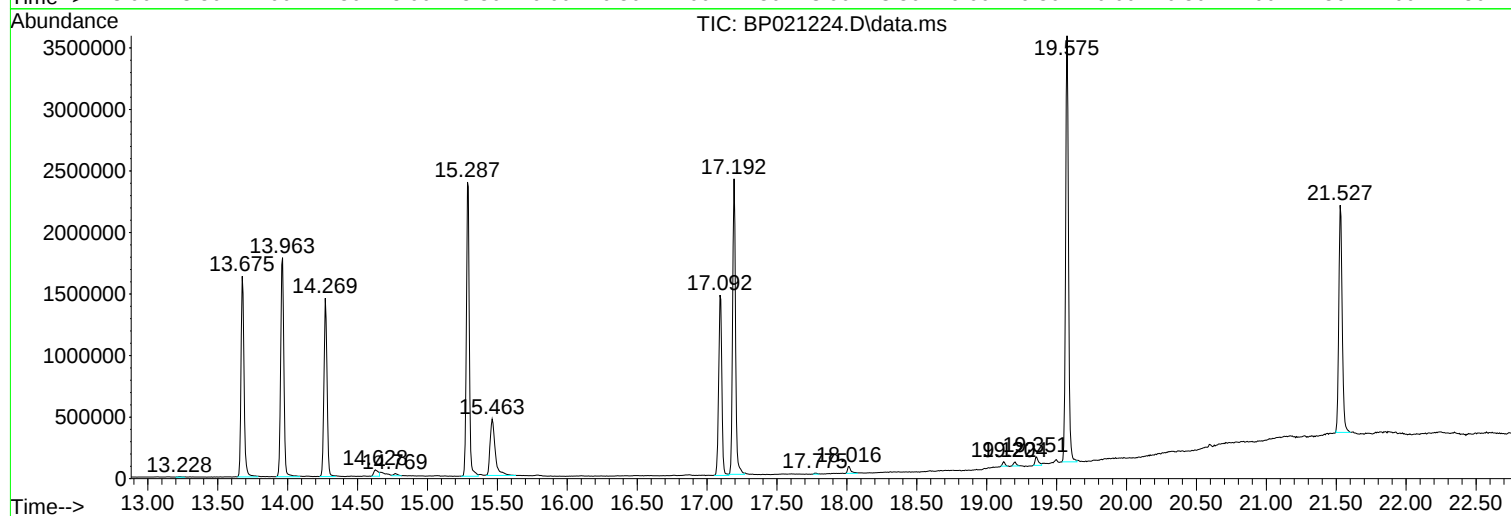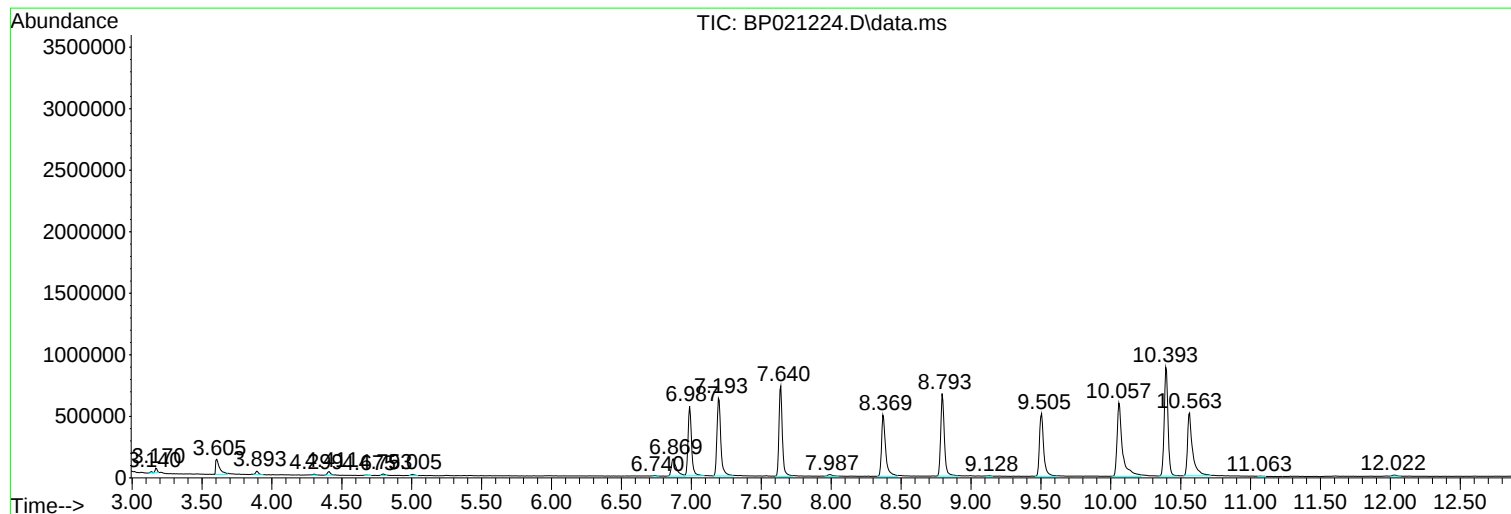

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021224.D
Acq On : 30 Jul 2024 01:51
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021224.D
Acq On : 30 Jul 2024 01:51
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc