

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021229.D
 Acq On : 30 Jul 2024 05:28
 Operator : MA/JU
 Sample : P3336-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	17	rBV5	4842	7252	0.10%	0.013%
2	3.175	28	32	36	rBV	39454	51089	0.74%	0.090%
3	3.599	102	104	116	rBV	118890	206912	2.98%	0.363%
4	3.887	150	153	159	rVB	11398	16058	0.23%	0.028%
5	3.999	169	172	182	rVB4	5590	10167	0.15%	0.018%
6	4.093	183	188	195	rVB2	12944	24823	0.36%	0.044%
7	4.258	210	216	224	rBV2	15629	27000	0.39%	0.047%
8	4.793	303	307	314	rVB2	5269	9542	0.14%	0.017%
9	5.228	377	381	385	rBV2	8367	14830	0.21%	0.026%
10	5.522	427	431	441	rVV	24476	46776	0.67%	0.082%
11	5.728	461	466	471	rBV9	4248	7526	0.11%	0.013%
12	6.858	648	658	673	rVV	150918	365816	5.27%	0.642%
13	6.987	673	680	695	rVV	569612	979136	14.11%	1.719%
14	7.099	695	699	705	rVV8	4895	11583	0.17%	0.020%
15	7.181	706	713	733	rVV	644611	1245867	17.95%	2.188%
16	7.334	736	739	747	rVB9	4882	11330	0.16%	0.020%
17	7.640	783	791	799	rBV	798843	1339111	19.29%	2.351%
18	7.705	799	802	821	rVB4	15920	51866	0.75%	0.091%
19	8.369	906	915	932	rBV	450966	1014865	14.62%	1.782%
20	8.481	932	934	940	rVB5	6790	9599	0.14%	0.017%
21	8.728	970	976	980	rBV	20894	43373	0.62%	0.076%
22	8.793	980	987	998	rBV	630683	1218926	17.56%	2.140%
23	8.934	1008	1011	1017	rVB7	7641	11970	0.17%	0.021%
24	9.505	1101	1108	1123	rBV	558512	1108178	15.97%	1.946%
25	9.834	1158	1164	1168	rBV8	3401	8405	0.12%	0.015%
26	10.052	1193	1201	1225	rBV	699090	1667401	24.02%	2.928%
27	10.334	1243	1249	1252	rBV	25385	43932	0.63%	0.077%
28	10.393	1252	1259	1267	rVV	1228629	1847685	26.62%	3.244%
29	10.563	1279	1288	1309	rBV	392860	1046629	15.08%	1.838%
30	11.181	1386	1393	1399	rBV3	16025	27723	0.40%	0.049%
31	11.246	1400	1404	1411	rVV7	5668	11564	0.17%	0.020%
32	11.657	1468	1474	1481	rBV	28610	49130	0.71%	0.086%
33	11.781	1489	1495	1515	rVB3	28379	85597	1.23%	0.150%
34	12.004	1526	1533	1542	rBV3	9005	25828	0.37%	0.045%
35	12.240	1567	1573	1583	rBV	24300	44170	0.64%	0.078%
36	12.593	1628	1633	1638	rBV7	3499	7258	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021229.D
 Acq On : 30 Jul 2024 05:28
 Operator : MA/JU
 Sample : P3336-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	13.116	1717	1722	1728	rBV4	5992	11474	0.17%	0.020%
38	13.687	1811	1819	1832	rBV	1624908	2616377	37.69%	4.594%
39	13.810	1837	1840	1846	rVB7	5570	8002	0.12%	0.014%
40	13.957	1858	1865	1882	rBV	1880281	3052258	43.97%	5.359%
41	14.269	1908	1918	1937	rBV	1621193	2631058	37.91%	4.620%
42	14.610	1969	1976	1987	rBV4	54686	213351	3.07%	0.375%
43	14.957	2032	2035	2038	rVB4	6809	8188	0.12%	0.014%
44	15.045	2046	2050	2057	rBV	91282	131953	1.90%	0.232%
45	15.104	2057	2060	2068	rVB5	20765	36572	0.53%	0.064%
46	15.287	2084	2091	2112	rVV	2264841	3975902	57.28%	6.981%
47	15.457	2114	2120	2146	rBV	830132	1475003	21.25%	2.590%
48	15.922	2194	2199	2204	rVV4	17451	26151	0.38%	0.046%
49	15.998	2208	2212	2217	rVV4	15431	19958	0.29%	0.035%
50	16.051	2217	2221	2225	rBV7	7943	12101	0.17%	0.021%
51	16.504	2293	2298	2304	rBV10	6133	14345	0.21%	0.025%
52	16.628	2313	2319	2322	rBV8	7810	12557	0.18%	0.022%
53	16.669	2323	2326	2330	rVB	11580	12122	0.17%	0.021%
54	16.881	2358	2362	2368	rVB5	5998	10547	0.15%	0.019%
55	17.087	2390	2397	2407	rBV	2267209	3161123	45.54%	5.550%
56	17.192	2407	2415	2429	rBV2	2790154	4836301	69.68%	8.492%
57	17.387	2445	2448	2458	rVB5	7217	15664	0.23%	0.028%
58	17.692	2493	2500	2507	rBV6	20455	40134	0.58%	0.070%
59	17.775	2510	2514	2518	rBV6	14044	20159	0.29%	0.035%
60	18.028	2552	2557	2563	rBV	98363	156242	2.25%	0.274%
61	18.275	2595	2599	2602	rVB5	12547	16121	0.23%	0.028%
62	18.316	2602	2606	2612	rVB7	17762	26705	0.38%	0.047%
63	18.451	2627	2629	2634	rBV5	8791	9988	0.14%	0.018%
64	18.545	2641	2645	2646	rBV2	30491	35238	0.51%	0.062%
65	18.904	2702	2706	2711	rBV4	20594	33346	0.48%	0.059%
66	19.122	2738	2743	2747	rBV	44771	67798	0.98%	0.119%
67	19.204	2753	2757	2764	rBV	43680	67033	0.97%	0.118%
68	19.351	2778	2782	2791	rBV5	64603	118669	1.71%	0.208%
69	19.498	2805	2807	2812	rBV4	13625	14139	0.20%	0.025%
70	19.581	2815	2821	2834	rVV	4173803	6106655	87.98%	10.722%
71	20.139	2914	2916	2921	rVB3	36301	37550	0.54%	0.066%
72	20.651	3001	3003	3008	rVB2	46667	44817	0.65%	0.079%
73	21.533	3147	3153	3171	rBV2	2013285	3783385	54.51%	6.643%
74	24.598	3663	3674	3693	rBV	2457264	6940976	100.00%	12.187%
75	24.833	3703	3714	3731	rVB	1303826	4454176	64.17%	7.821%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 56953055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

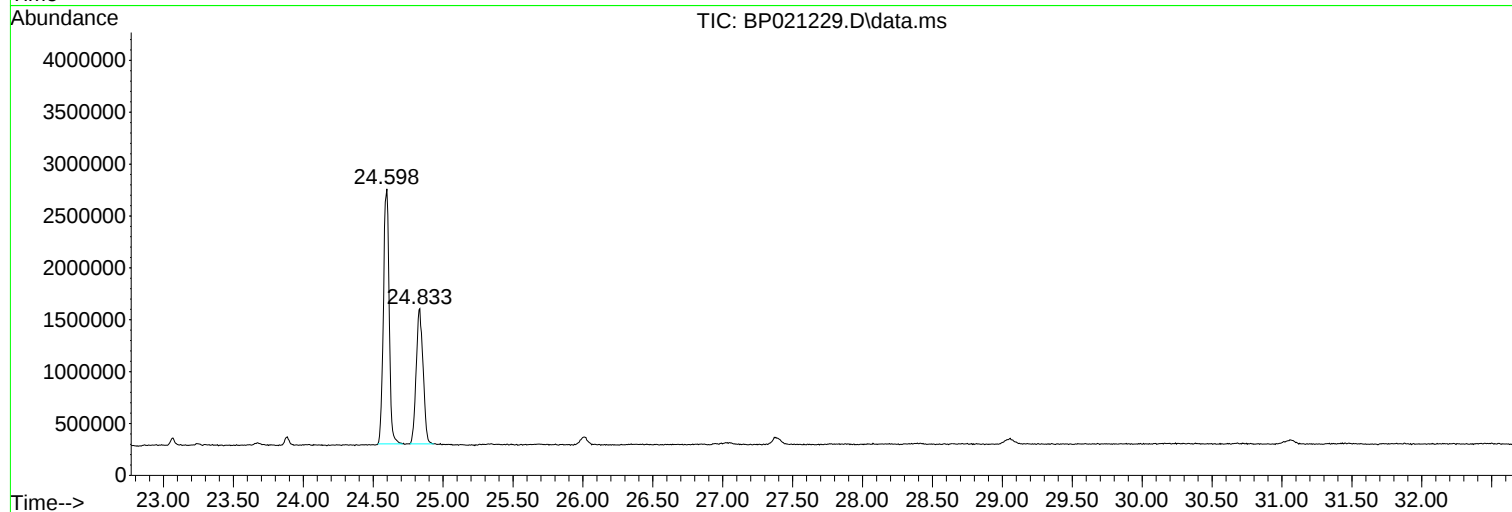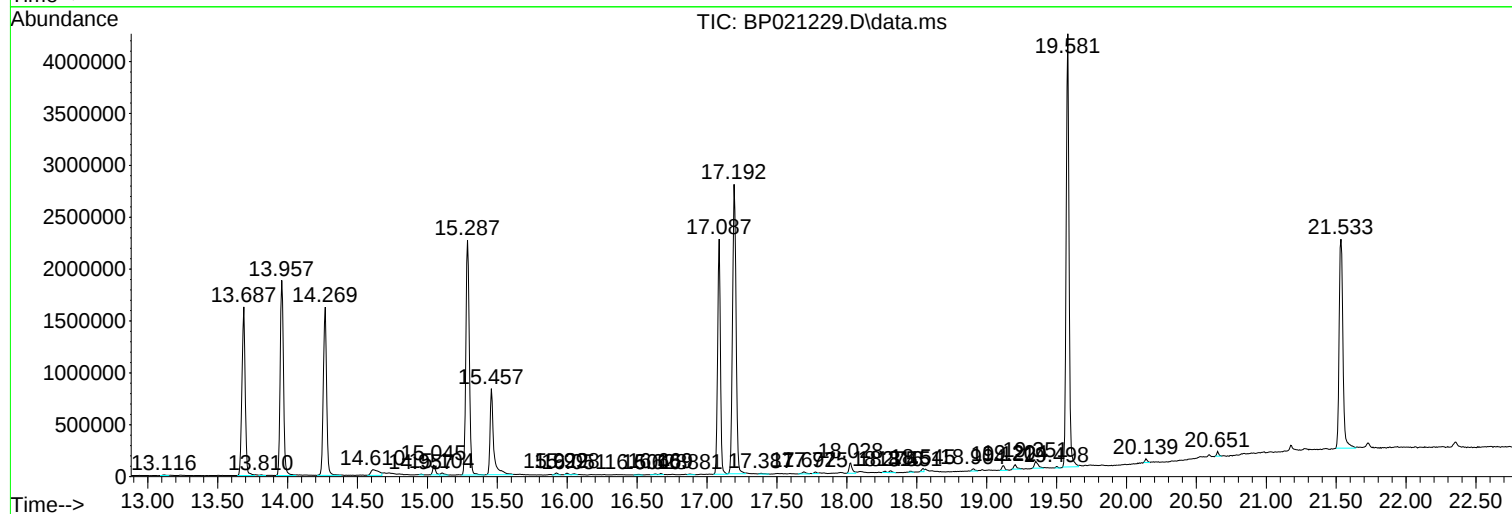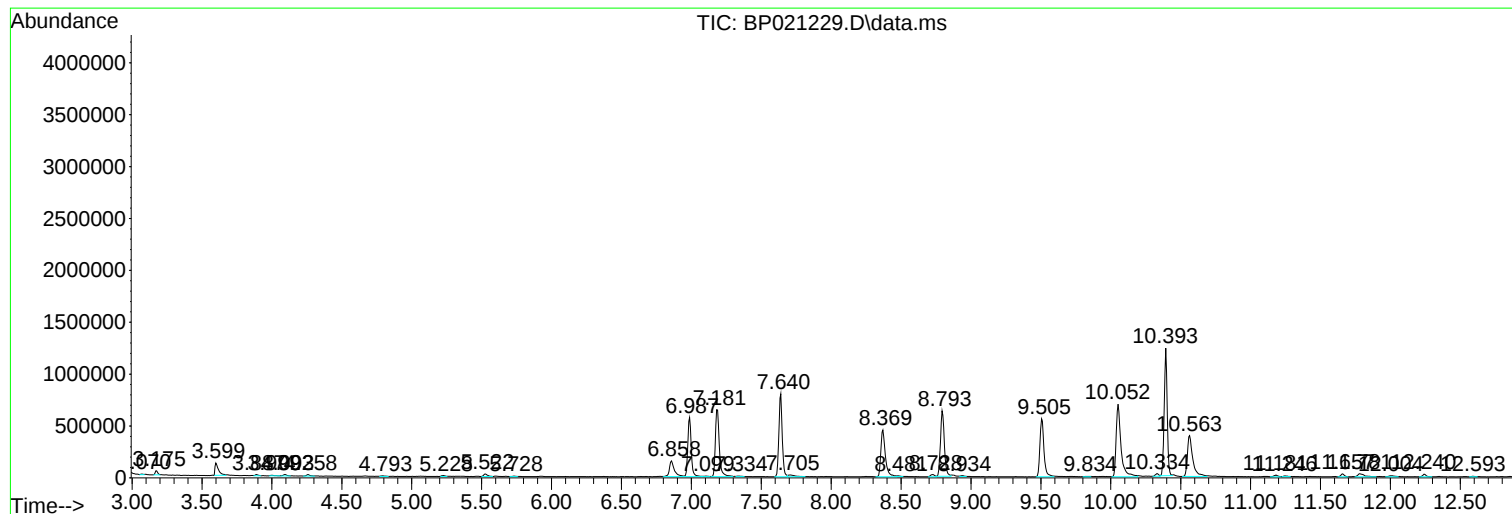

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc