

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021231.D
 Acq On : 30 Jul 2024 11:58
 Operator : MA/JU
 Sample : PB162326BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	37	rVB	40792	54757	1.39%	0.129%
2	3.581	98	101	123	rBV	432835	795054	20.12%	1.872%
3	3.881	148	152	158	rVB	10621	17240	0.44%	0.041%
4	4.316	222	226	233	rVB4	4480	9862	0.25%	0.023%
5	6.840	649	655	671	rBV	463057	994294	25.16%	2.341%
6	6.969	671	677	688	rVB	465884	763795	19.33%	1.798%
7	7.175	703	712	724	rBV	598239	1060098	26.83%	2.496%
8	7.622	778	788	807	rBV	655019	1049889	26.57%	2.472%
9	8.352	905	912	932	rBV	639921	1281126	32.42%	3.016%
10	8.775	975	984	1005	rBV	526964	1000861	25.33%	2.356%
11	9.493	1099	1106	1124	rBV	461166	884436	22.38%	2.082%
12	10.051	1192	1201	1226	rBV	595260	1336345	33.82%	3.146%
13	10.393	1250	1259	1272	rBV	816145	1424798	36.05%	3.355%
14	10.551	1278	1286	1312	rBV	576576	1287141	32.57%	3.030%
15	12.010	1529	1534	1543	rBV4	7819	19687	0.50%	0.046%
16	13.675	1809	1817	1837	rBV	1299284	2076597	52.55%	4.889%
17	13.957	1858	1865	1881	rBV	1498291	2353960	59.57%	5.542%
18	14.263	1909	1917	1932	rBV	1278986	1956546	49.51%	4.607%
19	14.581	1965	1971	1988	rBV	226922	689362	17.44%	1.623%
20	14.828	2009	2013	2016	rBV6	3332	4800	0.12%	0.011%
21	15.063	2049	2053	2058	rBV7	3341	8010	0.20%	0.019%
22	15.122	2059	2063	2065	rBV5	2595	4050	0.10%	0.010%
23	15.210	2073	2078	2080	rBV3	6501	9340	0.24%	0.022%
24	15.234	2080	2082	2084	rVV2	4186	4886	0.12%	0.012%
25	15.287	2084	2091	2105	rVB	2087905	2995463	75.80%	7.053%
26	15.457	2114	2120	2129	rBV	433469	837350	21.19%	1.971%
27	16.092	2222	2228	2232	rBV8	7177	13073	0.33%	0.031%
28	16.681	2322	2328	2329	rBV5	5679	8757	0.22%	0.021%
29	16.692	2329	2330	2335	rVB5	6927	6051	0.15%	0.014%
30	16.869	2358	2360	2367	rVB5	4394	7865	0.20%	0.019%
31	17.092	2392	2398	2405	rBV	1736177	2373842	60.07%	5.589%
32	17.192	2409	2415	2434	rVB	2001337	3286217	83.16%	7.737%
33	17.775	2510	2514	2515	rBV4	4510	4356	0.11%	0.010%
34	18.033	2552	2558	2566	rBV5	35298	90990	2.30%	0.214%
35	18.651	2656	2663	2666	rBV2	75902	180623	4.57%	0.425%
36	18.698	2666	2671	2676	rVB3	66086	158993	4.02%	0.374%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021231.D
Acq On : 30 Jul 2024 11:58
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	18.780	2682	2685	2700	rVB	69569	176916	4.48%	0.417%
38	19.127	2740	2744	2750	rVB3	31654	45301	1.15%	0.107%
39	19.210	2755	2758	2763	rVB	20310	30705	0.78%	0.072%
40	19.363	2781	2784	2788	rBV6	21719	37193	0.94%	0.088%
41	19.580	2815	2821	2833	rBV	2538802	3951842	100.00%	9.304%
42	21.545	3149	3155	3173	rVB2	1457887	2692161	68.12%	6.338%
43	24.621	3669	3678	3691	rBV2	1486143	3782724	95.72%	8.906%
44	24.857	3708	3718	3736	rVB	836824	2705811	68.47%	6.371%




Sum of corrected areas: 42473167

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021231.D
Acq On : 30 Jul 2024 11:58
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

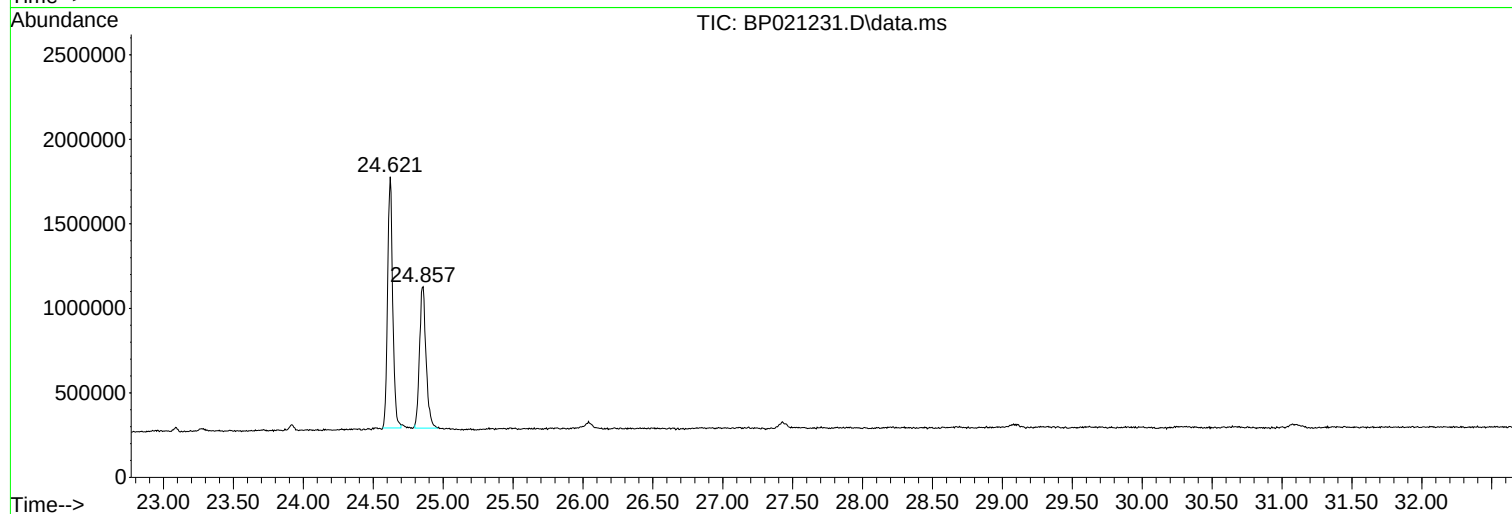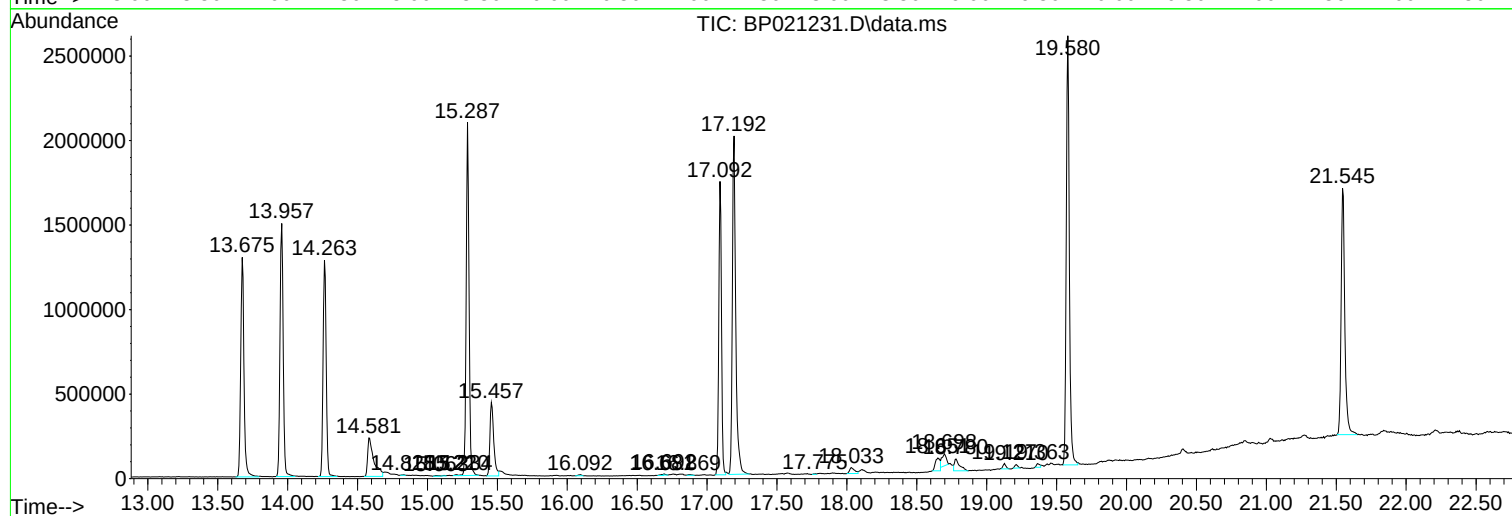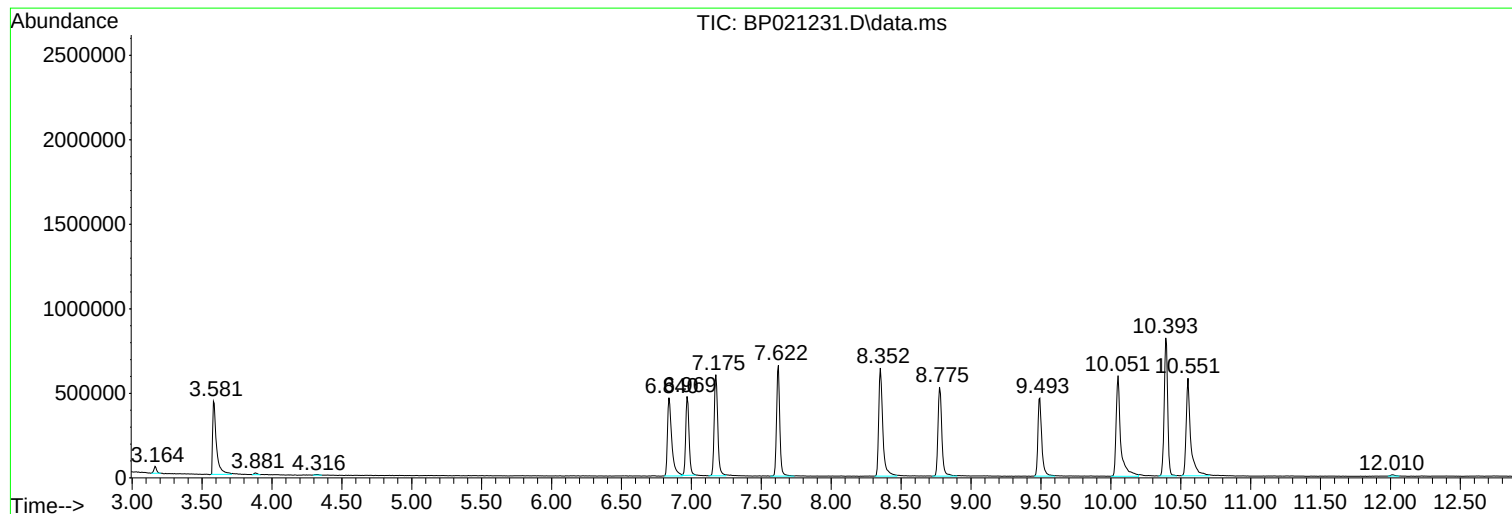

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021231.D
Acq On : 30 Jul 2024 11:58
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021231.D
Acq On : 30 Jul 2024 11:58
Operator : MA/JU
Sample : PB162326BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------