

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021233.D
 Acq On : 30 Jul 2024 13:25
 Operator : MA/JU
 Sample : P3373-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	38	rVB2	19881	29722	0.73%	0.084%
2	3.605	102	105	126	rBV	52764	133070	3.25%	0.377%
3	3.893	150	154	161	rVB2	7138	12201	0.30%	0.035%
4	4.258	213	216	222	rVB6	3193	4927	0.12%	0.014%
5	4.363	231	234	239	rVB5	4004	5623	0.14%	0.016%
6	4.669	282	286	291	rBV7	3149	5060	0.12%	0.014%
7	5.675	451	457	462	rBV9	2780	5974	0.15%	0.017%
8	6.869	654	660	673	rBV2	71600	188578	4.61%	0.534%
9	6.987	674	680	700	rVB	354322	630864	15.43%	1.785%
10	7.193	706	715	735	rBV	398274	777208	19.01%	2.199%
11	7.340	736	740	745	rVB7	3048	4863	0.12%	0.014%
12	7.634	779	790	801	rBV	476079	804414	19.68%	2.276%
13	8.375	909	916	931	rBV	295005	612831	14.99%	1.734%
14	8.793	978	987	1006	rBV	448867	814677	19.93%	2.305%
15	8.946	1008	1013	1018	rVB9	5770	12534	0.31%	0.035%
16	9.363	1079	1084	1090	rBV6	6135	12860	0.31%	0.036%
17	9.504	1101	1108	1122	rBV	375322	710165	17.37%	2.010%
18	9.828	1156	1163	1164	rBV7	7370	13286	0.32%	0.038%
19	10.063	1195	1203	1221	rBV	401623	1038091	25.39%	2.938%
20	10.398	1251	1260	1272	rBV	604350	1124266	27.50%	3.181%
21	10.569	1282	1289	1314	rBV	320618	779471	19.07%	2.206%
22	11.204	1388	1397	1399	rBV6	8846	18095	0.44%	0.051%
23	11.251	1400	1405	1416	rVB4	19155	52897	1.29%	0.150%
24	12.022	1530	1536	1541	rBV2	8271	16524	0.40%	0.047%
25	13.122	1717	1723	1732	rBV	61633	110571	2.70%	0.313%
26	13.686	1812	1819	1839	rBV	1113274	1711535	41.87%	4.843%
27	13.963	1859	1866	1884	rVV2	1132509	1985381	48.56%	5.618%
28	14.275	1910	1919	1938	rBV	992108	1593289	38.97%	4.509%
29	14.645	1977	1982	1986	rBV3	26136	58128	1.42%	0.164%
30	14.728	1994	1996	2002	rVB5	9608	13609	0.33%	0.039%
31	15.069	2049	2054	2061	rVB9	4395	8447	0.21%	0.024%
32	15.128	2061	2064	2069	rVB6	4679	4457	0.11%	0.013%
33	15.298	2085	2093	2106	rBV	1629955	2579267	63.09%	7.299%
34	15.475	2116	2123	2140	rBV	360101	808212	19.77%	2.287%
35	15.916	2196	2198	2205	rVB4	3575	6265	0.15%	0.018%
36	16.022	2213	2216	2219	rBV5	3509	5128	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021233.D
 Acq On : 30 Jul 2024 13:25
 Operator : MA/JU
 Sample : P3373-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	16.104	2227	2230	2234	rVB6	3184	4294	0.11%	0.012%
38	16.516	2294	2300	2305	rBV10	5085	10452	0.26%	0.030%
39	16.886	2359	2363	2367	rVB5	4269	6831	0.17%	0.019%
40	17.098	2392	2399	2407	rBV	1309080	2018946	49.38%	5.713%
41	17.204	2410	2417	2434	rVV	2022166	3078228	75.30%	8.711%
42	18.027	2552	2557	2567	rBV	88466	175510	4.29%	0.497%
43	19.133	2741	2745	2752	rBV3	31505	45760	1.12%	0.129%
44	19.216	2755	2759	2762	rBV	29130	46538	1.14%	0.132%
45	19.363	2780	2784	2793	rBV	50302	81017	1.98%	0.229%
46	19.586	2816	2822	2838	rBV	2677654	4088195	100.00%	11.569%
47	21.551	3151	3156	3170	rVB	1700485	2556637	62.54%	7.235%
48	24.627	3669	3679	3693	rVB	1389901	3980088	97.36%	11.263%
49	24.856	3710	3718	3730	rVB	925940	2553103	62.45%	7.225%




Sum of corrected areas: 35338089

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021233.D
Acq On : 30 Jul 2024 13:25
Operator : MA/JU
Sample : P3373-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08K0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

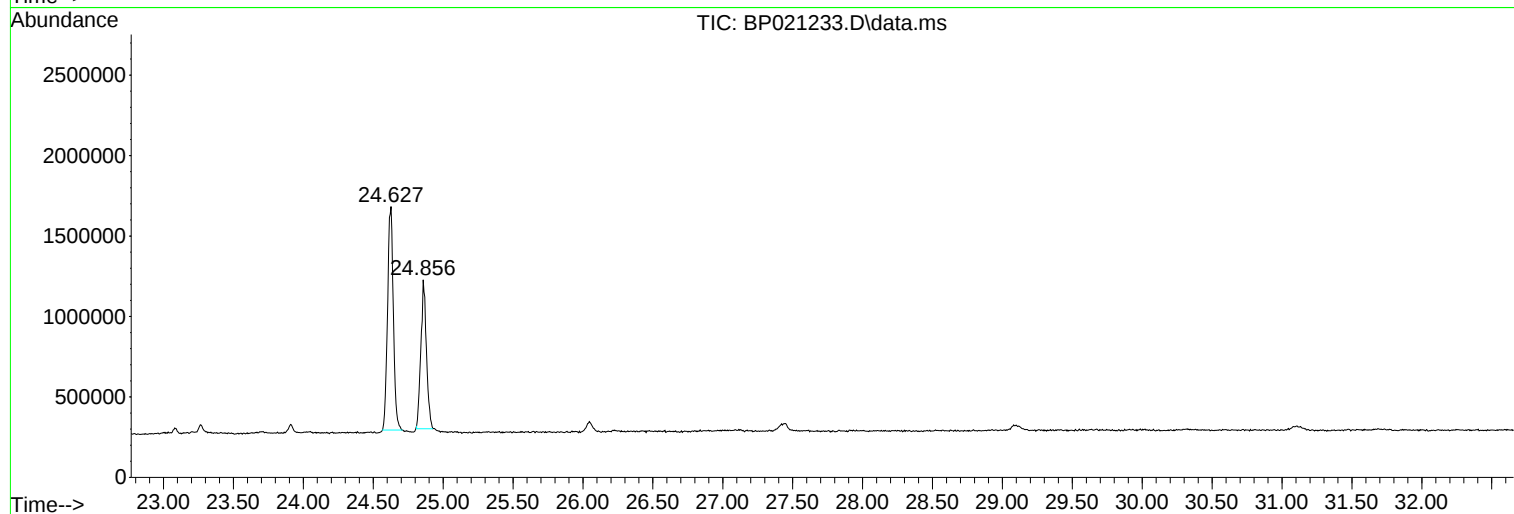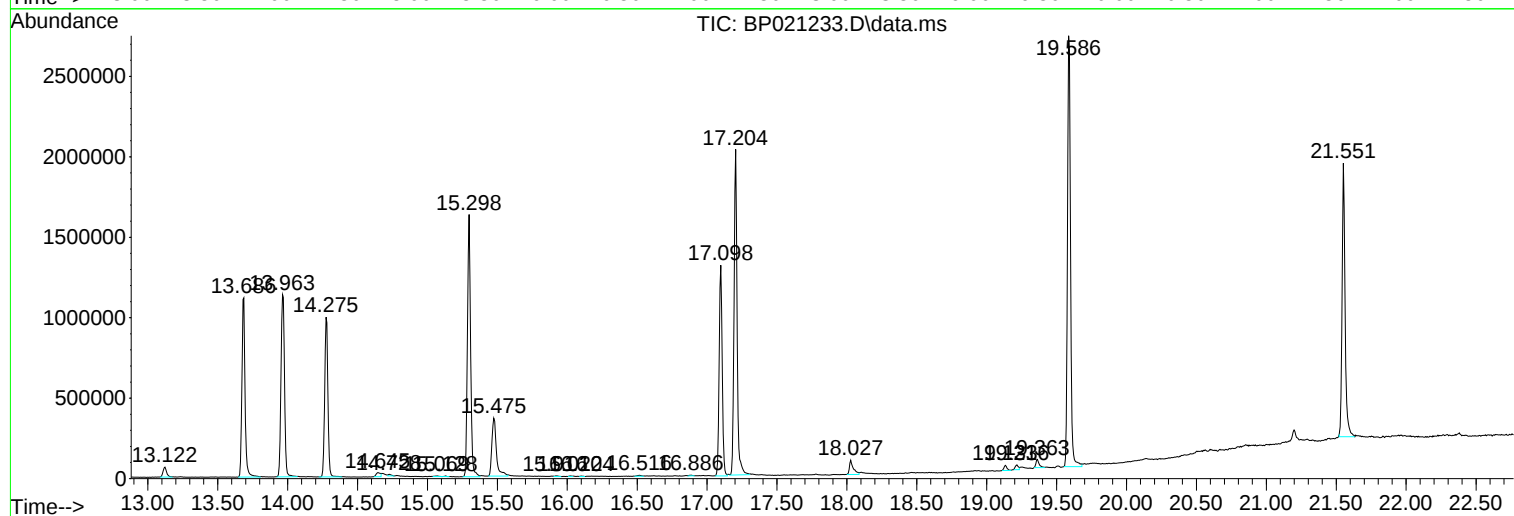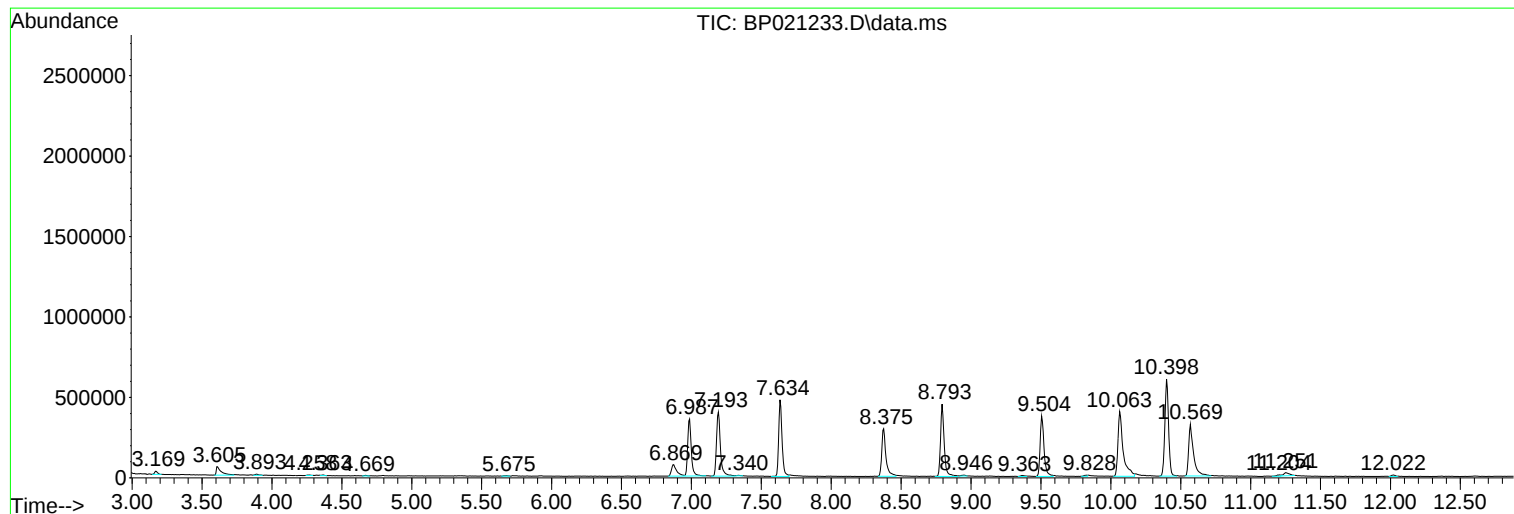

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021233.D
Acq On : 30 Jul 2024 13:25
Operator : MA/JU
Sample : P3373-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08K0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021233.D
Acq On : 30 Jul 2024 13:25
Operator : MA/JU
Sample : P3373-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08K0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc