

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021237.D
 Acq On : 30 Jul 2024 16:19
 Operator : MA/JU
 Sample : PB162343BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	27	31	37	rVB	27989	40833	1.13%	0.112%
2	3.593	100	103	125	rBV	294998	639157	17.75%	1.755%
3	3.887	149	153	161	rBV2	9109	16371	0.45%	0.045%
4	6.852	650	657	673	rBV	338969	796918	22.13%	2.188%
5	6.987	674	680	701	rVB	370795	636330	17.67%	1.747%
6	7.187	707	714	731	rBV	477602	856145	23.77%	2.351%
7	7.634	783	790	803	rBV	539150	923313	25.64%	2.535%
8	8.369	907	915	933	rBV	471682	1034131	28.71%	2.839%
9	8.793	977	987	1006	rBV	428114	805910	22.38%	2.213%
10	9.505	1100	1108	1123	rBV	316210	690912	19.18%	1.897%
11	10.057	1194	1202	1222	rBV	362765	1005415	27.92%	2.760%
12	10.393	1251	1259	1276	rVB	725740	1281241	35.58%	3.518%
13	10.563	1280	1288	1311	rBV	367491	1023060	28.41%	2.809%
14	12.046	1533	1540	1550	rBV4	5824	17510	0.49%	0.048%
15	13.687	1813	1819	1844	rBV	1177586	1679778	46.64%	4.612%
16	13.963	1859	1866	1881	rBV	1054215	1881360	52.24%	5.165%
17	14.269	1911	1918	1928	rBV	925050	1762547	48.94%	4.839%
18	14.598	1965	1974	1987	rBV	129031	463198	12.86%	1.272%
19	14.792	2004	2007	2012	rVB6	7060	13112	0.36%	0.036%
20	14.957	2032	2035	2041	rBV7	2037	3966	0.11%	0.011%
21	15.292	2084	2092	2109	rBV	1314216	2440180	67.75%	6.700%
22	15.469	2114	2122	2126	rBV	243321	473650	13.15%	1.300%
23	16.092	2225	2228	2233	rVB6	4065	5906	0.16%	0.016%
24	16.769	2340	2343	2348	rVB7	3605	5501	0.15%	0.015%
25	16.892	2358	2364	2369	rBV3	3952	7098	0.20%	0.019%
26	17.098	2392	2399	2409	rBV	1417067	2223774	61.75%	6.105%
27	17.204	2410	2417	2438	rVB2	1506436	2762112	76.69%	7.583%
28	17.792	2513	2517	2520	rBV5	14865	19352	0.54%	0.053%
29	19.145	2742	2747	2752	rBV3	23016	40441	1.12%	0.111%
30	19.222	2757	2760	2765	rVV	17514	27766	0.77%	0.076%
31	19.598	2817	2824	2837	rBV	2215762	3566593	99.03%	9.792%
32	21.551	3151	3156	3173	rBV2	1476013	2715725	75.41%	7.456%
33	24.627	3671	3679	3699	rVB	1424430	3601496	100.00%	9.888%
34	24.863	3711	3719	3737	rVB	896053	2961916	82.24%	8.132%

Sum of corrected areas: 36422717




Instrument :
BNA_P
ClientSampleId :
SBLK343

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021237.D
Acq On : 30 Jul 2024 16:19
Operator : MA/JU
Sample : PB162343BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

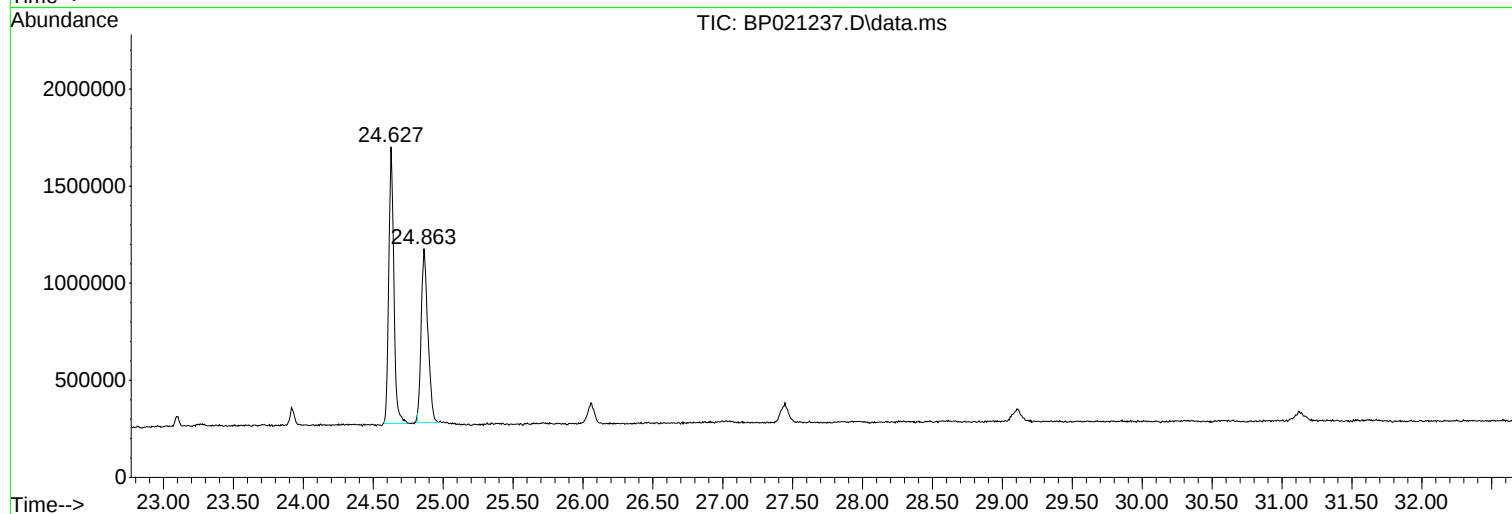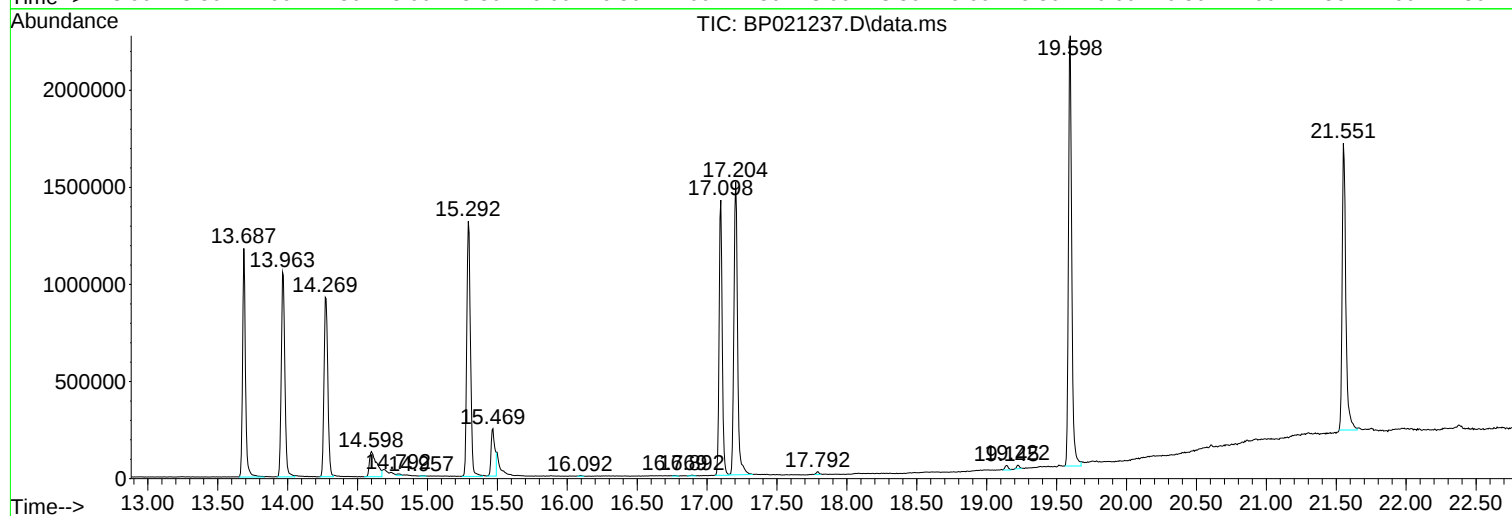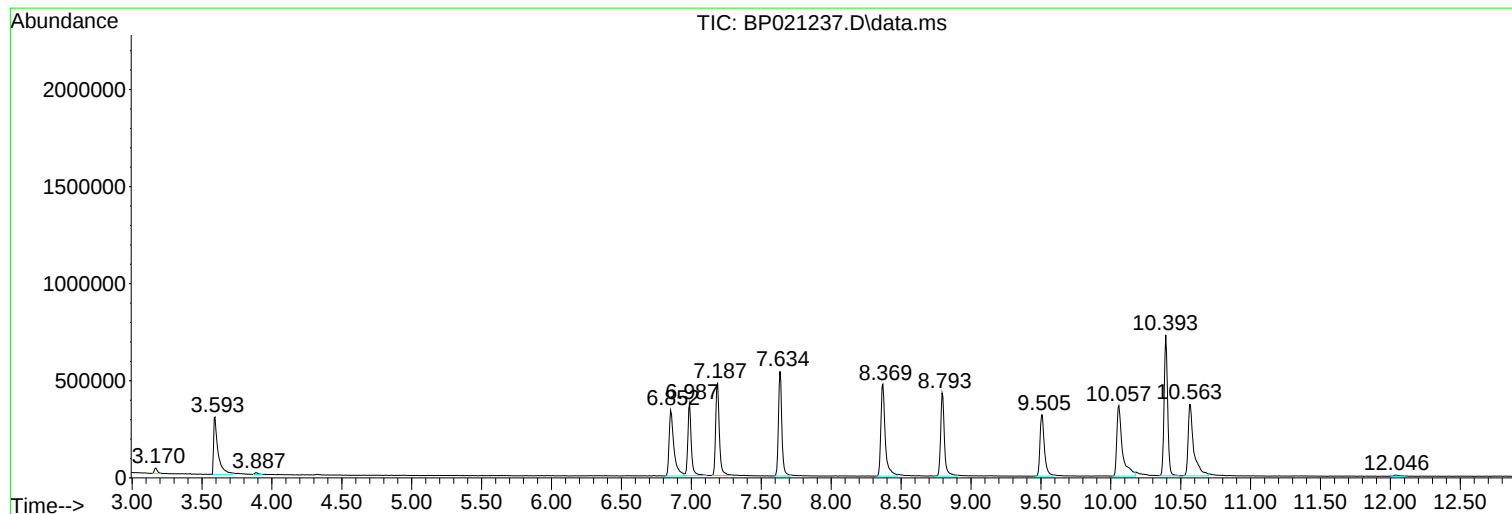

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021237.D
Acq On : 30 Jul 2024 16:19
Operator : MA/JU
Sample : PB162343BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021237.D
Acq On : 30 Jul 2024 16:19
Operator : MA/JU
Sample : PB162343BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc