

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021245.D
 Acq On : 30 Jul 2024 22:09
 Operator : MA/JU
 Sample : P3347-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COB03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	27	30	38	rVB	26645	41766	0.75%	0.093%
2	3.887	150	153	157	rVB2	5986	8737	0.16%	0.020%
3	4.258	213	216	221	rVB6	6166	8105	0.15%	0.018%
4	5.663	450	455	464	rVB5	6937	14980	0.27%	0.034%
5	6.863	649	659	673	rBV	172051	443373	8.00%	0.992%
6	6.987	674	680	700	rVB	446832	797730	14.39%	1.785%
7	7.187	708	714	735	rBV	583275	1094433	19.74%	2.448%
8	7.634	783	790	804	rBV	601799	946019	17.06%	2.116%
9	7.734	804	807	817	rVB2	6262	15167	0.27%	0.034%
10	8.252	889	895	901	rBV10	3480	7108	0.13%	0.016%
11	8.363	908	914	933	rBV	482998	1064446	19.20%	2.381%
12	8.722	970	975	980	rBV5	7529	12995	0.23%	0.029%
13	8.787	980	986	1002	rVV	520700	1019789	18.39%	2.281%
14	8.899	1002	1005	1010	rVV3	14812	28188	0.51%	0.063%
15	8.957	1010	1015	1025	rVB7	9270	23124	0.42%	0.052%
16	9.357	1078	1083	1096	rBV3	46370	102283	1.84%	0.229%
17	9.504	1101	1108	1129	rVV	425041	905404	16.33%	2.026%
18	10.069	1196	1204	1222	rBV	470350	1338418	24.14%	2.994%
19	10.404	1252	1261	1273	rBV	708137	1324764	23.89%	2.964%
20	10.587	1285	1292	1308	rBV	75440	218805	3.95%	0.490%
21	11.281	1403	1410	1414	rBV9	5308	11648	0.21%	0.026%
22	11.604	1460	1465	1470	rBV8	3596	5802	0.10%	0.013%
23	12.022	1530	1536	1543	rBV4	8450	17401	0.31%	0.039%
24	13.687	1813	1819	1843	rBV	1333614	2182459	39.36%	4.883%
25	13.969	1859	1867	1883	rBV	1445946	2503818	45.16%	5.601%
26	14.275	1911	1919	1938	rBV	1181780	1918887	34.61%	4.293%
27	14.622	1972	1978	1993	rBV	67036	262021	4.73%	0.586%
28	15.134	2061	2065	2069	rVB6	6831	8021	0.14%	0.018%
29	15.292	2086	2092	2111	rVV	2149407	3217618	58.03%	7.198%
30	15.475	2116	2123	2132	rBV	549355	993673	17.92%	2.223%
31	15.681	2154	2158	2164	rVB4	10583	18302	0.33%	0.041%
32	15.881	2186	2192	2197	rBV10	2847	5996	0.11%	0.013%
33	16.016	2210	2215	2221	rBV2	12510	20919	0.38%	0.047%
34	16.828	2350	2353	2357	rBV2	11928	16174	0.29%	0.036%
35	16.881	2359	2362	2367	rVB4	7995	11017	0.20%	0.025%
36	17.098	2393	2399	2406	rBV	1716366	2422921	43.70%	5.420%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021245.D
Acq On : 30 Jul 2024 22:09
Operator : MA/JU
Sample : P3347-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	17.198	2409	2416	2435	rVB	2239171	3776010	68.11%	8.448%
38	17.598	2481	2484	2490	rVB6	10028	15319	0.28%	0.034%
39	17.780	2510	2515	2523	rBV3	47943	77857	1.40%	0.174%
40	17.957	2542	2545	2548	rVB5	9895	12036	0.22%	0.027%
41	18.033	2552	2558	2565	rBV4	34191	70890	1.28%	0.159%
42	18.310	2603	2605	2609	rVB4	12342	13345	0.24%	0.030%
43	19.122	2739	2743	2750	rVB2	33619	46829	0.84%	0.105%
44	19.216	2755	2759	2763	rVV	29794	39942	0.72%	0.089%
45	19.363	2780	2784	2791	rBV9	23191	52269	0.94%	0.117%
46	19.586	2814	2822	2835	rBV	2916225	5066985	91.39%	11.336%
47	21.545	3149	3155	3165	rBV	1852948	3248191	58.59%	7.267%
48	24.627	3669	3679	3695	rVB	2150106	5544347	100.00%	12.404%
49	24.851	3707	3717	3735	rVB2	1190469	3703007	66.79%	8.284%




Sum of corrected areas: 44699338

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021245.D
Acq On : 30 Jul 2024 22:09
Operator : MA/JU
Sample : P3347-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

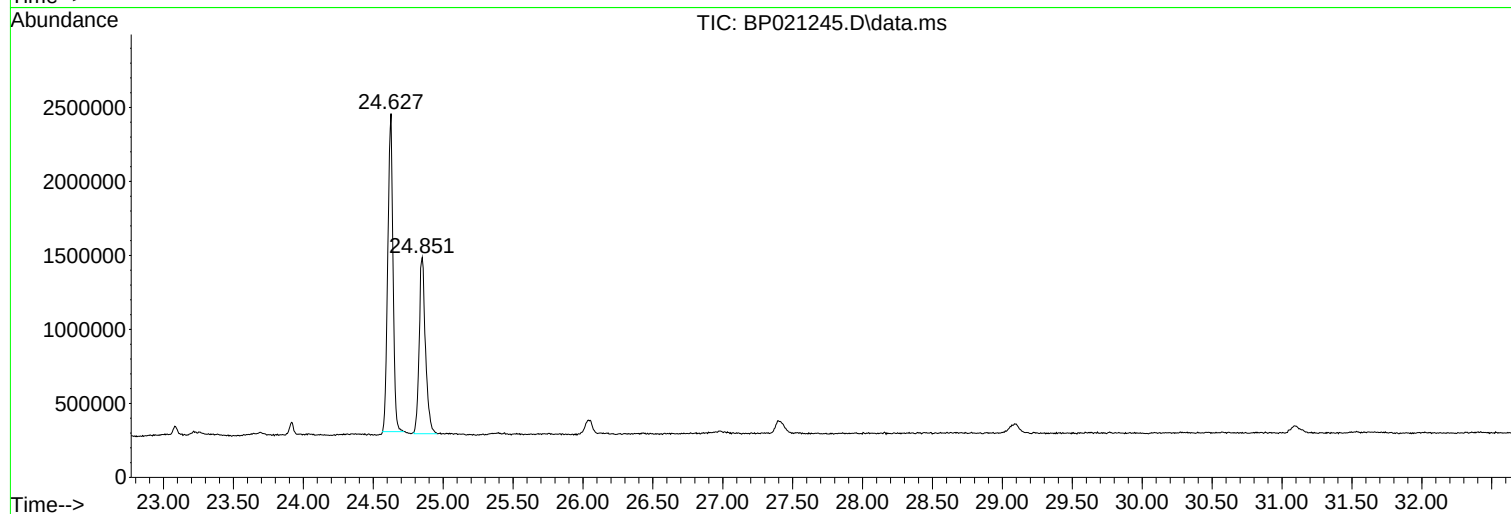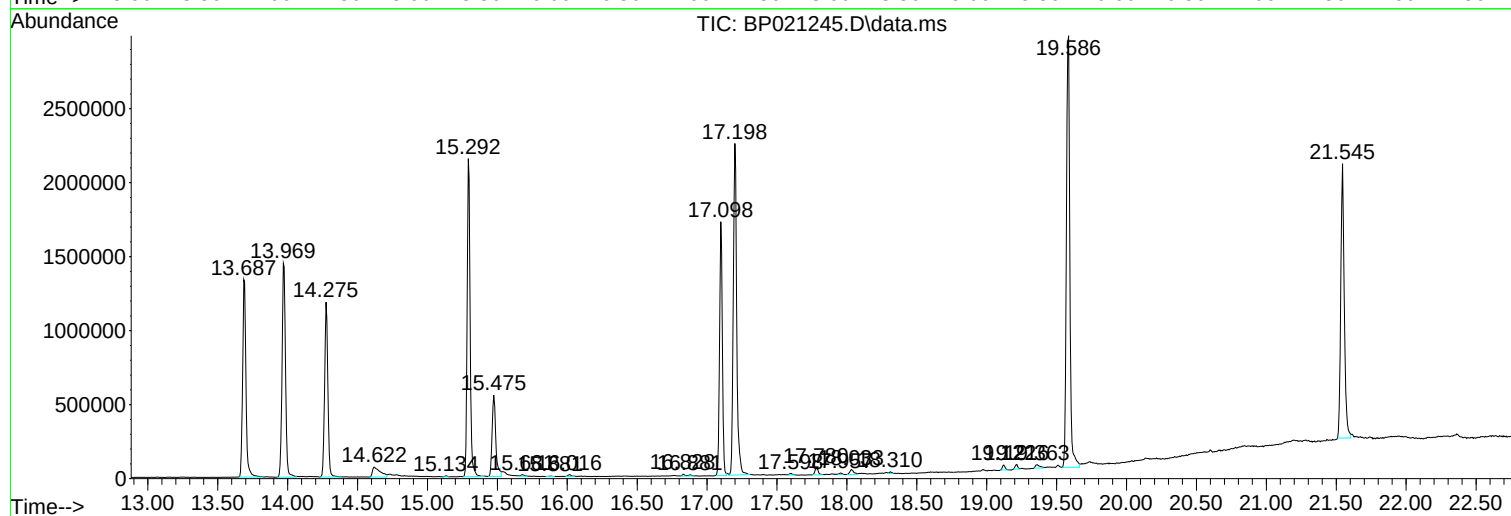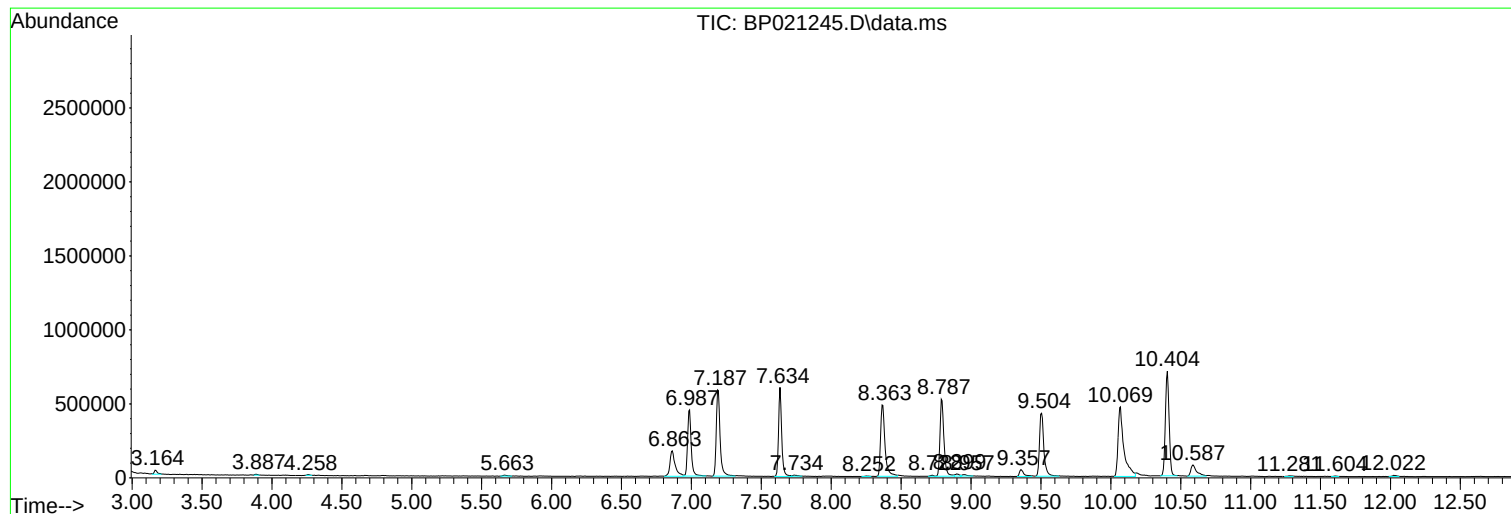

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021245.D
Acq On : 30 Jul 2024 22:09
Operator : MA/JU
Sample : P3347-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021245.D
Acq On : 30 Jul 2024 22:09
Operator : MA/JU
Sample : P3347-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc