

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021253.D
 Acq On : 31 Jul 2024 04:38
 Operator : MA/JU
 Sample : PB162261BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	27	31	42	rVB	36039	55533	1.24%	0.133%
2	3.587	99	102	128	rBV	376625	762720	17.02%	1.827%
3	3.893	149	154	159	rVB	8683	13657	0.30%	0.033%
4	6.852	649	657	675	rBV	433546	960307	21.43%	2.300%
5	6.987	675	680	703	rVV	409091	760878	16.98%	1.822%
6	7.187	707	714	734	rBV	572424	1018142	22.72%	2.438%
7	7.634	783	790	807	rBV	525485	916138	20.44%	2.194%
8	8.363	907	914	937	rBV	488618	1230026	27.45%	2.946%
9	8.793	979	987	1007	rBV	456838	964358	21.52%	2.310%
10	9.510	1101	1109	1125	rBV	424109	838214	18.70%	2.007%
11	10.057	1196	1202	1222	rBV	501058	1222339	27.28%	2.927%
12	10.404	1253	1261	1278	rVB	720065	1270872	28.36%	3.044%
13	10.563	1280	1288	1313	rBV	440100	1242247	27.72%	2.975%
14	12.051	1529	1541	1548	rBV2	8074	20885	0.47%	0.050%
15	13.687	1811	1819	1834	rBV	1040892	2017027	45.01%	4.831%
16	13.969	1859	1867	1880	rBV	1575966	2304361	51.42%	5.519%
17	14.275	1909	1919	1932	rBV	1142135	1782677	39.78%	4.269%
18	14.598	1967	1974	1989	rBV2	171060	623059	13.90%	1.492%
19	14.810	2007	2010	2015	rVB6	6700	10177	0.23%	0.024%
20	15.292	2084	2092	2110	rBV	1738395	2987129	66.65%	7.154%
21	15.469	2116	2122	2142	rBV	429768	872819	19.48%	2.090%
22	16.098	2225	2229	2236	rVB6	6817	10927	0.24%	0.026%
23	16.763	2338	2342	2348	rVB8	3947	6783	0.15%	0.016%
24	16.881	2359	2362	2369	rBV5	3227	5538	0.12%	0.013%
25	17.098	2392	2399	2409	rBV	1528956	2298853	51.30%	5.505%
26	17.204	2410	2417	2426	rBV	2010548	3347424	74.69%	8.017%
27	17.781	2513	2515	2526	rVB	7319	11361	0.25%	0.027%
28	19.133	2741	2745	2752	rBV4	30452	48279	1.08%	0.116%
29	19.222	2756	2760	2766	rBV	26306	44614	1.00%	0.107%
30	19.592	2816	2823	2836	rBV	2724000	4481534	100.00%	10.733%
31	21.545	3149	3155	3171	rBV	1494021	2765047	61.70%	6.622%
32	24.621	3668	3678	3699	rBV	1522953	4077559	90.99%	9.765%
33	24.845	3707	3716	3740	rVB	814428	2784366	62.13%	6.668%




Sum of corrected areas: 41755850

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021253.D
Acq On : 31 Jul 2024 04:38
Operator : MA/JU
Sample : PB162261BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

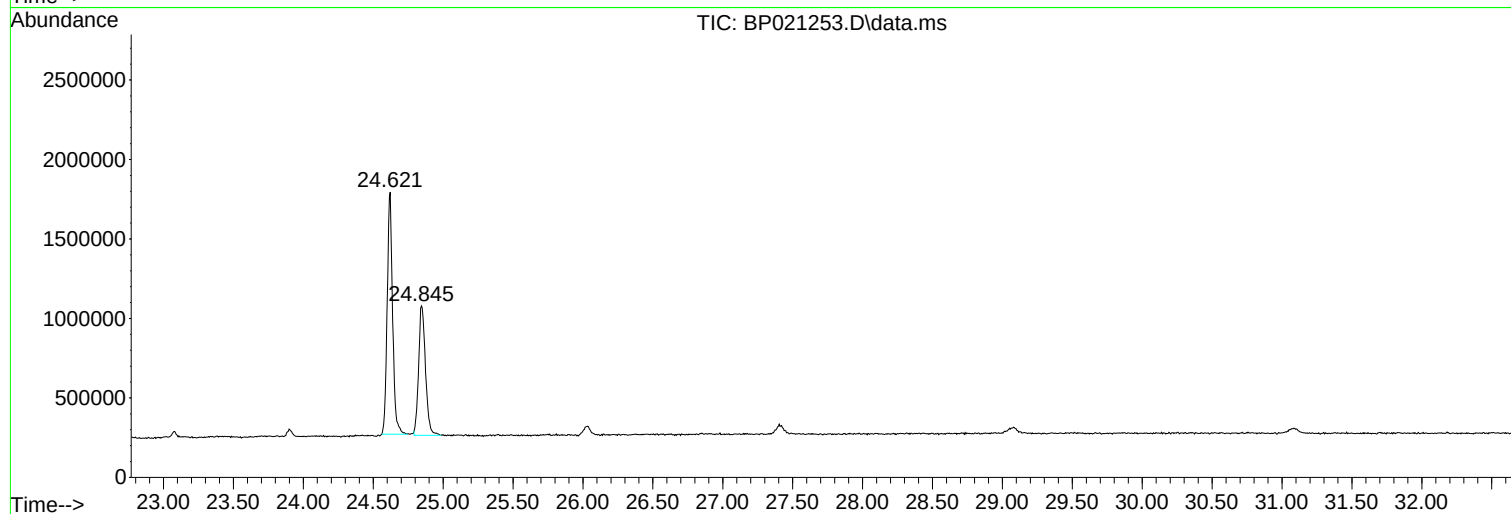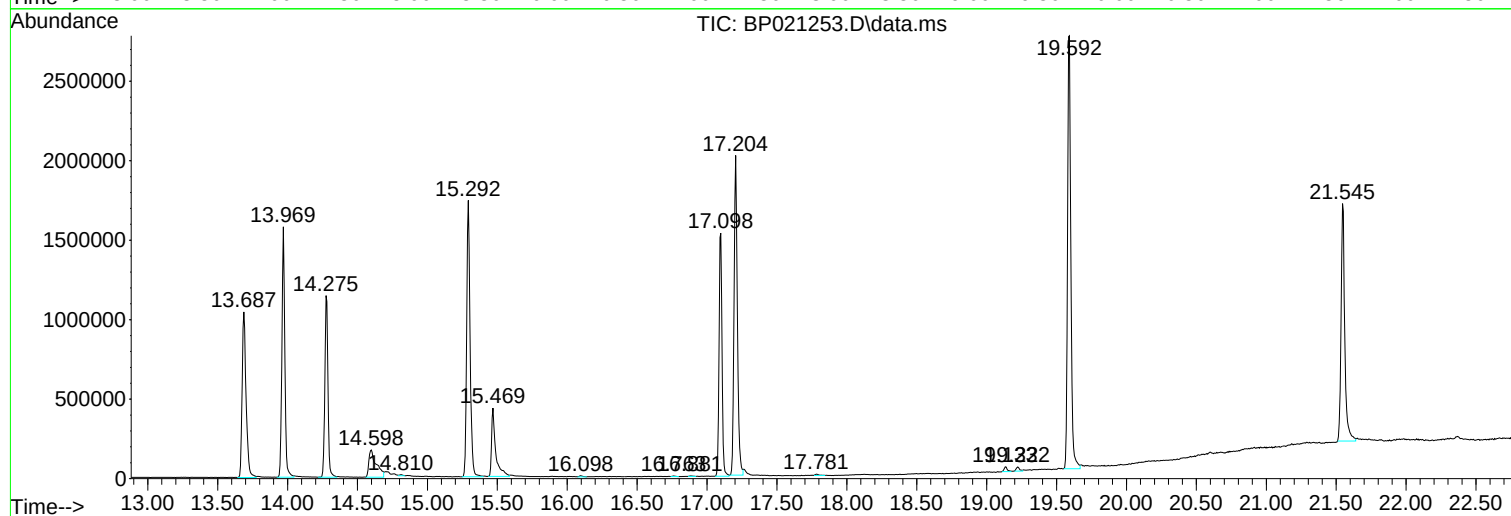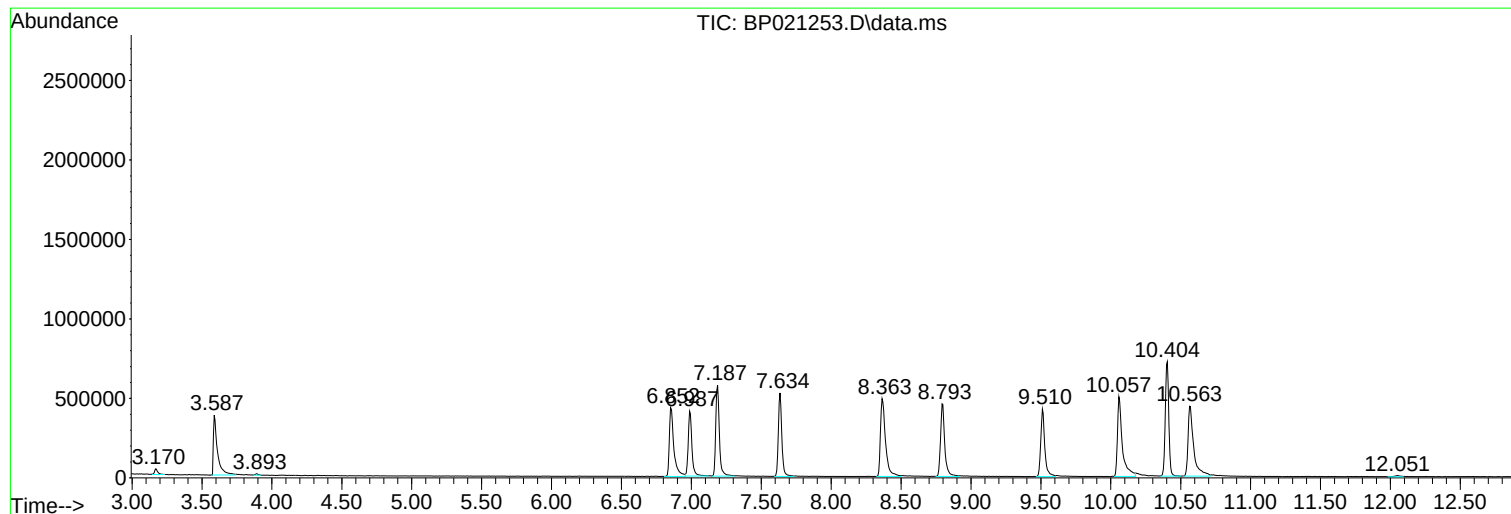

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021253.D
Acq On : 31 Jul 2024 04:38
Operator : MA/JU
Sample : PB162261BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021253.D
Acq On : 31 Jul 2024 04:38
Operator : MA/JU
Sample : PB162261BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------