

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021265.D
 Acq On : 31 Jul 2024 17:50
 Operator : CG/JU
 Sample : P3265-02DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4DL0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.881	148	152	158	rVB4	6349	11091	0.25%	0.020%
2	6.887	650	663	674	rBV2	60316	250960	5.68%	0.453%
3	6.981	674	679	688	rVV	63744	108257	2.45%	0.195%
4	7.064	688	693	707	rVV	356237	575650	13.03%	1.038%
5	7.211	713	718	740	rVB	322799	666488	15.09%	1.202%
6	7.628	781	789	792	rBV	488827	847555	19.19%	1.528%
7	7.663	792	795	807	rVB	648732	1052924	23.84%	1.899%
8	7.975	840	848	867	rBV	548075	1045628	23.68%	1.886%
9	8.387	910	918	920	rBV	59716	105162	2.38%	0.190%
10	8.428	920	925	941	rVB	428662	793571	17.97%	1.431%
11	8.805	981	989	1007	rBV	61970	131644	2.98%	0.237%
12	9.169	1048	1051	1059	rVB8	3853	7978	0.18%	0.014%
13	9.340	1073	1080	1097	rBV	627667	1162588	26.32%	2.096%
14	9.534	1102	1113	1127	rVV2	172705	447508	10.13%	0.807%
15	9.652	1128	1133	1140	rVB2	23160	42701	0.97%	0.077%
16	10.075	1195	1205	1234	rBV2	481140	1604132	36.32%	2.893%
17	10.387	1251	1258	1262	rBV	633976	1107323	25.07%	1.997%
18	10.434	1262	1266	1286	rVB	922386	1601946	36.27%	2.889%
19	10.587	1286	1292	1306	rBV2	42822	115385	2.61%	0.208%
20	11.199	1389	1396	1401	rBV8	3873	9005	0.20%	0.016%
21	11.757	1484	1491	1505	rBV	78964	179913	4.07%	0.324%
22	11.957	1518	1525	1529	rBV5	4210	8067	0.18%	0.015%
23	12.063	1535	1543	1557	rBV	975091	1892620	42.85%	3.413%
24	12.281	1575	1580	1587	rVB3	10267	19380	0.44%	0.035%
25	12.716	1646	1654	1664	rBV	129140	263111	5.96%	0.474%
26	12.810	1664	1670	1691	rVB	185339	478378	10.83%	0.863%
27	13.051	1707	1711	1717	rVB7	3825	6971	0.16%	0.013%
28	13.310	1753	1755	1761	rVB5	4414	6000	0.14%	0.011%
29	13.681	1812	1818	1830	rBV	184356	283737	6.42%	0.512%
30	13.863	1842	1849	1860	rBV	1096225	1684231	38.14%	3.037%
31	13.987	1860	1870	1888	rVB2	783415	1657570	37.53%	2.989%
32	14.263	1911	1917	1923	rBV	987669	1465246	33.18%	2.642%
33	14.334	1923	1929	1935	rVV	1344099	2192401	49.64%	3.953%
34	14.381	1935	1937	1945	rVB2	16663	26783	0.61%	0.048%
35	14.687	1974	1989	2017	rBV2	620968	1628119	36.87%	2.936%
36	14.957	2030	2035	2036	rBV5	5660	7374	0.17%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021265.D
 Acq On : 31 Jul 2024 17:50
 Operator : CG/JU
 Sample : P3265-02DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4DL0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	15.110	2055	2061	2077	rBV	1480755	1944042	44.02%	3.506%
38	15.281	2084	2090	2094	rBV	297782	441343	9.99%	0.796%
39	15.334	2094	2099	2116	rVB2	1449343	2659243	60.21%	4.795%
40	15.498	2121	2127	2138	rVV2	30993	75245	1.70%	0.136%
41	15.592	2139	2143	2152	rVB3	15487	25796	0.58%	0.047%
42	15.857	2182	2188	2191	rBV8	5033	9608	0.22%	0.017%
43	15.945	2200	2203	2210	rVB6	7538	11424	0.26%	0.021%
44	16.057	2218	2222	2232	rVB10	6542	15363	0.35%	0.028%
45	16.251	2250	2255	2268	rVB	516642	771977	17.48%	1.392%
46	16.610	2312	2316	2319	rBV4	3824	5661	0.13%	0.010%
47	16.745	2332	2339	2358	rBV	476372	931260	21.09%	1.679%
48	17.087	2390	2397	2401	rBV	1227180	1698955	38.47%	3.064%
49	17.128	2401	2404	2410	rVV	577828	803741	18.20%	1.449%
50	17.187	2410	2414	2417	rVV	276464	460541	10.43%	0.830%
51	17.228	2417	2421	2440	rVB	1189932	1915452	43.37%	3.454%
52	17.722	2500	2505	2510	rBV7	12796	26896	0.61%	0.049%
53	17.781	2511	2515	2520	rVB	31605	40887	0.93%	0.074%
54	18.022	2551	2556	2561	rBV3	30124	52108	1.18%	0.094%
55	18.086	2562	2567	2576	rVV	1190122	1544395	34.97%	2.785%
56	18.416	2619	2623	2628	rBV7	8579	18162	0.41%	0.033%
57	18.498	2634	2637	2642	rVB5	8616	14237	0.32%	0.026%
58	18.604	2650	2655	2667	rBV	58335	127064	2.88%	0.229%
59	19.228	2756	2761	2774	rBV	1075548	1661433	37.62%	2.996%
60	19.357	2780	2783	2789	rVB6	18237	28163	0.64%	0.051%
61	19.581	2816	2821	2833	rBV	371681	626277	14.18%	1.129%
62	20.545	2981	2985	2991	rBV	201928	254148	5.75%	0.458%
63	21.422	3128	3134	3142	rBV	3504606	4416414	100.00%	7.964%
64	21.533	3145	3153	3172	rVV3	1346193	3425546	77.56%	6.177%
65	22.669	3340	3346	3356	rVB	1398129	2406195	54.48%	4.339%
66	23.792	3531	3537	3544	rBV	456734	1065787	24.13%	1.922%
67	23.869	3544	3550	3562	rVB	344601	1016839	23.02%	1.834%
68	24.621	3673	3678	3683	rBV	175784	369178	8.36%	0.666%
69	24.698	3685	3691	3701	rVB	301383	759128	17.19%	1.369%
70	24.833	3707	3714	3730	rVB	812964	2345355	53.11%	4.229%




Sum of corrected areas: 55455260

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021265.D
Acq On : 31 Jul 2024 17:50
Operator : CG/JU
Sample : P3265-02DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4DL0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

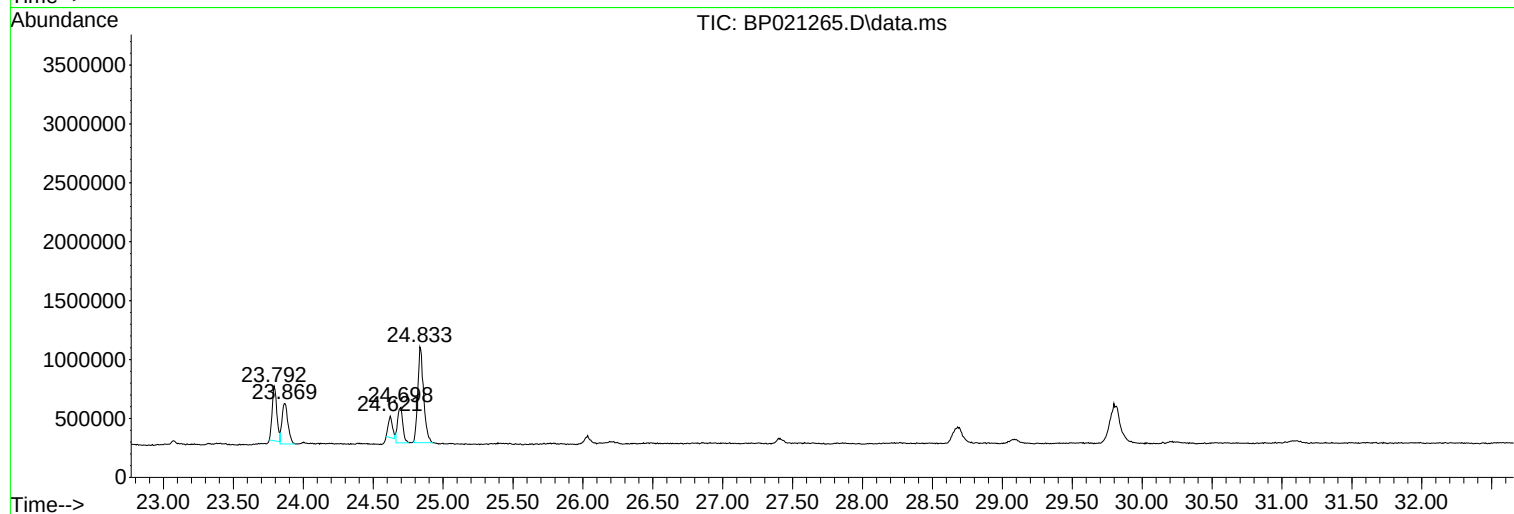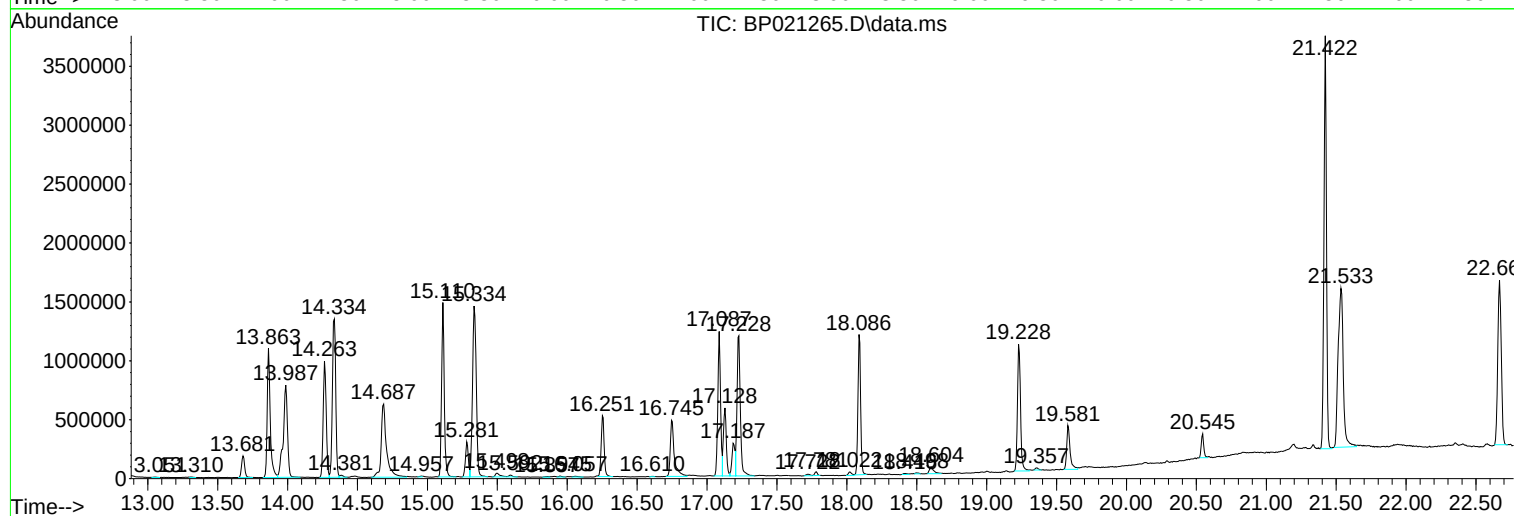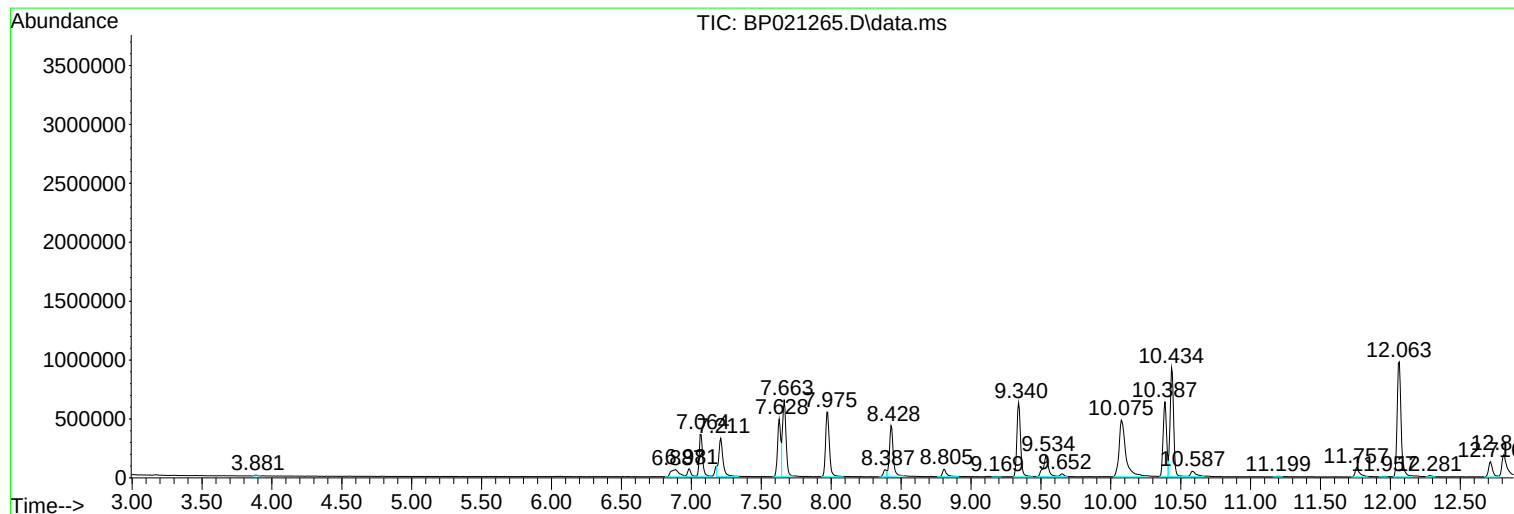

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021265.D
Acq On : 31 Jul 2024 17:50
Operator : CG/JU
Sample : P3265-02DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4DL0DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,2-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.975	24.67 ng/ul	1045630	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	98
2			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
3			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	97
4			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
5			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	96

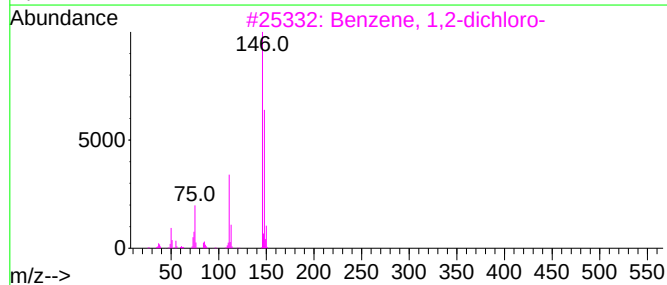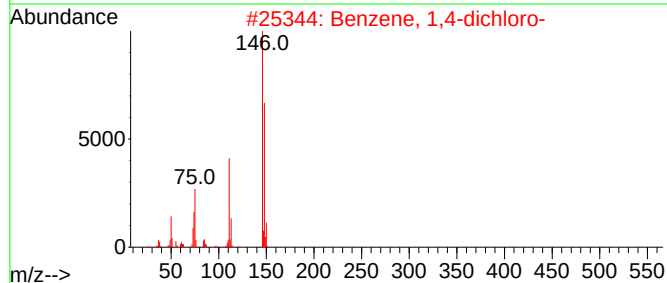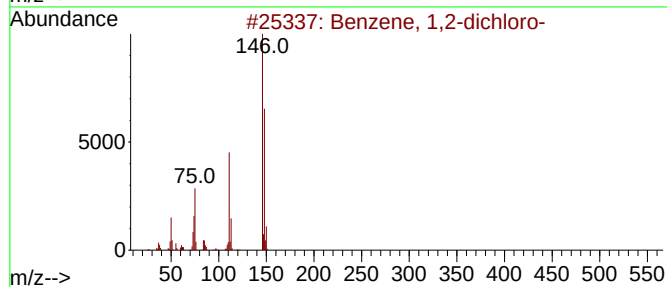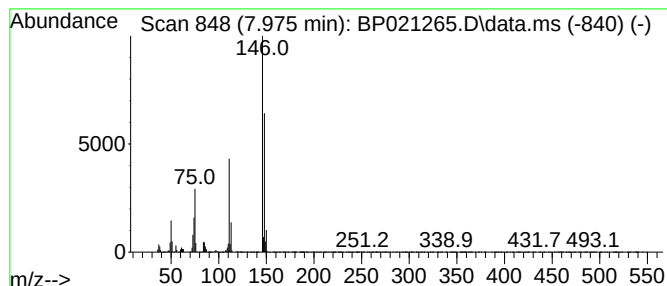

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021265.D
Acq On : 31 Jul 2024 17:50
Operator : CG/JU
Sample : P3265-02DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4DL0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,2-di...	7.975	24.7	ng/ul	1045630	1	7.628	847555	20.0