

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021276.D
 Acq On : 01 Aug 2024 01:52
 Operator : CG/JU
 Sample : P3347-06DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.617	105	107	118	rBV	21838	45975	1.32%	0.156%
2	3.887	150	153	159	rVB3	6372	9017	0.26%	0.031%
3	4.634	275	280	286	rBV8	4503	10300	0.29%	0.035%
4	4.775	299	304	306	rBV6	2776	4685	0.13%	0.016%
5	5.187	368	374	380	rBV5	4129	7980	0.23%	0.027%
6	5.681	450	458	464	rBV5	4653	11636	0.33%	0.040%
7	6.734	632	637	642	rBV6	5475	10043	0.29%	0.034%
8	6.875	654	661	663	rBV3	32900	58549	1.68%	0.199%
9	6.993	676	681	694	rVB	97855	182765	5.23%	0.621%
10	7.193	709	715	725	rBV	117381	233651	6.69%	0.793%
11	7.275	725	729	736	rVB2	10922	21435	0.61%	0.073%
12	7.628	780	789	797	rBV	519707	948146	27.15%	3.220%
13	7.693	797	800	820	rVB4	41181	140343	4.02%	0.477%
14	7.981	842	849	858	rBV	89580	164575	4.71%	0.559%
15	8.164	876	880	885	rBV3	4401	7098	0.20%	0.024%
16	8.381	910	917	933	rBV	90968	252821	7.24%	0.859%
17	8.493	933	936	942	rVB7	6324	10492	0.30%	0.036%
18	8.734	968	977	982	rBV6	9208	21817	0.62%	0.074%
19	8.805	982	989	1006	rVV	112905	246699	7.06%	0.838%
20	8.958	1011	1015	1023	rVB5	7424	16619	0.48%	0.056%
21	9.093	1031	1038	1041	rBV2	11453	25553	0.73%	0.087%
22	9.234	1057	1062	1066	rVB7	1869	4006	0.11%	0.014%
23	9.287	1066	1071	1075	rBV6	3059	4650	0.13%	0.016%
24	9.516	1103	1110	1125	rBV	96352	220283	6.31%	0.748%
25	9.646	1127	1132	1136	rVB3	6092	10516	0.30%	0.036%
26	9.793	1148	1157	1160	rBV4	10716	23667	0.68%	0.080%
27	9.899	1170	1175	1178	rBV5	5021	7865	0.23%	0.027%
28	10.081	1198	1206	1228	rBV2	99635	330595	9.47%	1.123%
29	10.387	1251	1258	1262	rBV	866501	1384934	39.66%	4.703%
30	10.434	1262	1266	1281	rVV	1584503	2733410	78.27%	9.283%
31	10.575	1282	1290	1308	rVV4	110981	335900	9.62%	1.141%
32	10.816	1327	1331	1336	rVB7	4222	7346	0.21%	0.025%
33	11.087	1371	1377	1379	rBV	4992	9184	0.26%	0.031%
34	11.516	1448	1450	1457	rVB7	2654	4238	0.12%	0.014%
35	11.605	1460	1465	1470	rVB3	8358	14590	0.42%	0.050%
36	11.963	1520	1526	1529	rBV4	11372	20972	0.60%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021276.D
 Acq On : 01 Aug 2024 01:52
 Operator : CG/JU
 Sample : P3347-06DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	12.069	1536	1544	1557	rBV	135062	312990	8.96%	1.063%
38	12.193	1559	1565	1572	rVV8	5262	13142	0.38%	0.045%
39	12.281	1572	1580	1593	rVB	127976	255351	7.31%	0.867%
40	12.499	1613	1617	1622	rVB8	2315	3600	0.10%	0.012%
41	12.587	1628	1632	1637	rVB7	3159	5789	0.17%	0.020%
42	13.034	1701	1708	1712	rBV9	2257	4153	0.12%	0.014%
43	13.093	1712	1718	1726	rBV2	23125	53332	1.53%	0.181%
44	13.257	1738	1746	1747	rBV7	3998	6736	0.19%	0.023%
45	13.293	1747	1752	1759	rVB3	8747	19080	0.55%	0.065%
46	13.422	1768	1774	1782	rBV6	11281	33747	0.97%	0.115%
47	13.581	1793	1801	1807	rBV3	21102	49663	1.42%	0.169%
48	13.681	1812	1818	1830	rVB	375085	617974	17.70%	2.099%
49	13.816	1836	1841	1852	rVB4	15578	38688	1.11%	0.131%
50	13.957	1858	1865	1880	rBV	444953	697924	19.99%	2.370%
51	14.198	1900	1906	1908	rBV6	5210	8962	0.26%	0.030%
52	14.263	1911	1917	1924	rVV	1281799	1997313	57.19%	6.783%
53	14.328	1924	1928	1941	rVV	187440	335829	9.62%	1.140%
54	14.451	1942	1949	1958	rVV	13802	43072	1.23%	0.146%
55	14.581	1966	1971	1976	rVB3	10038	19555	0.56%	0.066%
56	14.687	1982	1989	1999	rBV	102397	190664	5.46%	0.648%
57	15.051	2047	2051	2052	rBV4	3198	3705	0.11%	0.013%
58	15.110	2058	2061	2063	rBV4	4206	4900	0.14%	0.017%
59	15.281	2082	2090	2096	rBV	584428	931732	26.68%	3.164%
60	15.345	2096	2101	2109	rVB	113595	218654	6.26%	0.743%
61	15.475	2114	2123	2132	rBV5	81680	261992	7.50%	0.890%
62	15.645	2149	2152	2158	rVB2	13509	19536	0.56%	0.066%
63	15.798	2172	2178	2185	rBV5	17985	41790	1.20%	0.142%
64	15.887	2188	2193	2196	rVB4	14099	20682	0.59%	0.070%
65	16.151	2234	2238	2248	rBV6	12243	26980	0.77%	0.092%
66	16.387	2272	2278	2285	rVB6	15084	35564	1.02%	0.121%
67	16.904	2362	2366	2374	rVB	23007	36932	1.06%	0.125%
68	17.004	2378	2383	2390	rBV8	18882	54995	1.57%	0.187%
69	17.081	2390	2396	2401	rVV	1782423	2568009	73.54%	8.721%
70	17.122	2401	2403	2409	rVV	208612	300378	8.60%	1.020%
71	17.192	2409	2415	2426	rVB	634863	1158054	33.16%	3.933%
72	17.316	2431	2436	2442	rVB2	22692	47625	1.36%	0.162%
73	17.516	2465	2470	2483	rVB	167706	355115	10.17%	1.206%
74	17.716	2502	2504	2510	rBV4	11328	18944	0.54%	0.064%
75	17.781	2510	2515	2520	rBV	39258	70927	2.03%	0.241%
76	17.834	2521	2524	2528	rBV	22794	29799	0.85%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021276.D
 Acq On : 01 Aug 2024 01:52
 Operator : CG/JU
 Sample : P3347-06DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

77	17.992	2545	2551	2552	rBV3	22741	39478	1.13%	0.134%
78	18.022	2553	2556	2559	rVV	50362	67940	1.95%	0.231%
79	18.057	2559	2562	2572	rVB7	38773	77206	2.21%	0.262%
80	18.198	2583	2586	2594	rVB4	34708	62173	1.78%	0.211%
81	18.316	2602	2606	2611	rBV3	36618	84453	2.42%	0.287%
82	18.763	2679	2682	2686	rBV4	20749	26022	0.75%	0.088%
83	18.875	2697	2701	2705	rBV4	24678	36751	1.05%	0.125%
84	19.092	2735	2738	2741	rBV2	27394	45165	1.29%	0.153%
85	19.233	2758	2762	2771	rVB	166372	238414	6.83%	0.810%
86	19.351	2779	2782	2787	rVB6	40271	52010	1.49%	0.177%
87	19.451	2796	2799	2802	rBV	39756	47667	1.36%	0.162%
88	19.581	2815	2821	2831	rBV	1040739	1772270	50.75%	6.019%
89	21.139	3082	3086	3089	rBV	98748	147058	4.21%	0.499%
90	21.533	3147	3153	3159	rBV	2062982	3413010	97.73%	11.591%
91	24.604	3668	3675	3684	rVB	563241	1387969	39.75%	4.714%
92	24.833	3704	3714	3726	rVB	1256357	3492132	100.00%	11.859%




Sum of corrected areas: 29445950

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021276.D
Acq On : 01 Aug 2024 01:52
Operator : CG/JU
Sample : P3347-06DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

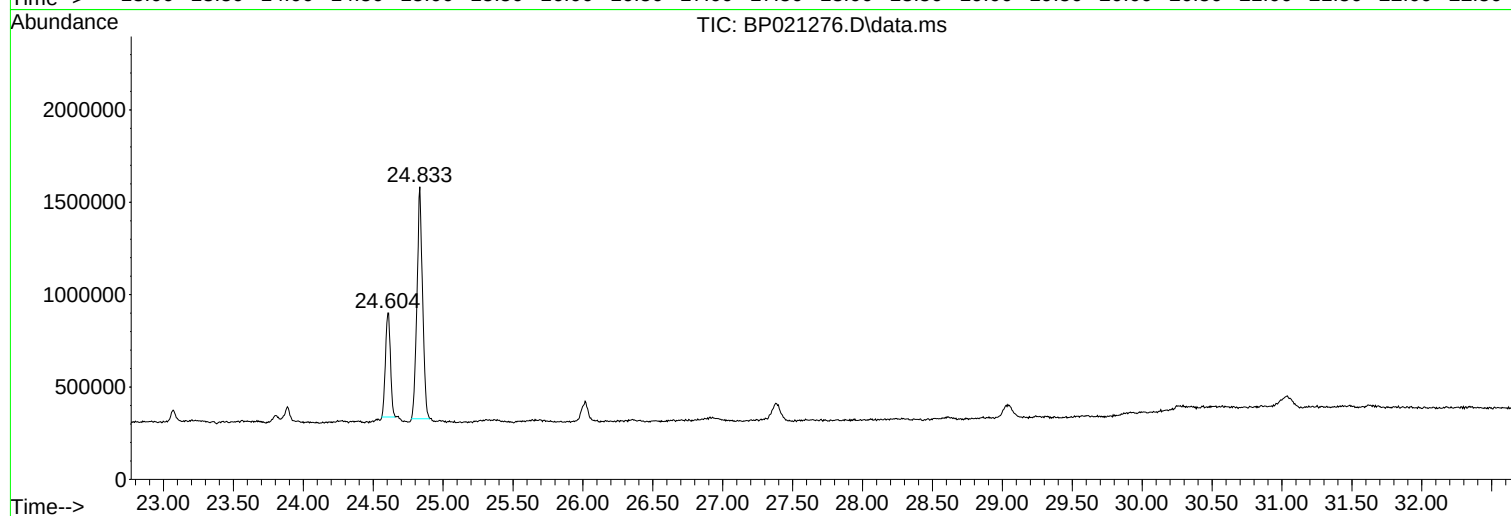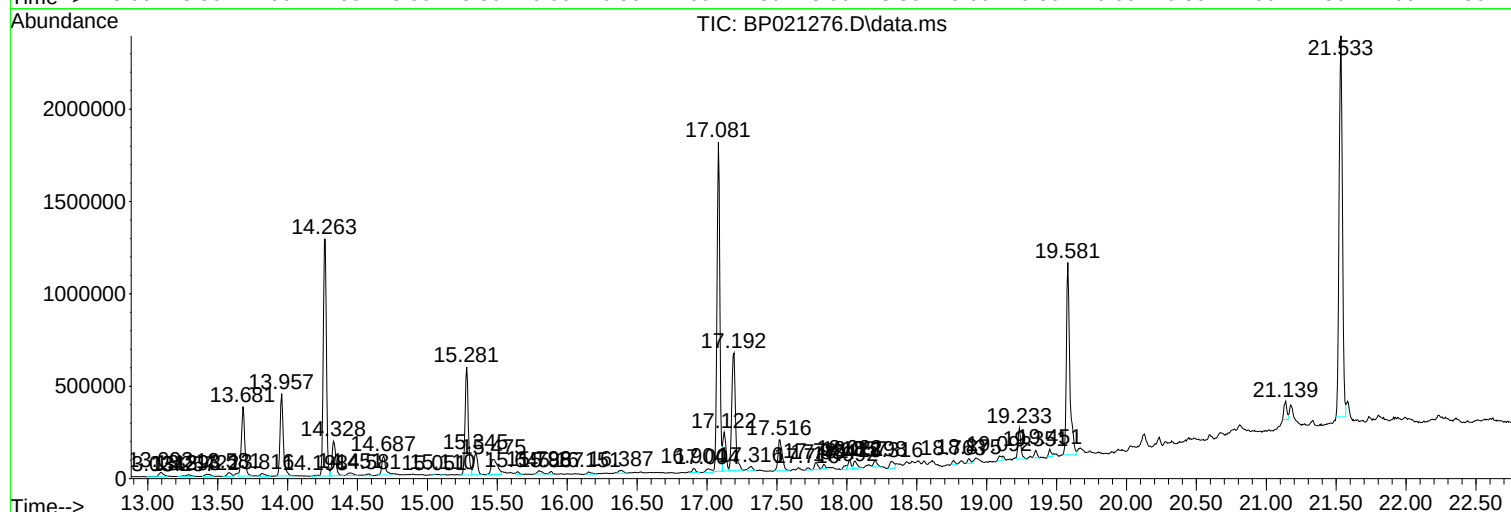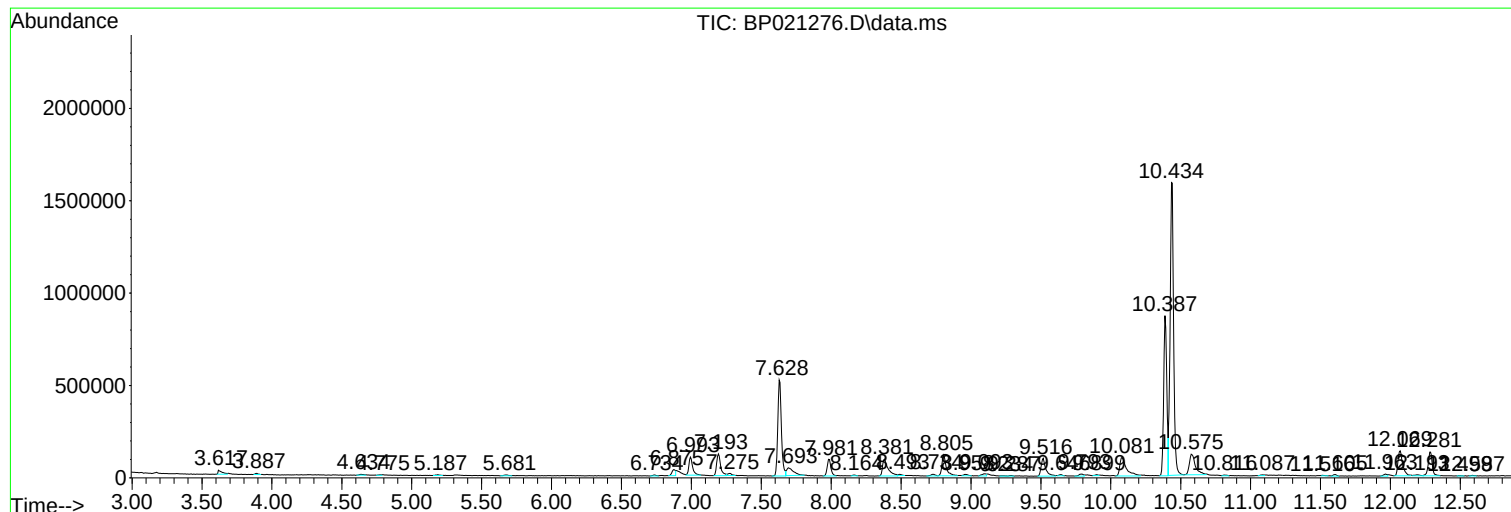

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021276.D
Acq On : 01 Aug 2024 01:52
Operator : CG/JU
Sample : P3347-06DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ0DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.693	2.96 ng/ul	140343	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	59
5	2-Propyl-1-pentanol			130	C8H18O	058175-57-8	50

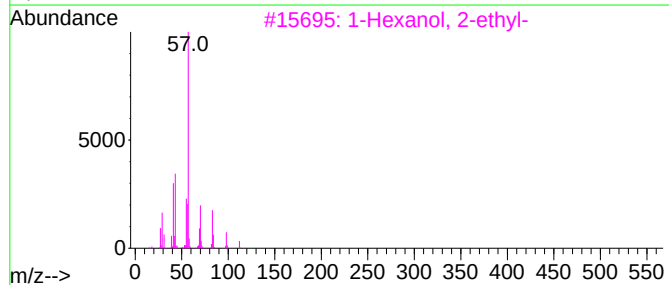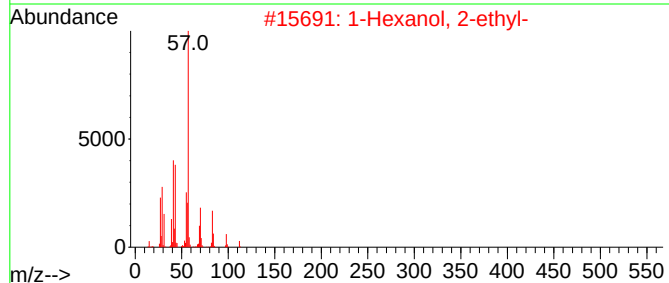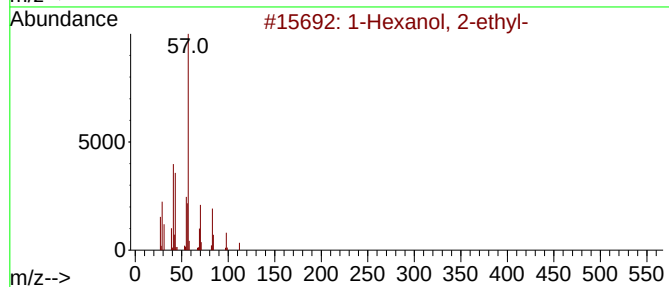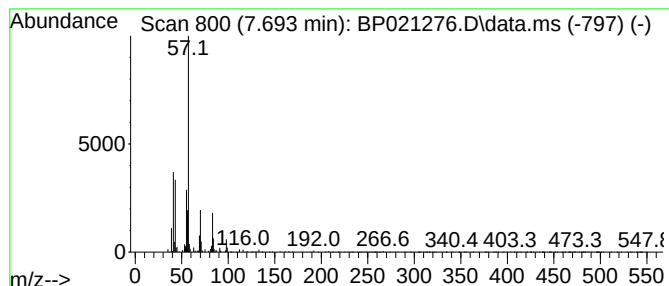

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021276.D
Acq On : 01 Aug 2024 01:52
Operator : CG/JU
Sample : P3347-06DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ0DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.981	3.47 ng/ul	164575	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	93
2	Indane			118	C9H10	000496-11-7	91
3	Indane			118	C9H10	000496-11-7	87
4	Indane			118	C9H10	000496-11-7	87
5	Benzene, 2-propenyl-			118	C9H10	000300-57-2	83

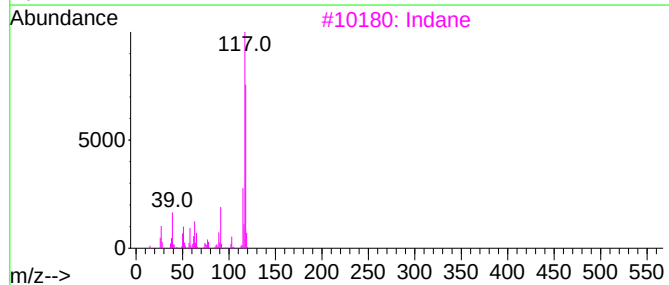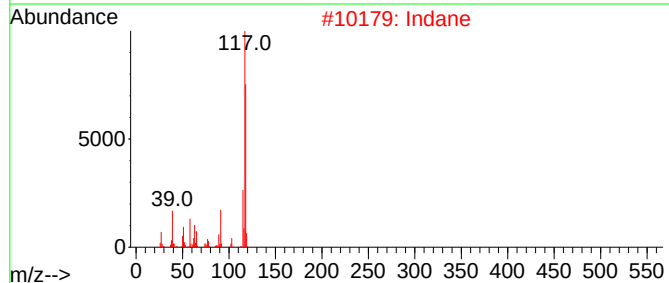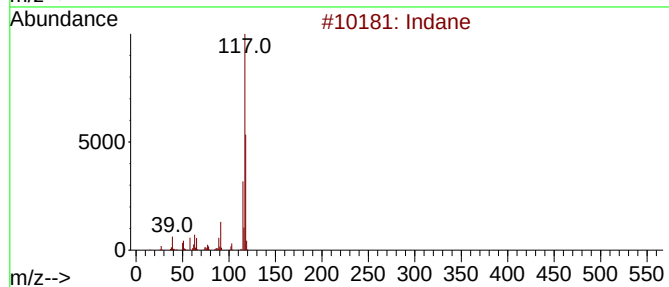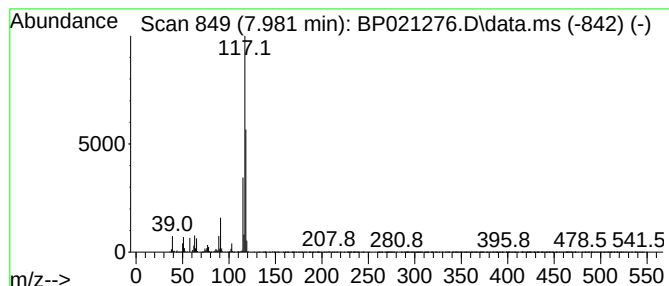

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021276.D
Acq On : 01 Aug 2024 01:52
Operator : CG/JU
Sample : P3347-06DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	7.693	3.0	ng/ul	140343	1	7.628	948146	20.0
Indane	7.981	3.5	ng/ul	164575	1	7.628	948146	20.0