
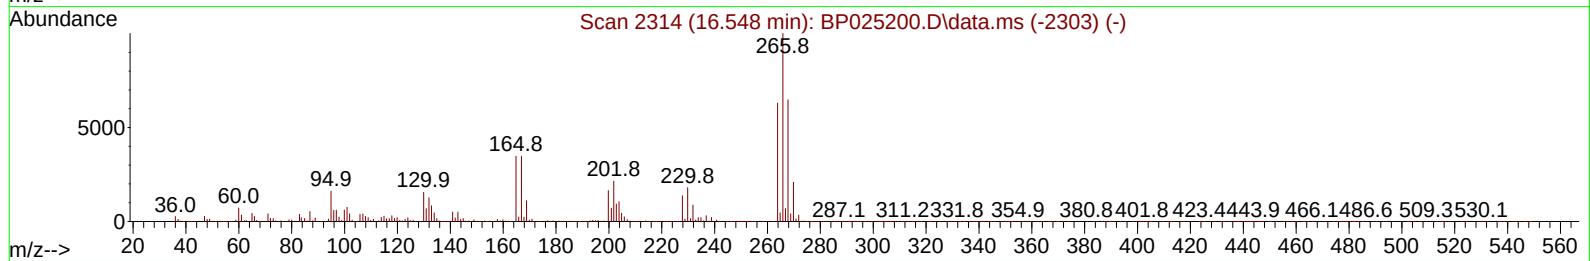
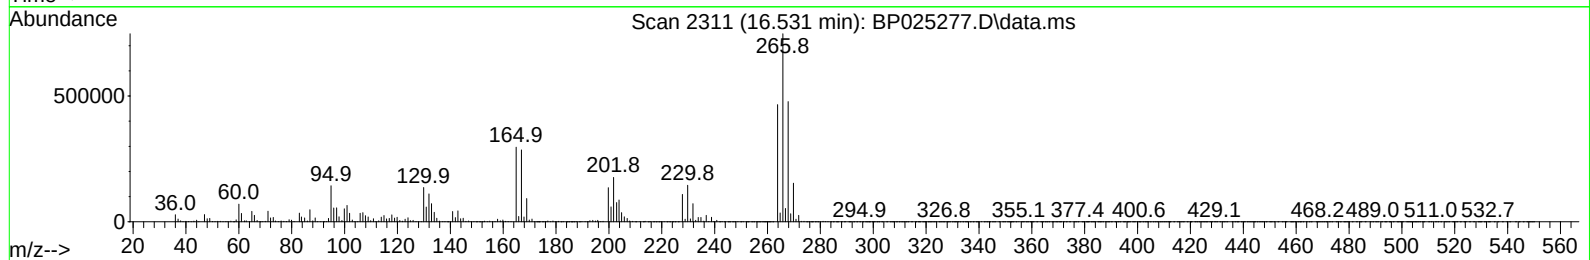


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073125\
Data File : BP025277.D
Acq On : 31 Jul 2025 11:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 12:50:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

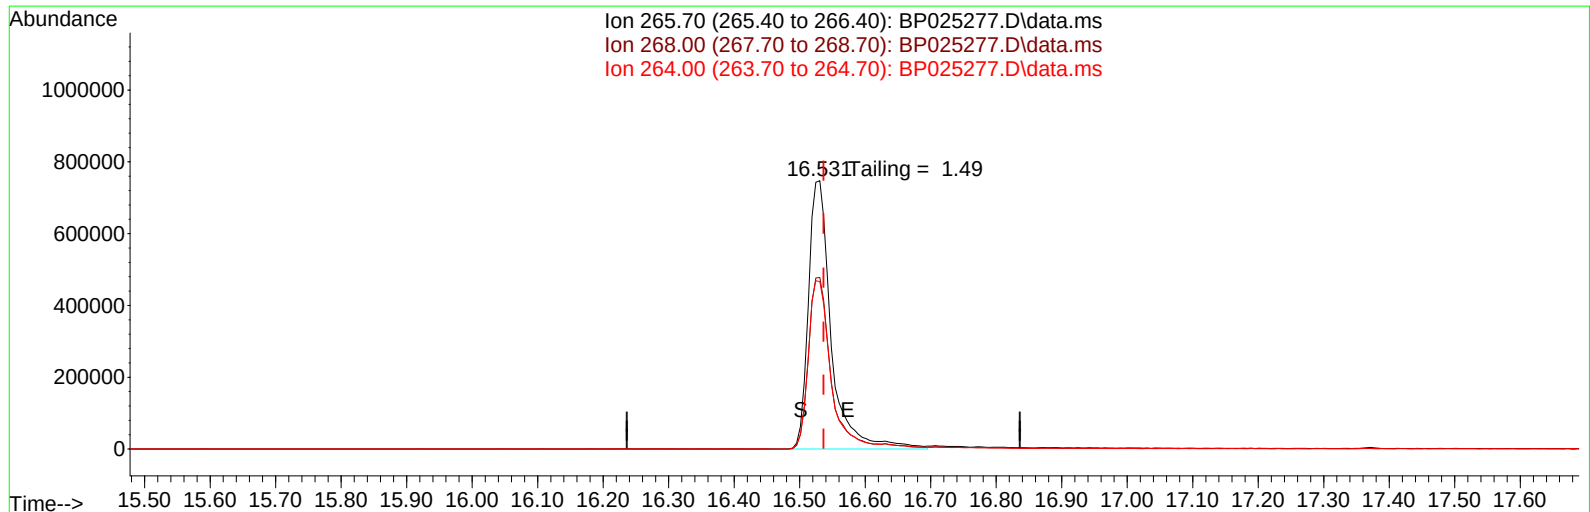

TIC: BP025277.D\data.ms

(70) Pentachlorophenol (C)




16.531min (-0.006) 146742.07 ng

response 1813117

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.94
264.00	62.90	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073125\
Data File : BP025277.D
Acq On : 31 Jul 2025 11:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 12:50:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

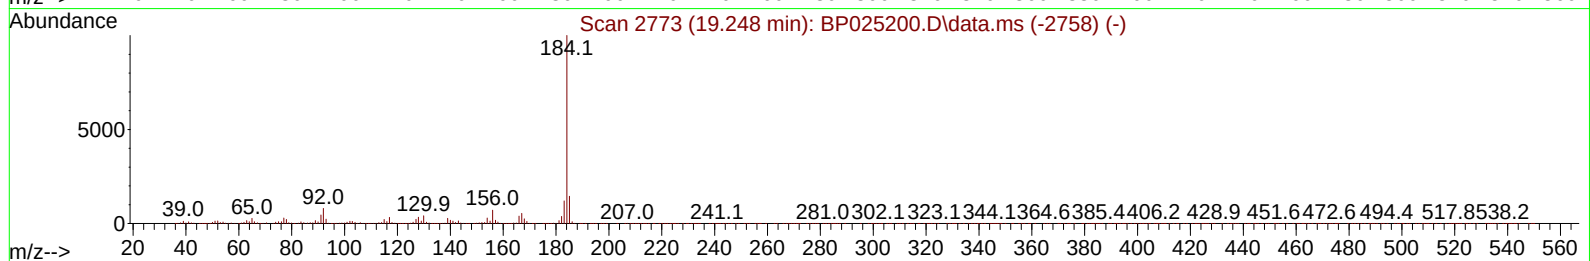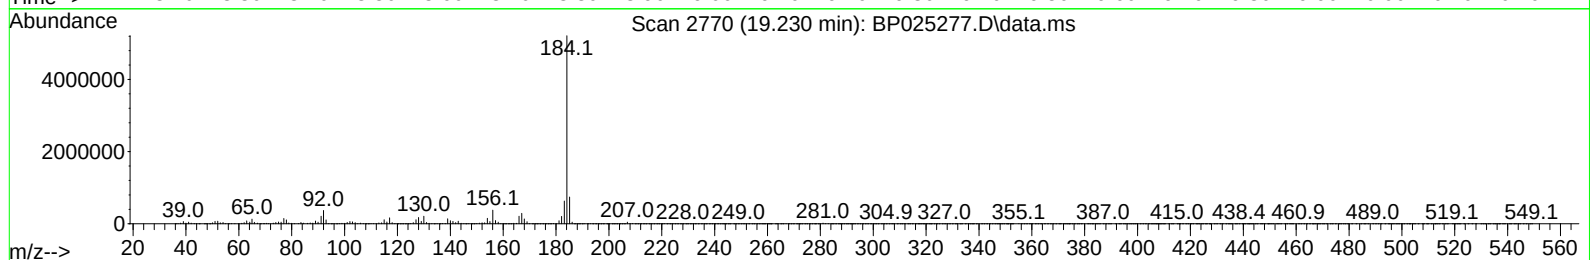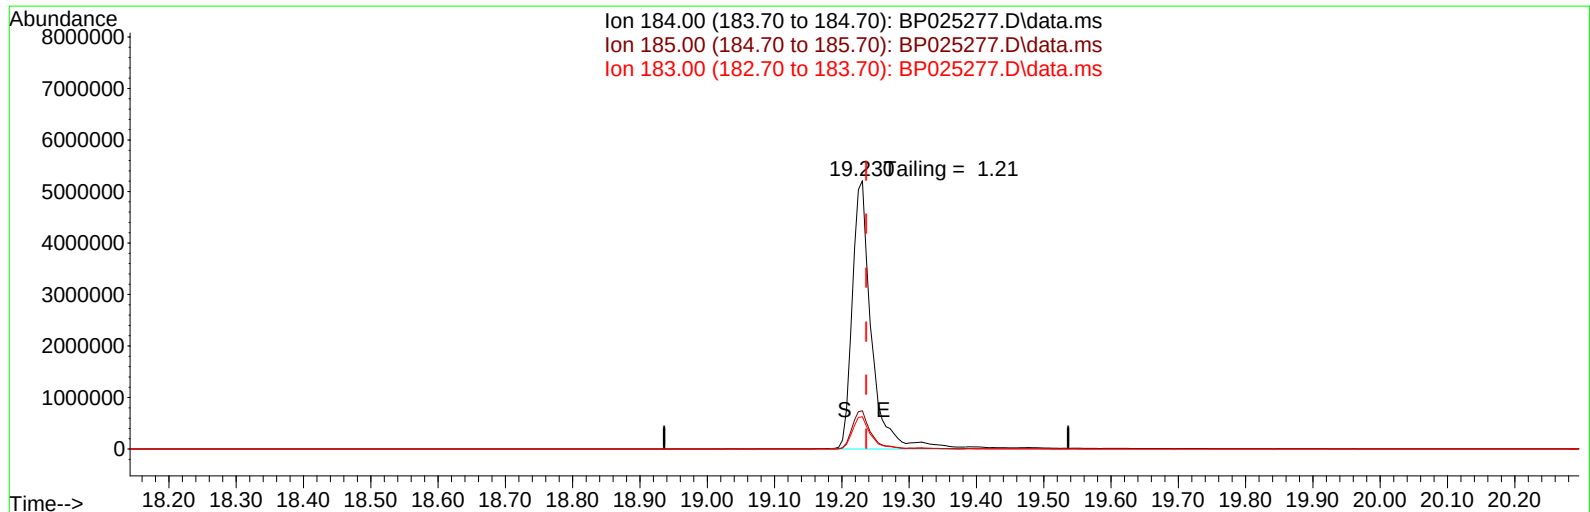

TIC: BP025277.D\data.ms

(77) Benzidine**19.230min (-0.006) 1350357.33 ng****response 9908321**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	12.00	12.05
0.00	0.00	0.00