
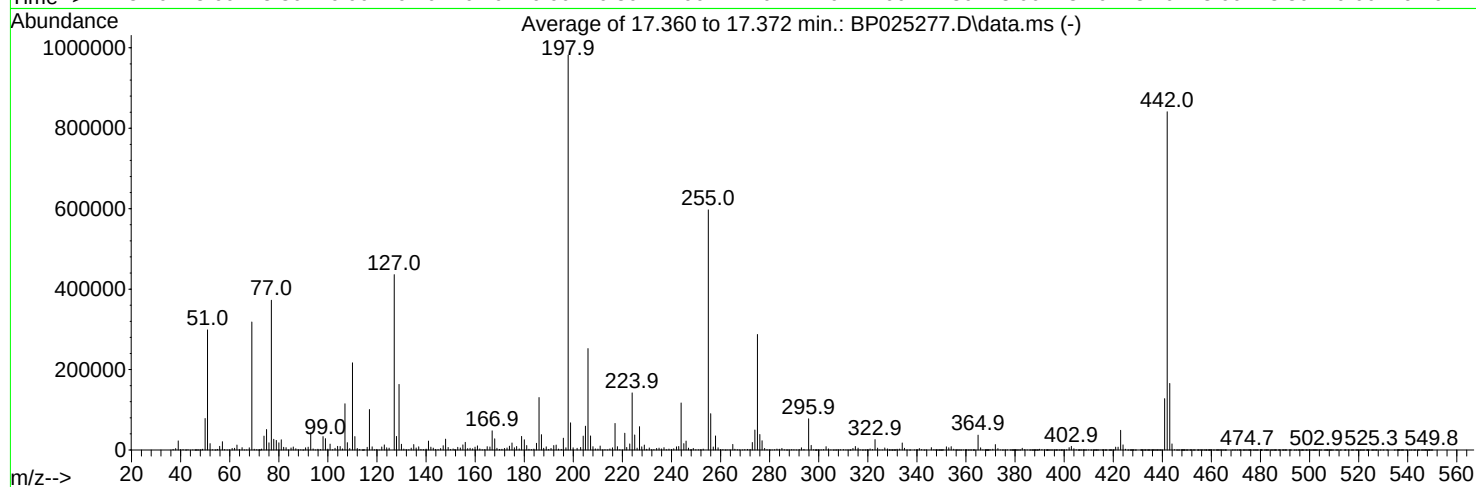


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073125\
Data File : BP025277.D
Acq On : 31 Jul 2025 11:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 29 15:28:11 2025

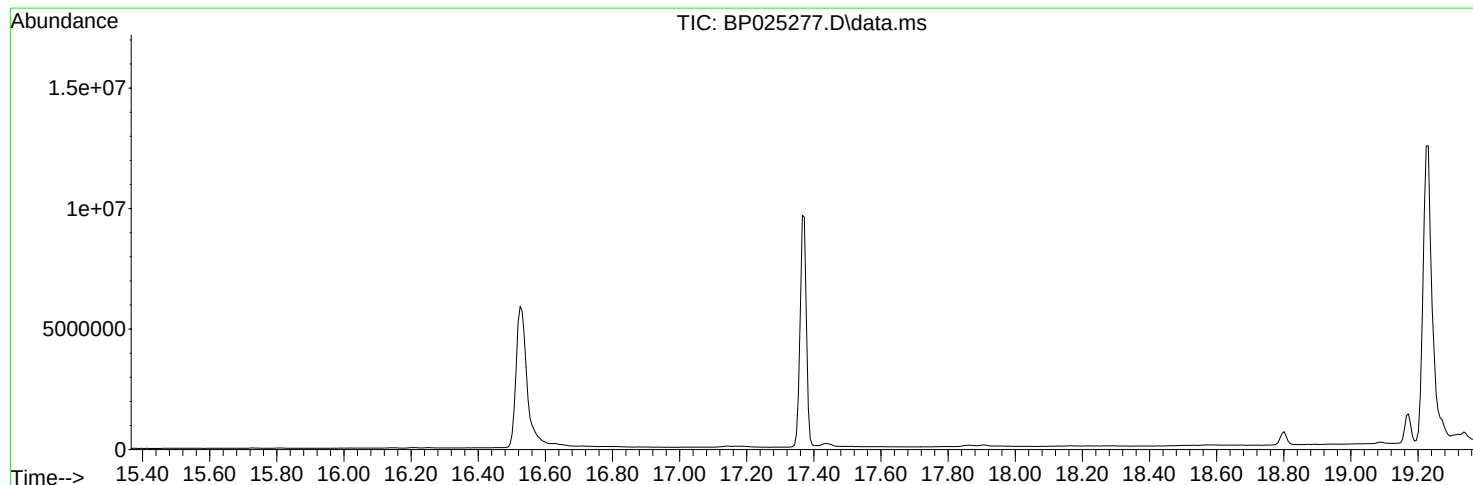




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5440	PASS
69	69	100	100	100.0	318472	PASS
70	69	0.00	2	0.6	1904	PASS
197	198	0.00	2	0.6	5448	PASS
198	198	100	100	100.0	981720	PASS
199	198	5	9	6.9	67864	PASS
365	198	1	100	3.8	36888	PASS
441	443	0.01	150	77.2	127711	PASS
442	442	100	100	100.0	841118	PASS
443	442	15	24	19.7	165493	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073125\
Data File : BP025277.D
Acq On : 31 Jul 2025 11:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 31 12:50:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

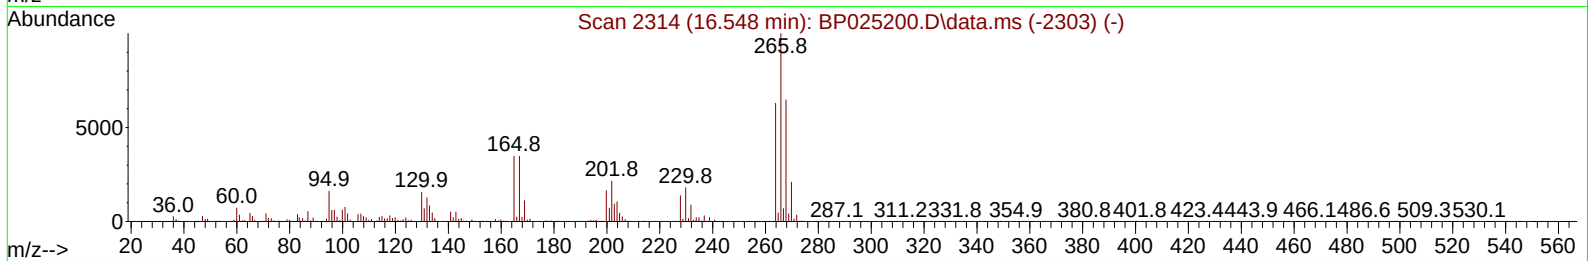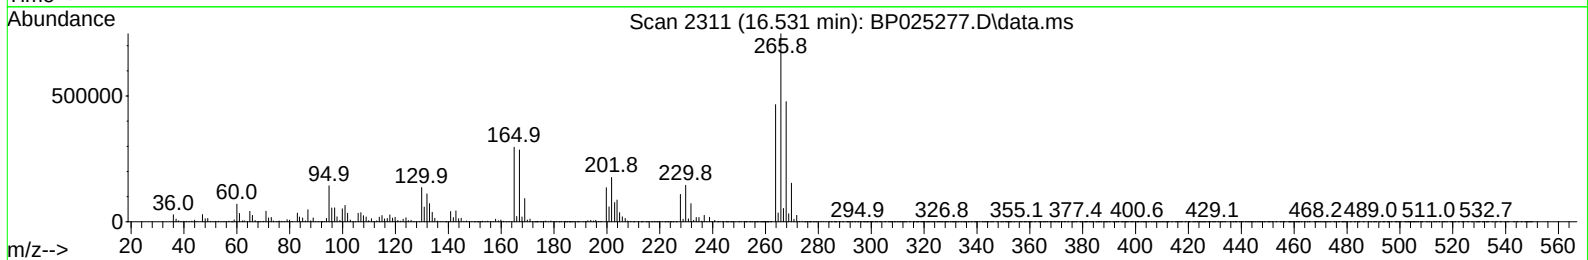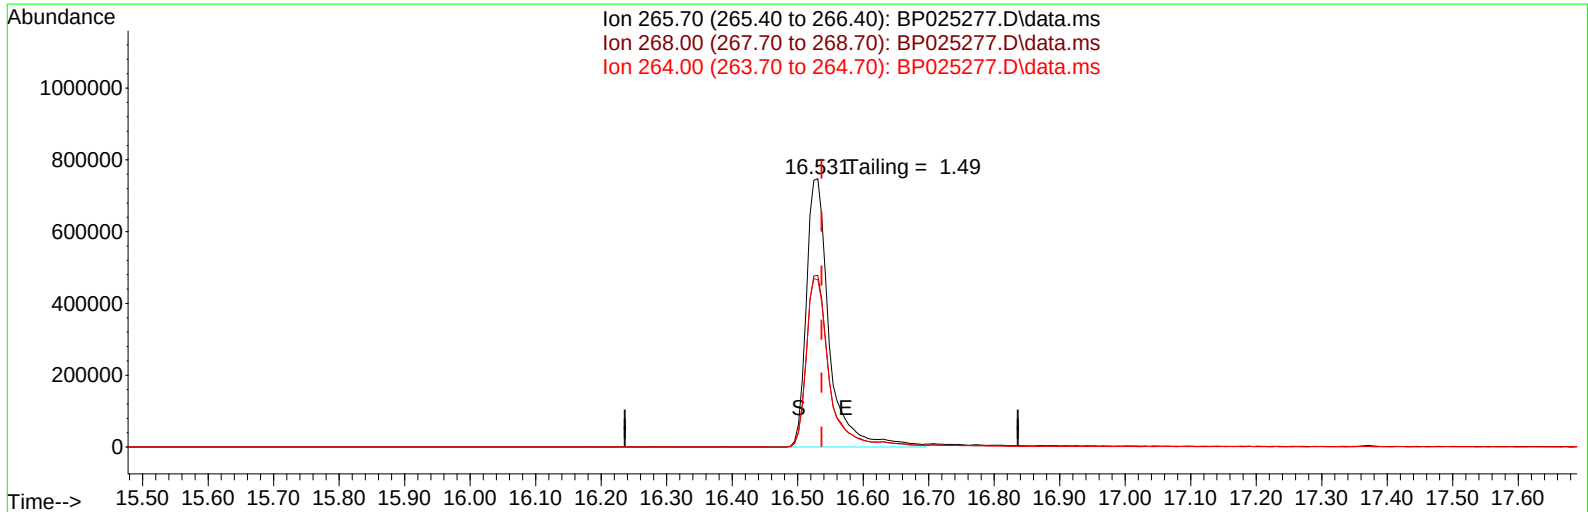

TIC: BP025277.D\data.ms

(70) Pentachlorophenol (C)

16.531min (-0.006) 146742.07 ng




response 1813117

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.94
264.00	62.90	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073125\
Data File : BP025277.D
Acq On : 31 Jul 2025 11:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 31 12:50:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

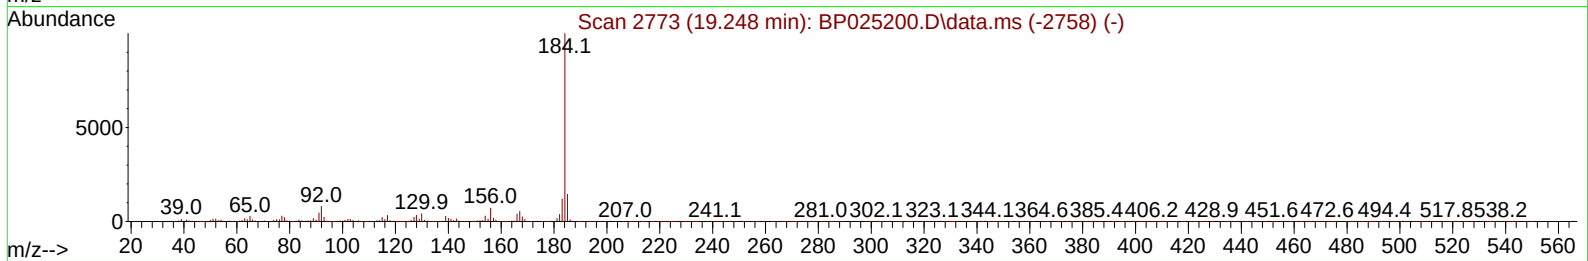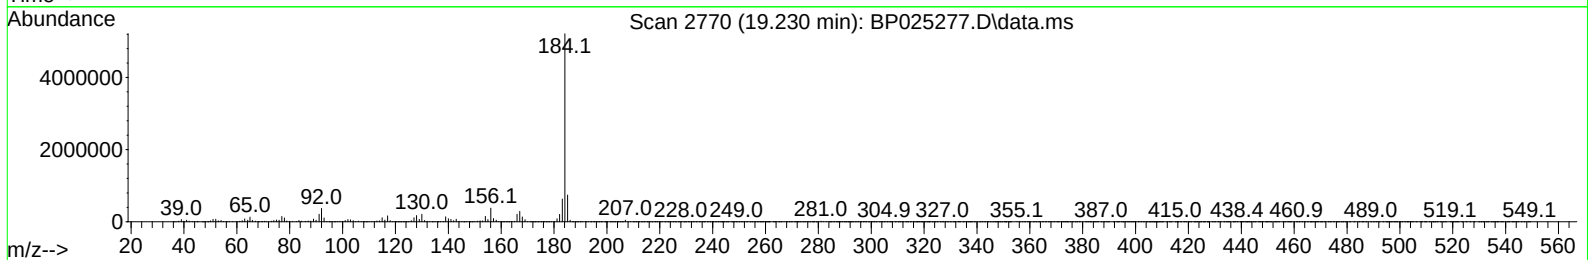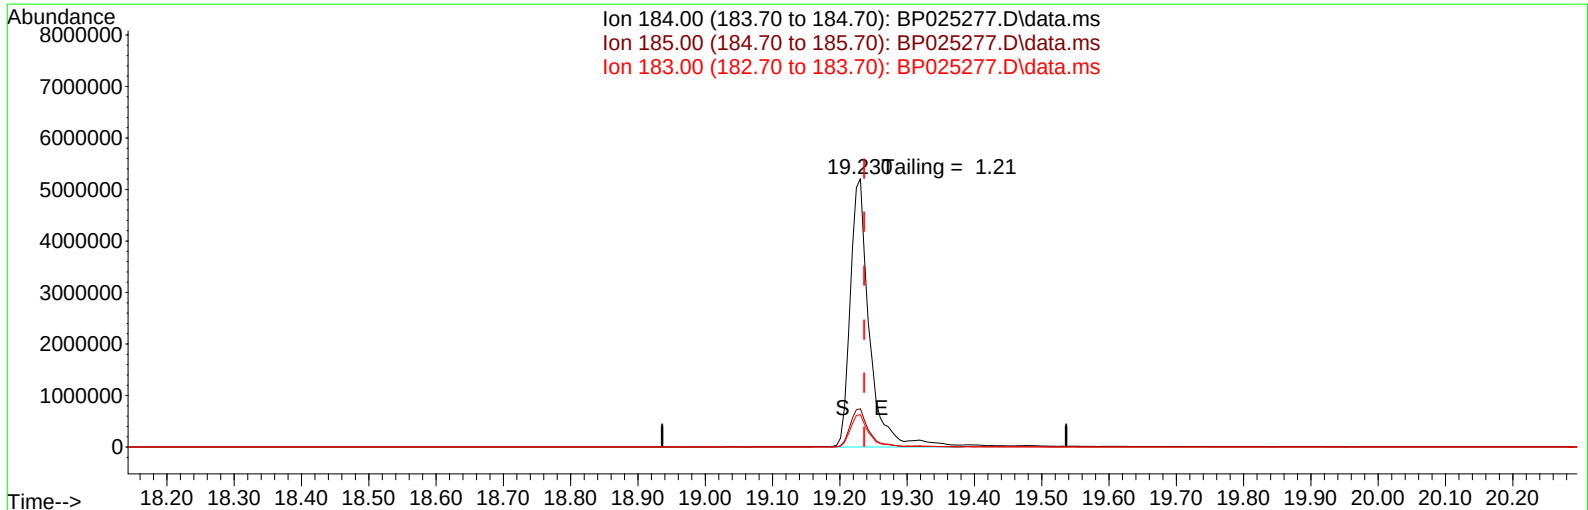

TIC: BP025277.D\data.ms

(77) Benzidine

19.230min (-0.006) 1350357.33 ng

response 9908321

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	12.00	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2025	BNA_P	<u>BP025277.D</u>
Compound Name	Response	Retention Time
DDT	4251823	20.525
DDD	86881	20.06
DDE	6668	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
93549	4345372	2.15

Instrument :
BNA_P
ClientSampleId :
DFTPP