
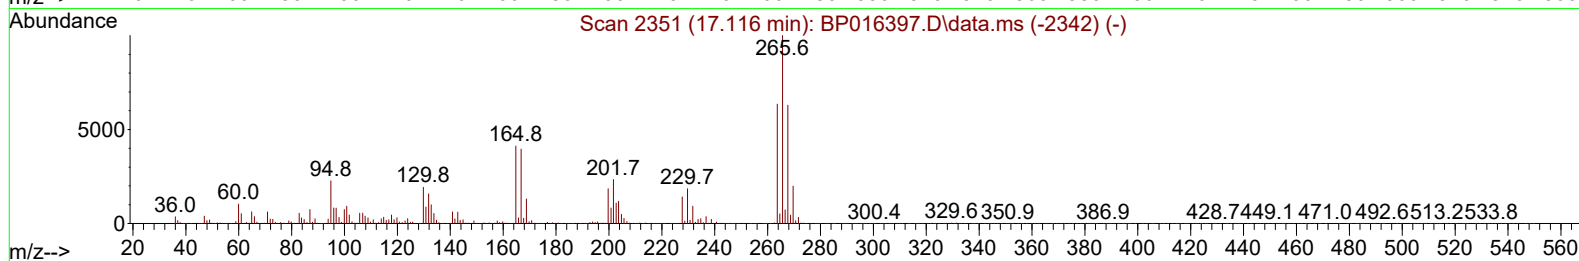
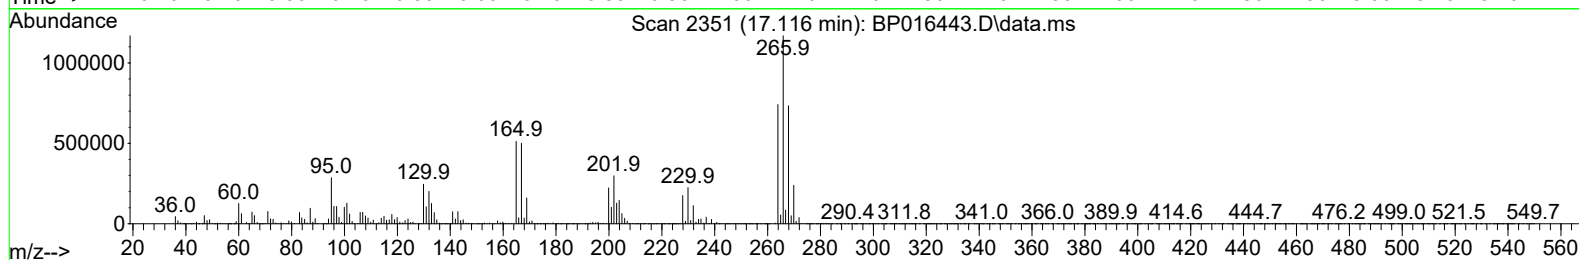


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016443.D
Acq On : 01 Aug 2023 07:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 05:55:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

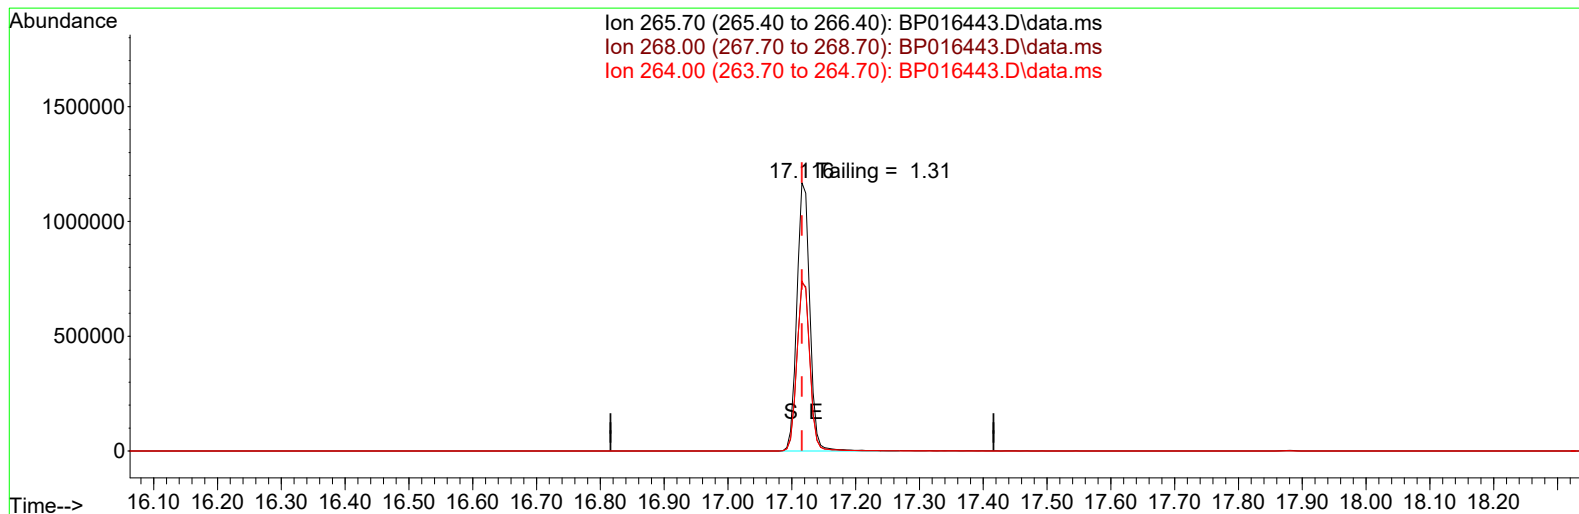

TIC: BP016443.D\data.ms

(70) Pentachlorophenol (C)




17.116min (-0.000) 329825.30 ng

response 1657549

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	62.74
264.00	68.60	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016443.D
Acq On : 01 Aug 2023 07:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 05:55:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

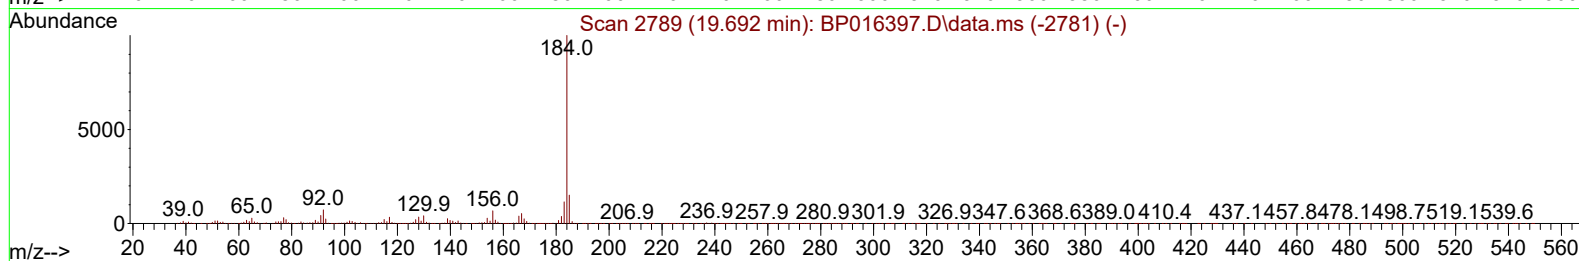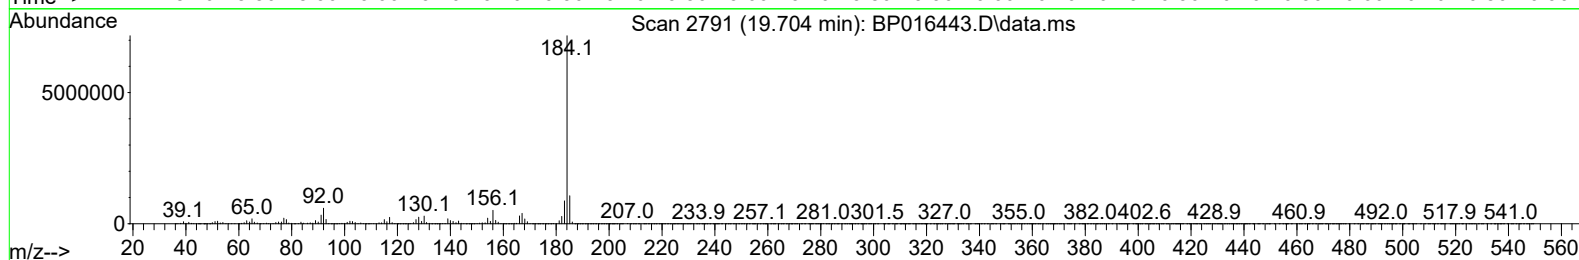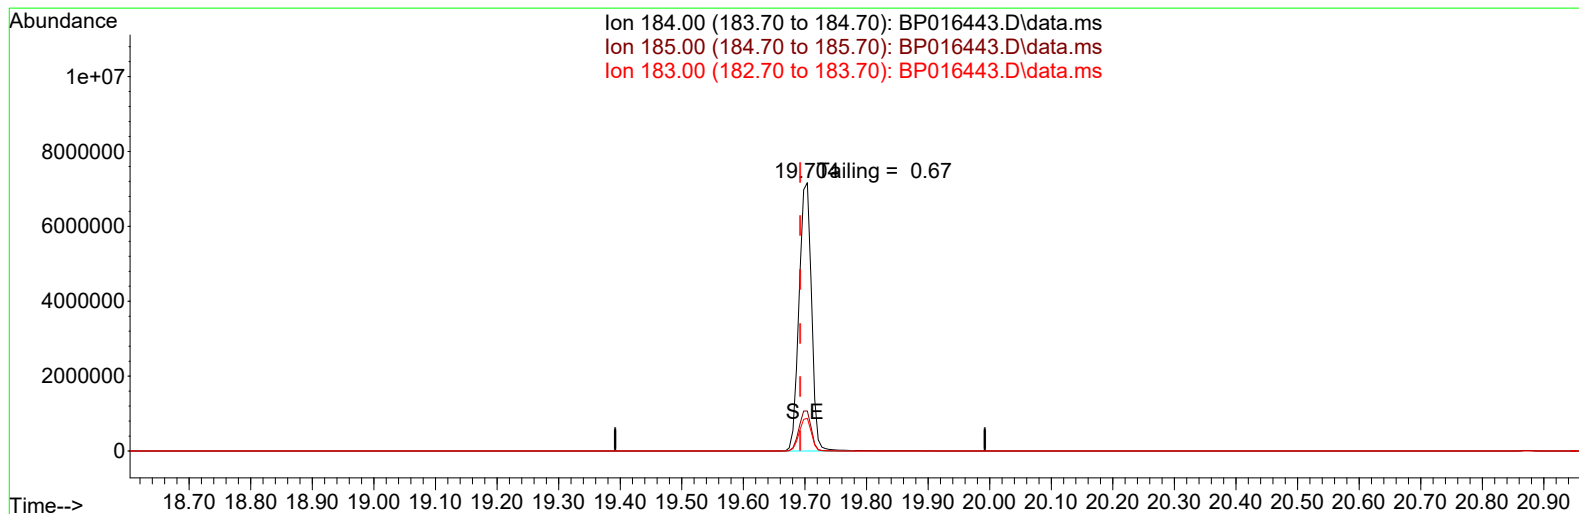

TIC: BP016443.D\data.ms

(77) Benzidine**19.704min (+ 0.012) 468872.07 ng****response 10096428**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.90
183.00	11.50	12.21
0.00	0.00	0.00