

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
 Data File : BP016452.D
 Acq On : 01 Aug 2023 12:47
 Operator : MA/JU
 Sample : 03686-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-21-16-18-20230719

Quant Time: Aug 01 15:52:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 01:48:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	428618	20.000	ng	-0.01
21) Naphthalene-d8	10.910	136	1868534	20.000	ng	-0.02
39) Acenaphthene-d10	14.728	164	1151589	20.000	ng	0.00
64) Phenanthrene-d10	17.492	188	2477462	20.000	ng	0.00
76) Chrysene-d12	21.592	240	1816989	20.000	ng	0.00
86) Perylene-d12	24.186	264	1749009	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.593	112	4455415	169.583	ng	-0.01
7) Phenol-d6	7.216	99	5923585	164.492	ng	-0.01
23) Nitrobenzene-d5	9.275	82	3554847	106.498	ng	-0.02
42) 2,4,6-Tribromophenol	16.222	330	1617474	95.474	ng	0.00
45) 2-Fluorobiphenyl	13.351	172	8040577	100.101	ng	-0.01
79) Terphenyl-d14	20.045	244	11351760	131.975	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016452.D
Acq On : 01 Aug 2023 12:47
Operator : MA/JU
Sample : 03686-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-21-16-18-20230719

Quant Time: Aug 01 15:52:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration




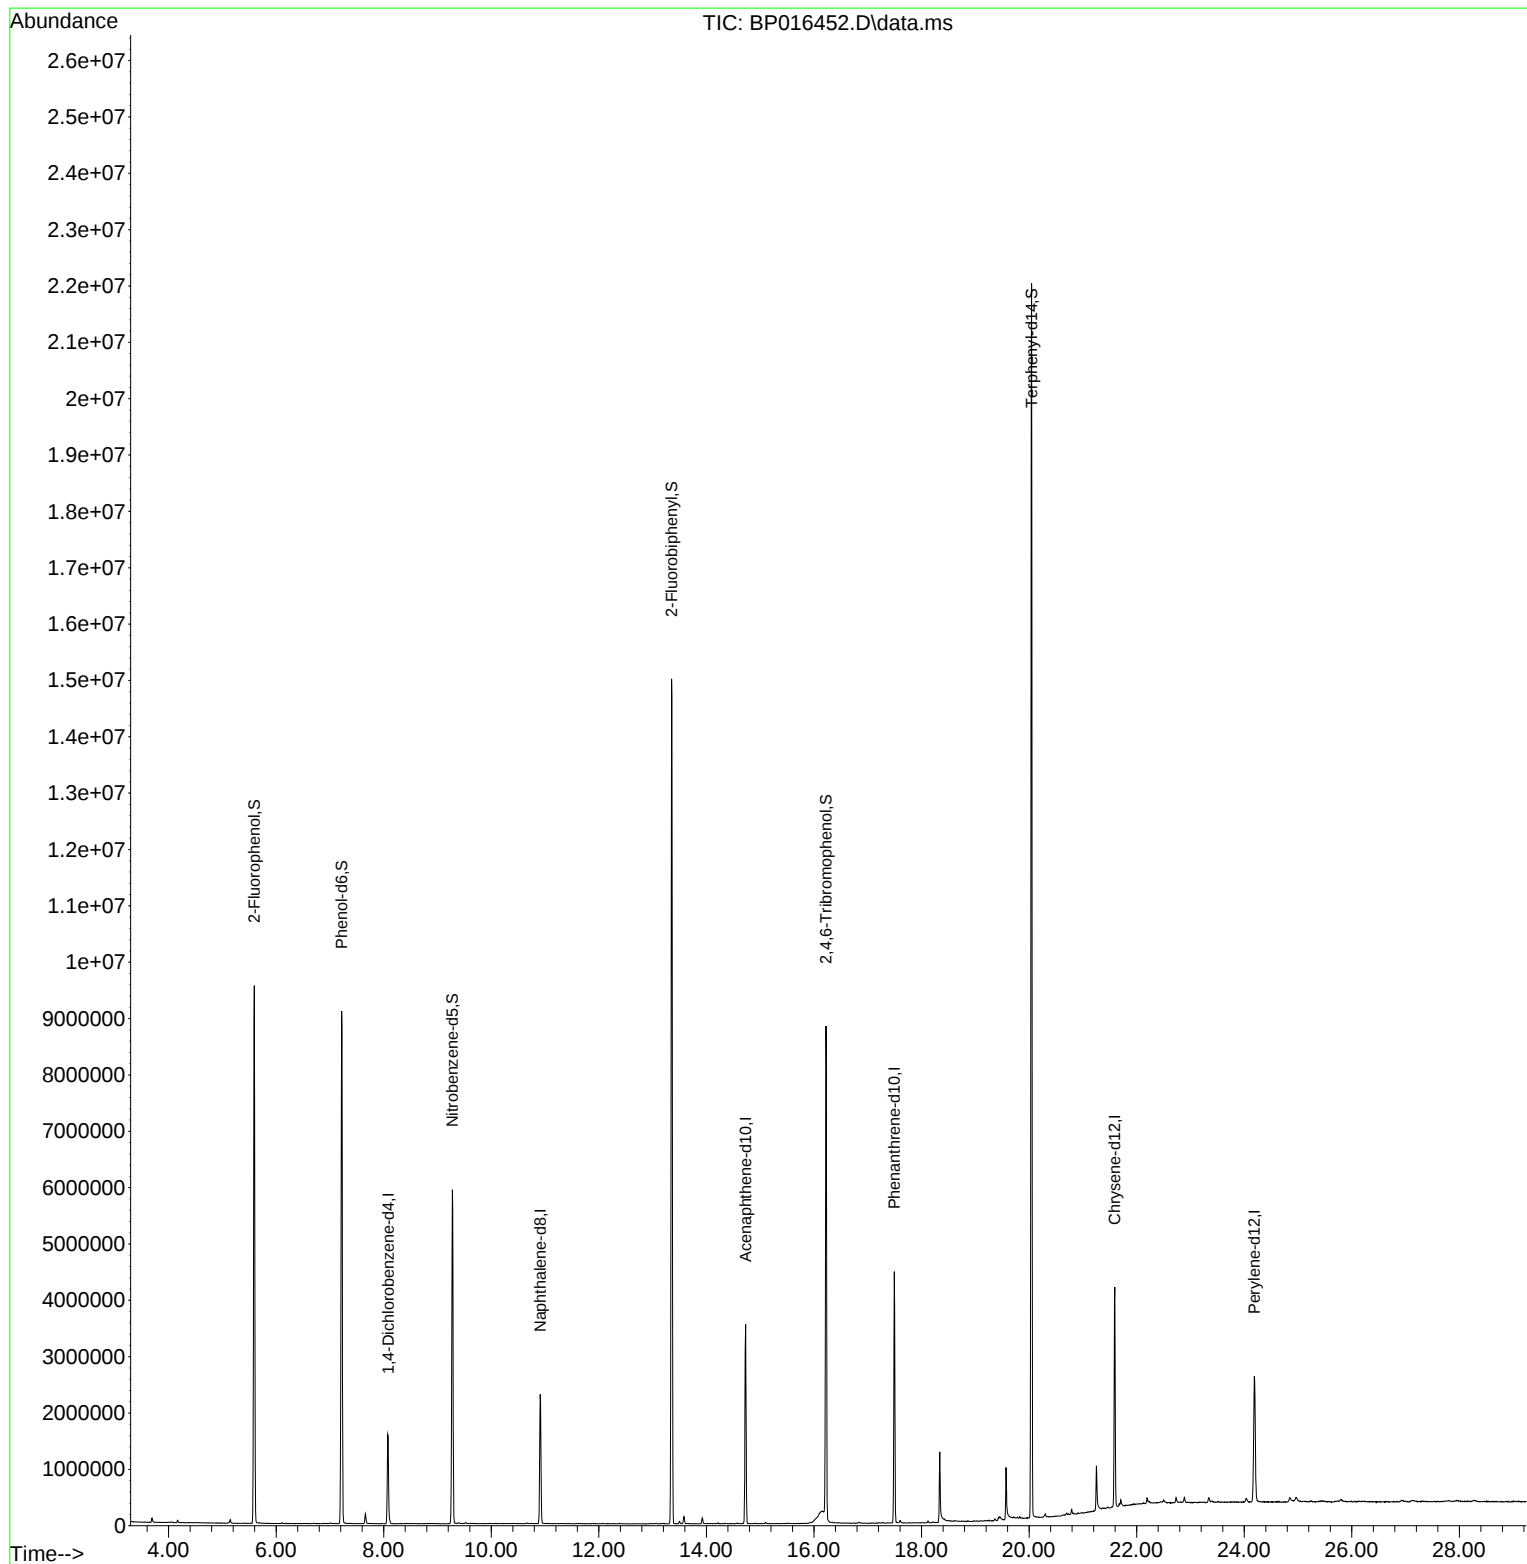




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.081 min Scan# 817
Delta R.T. -0.012 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47




Instrument :
BNA_P
ClientSampleId :
SB-21-16-18-20230719


Tgt Ion:152 Resp: 428618
Ion Ratio Lower Upper
152 100
150 155.7 124.9 187.3
115 59.3 46.8 70.2

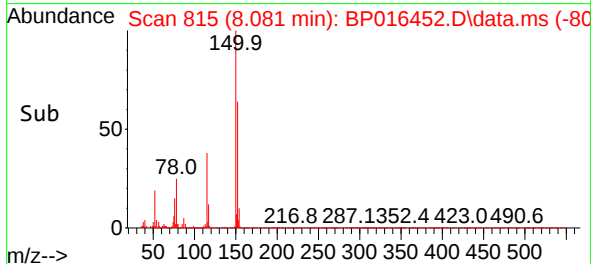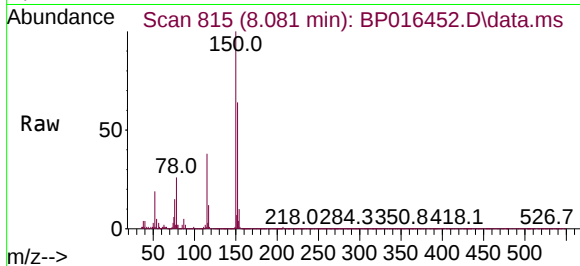

#5
2-Fluorophenol
Concen: 169.583 ng
RT: 5.593 min Scan# 392
Delta R.T. -0.012 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47

Tgt Ion:112 Resp: 4455415
Ion Ratio Lower Upper
112 100
64 50.8 40.0 60.0
63 26.3 21.2 31.8


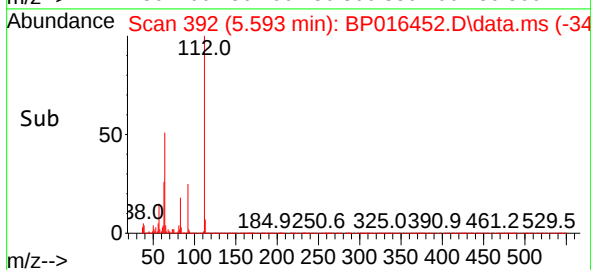

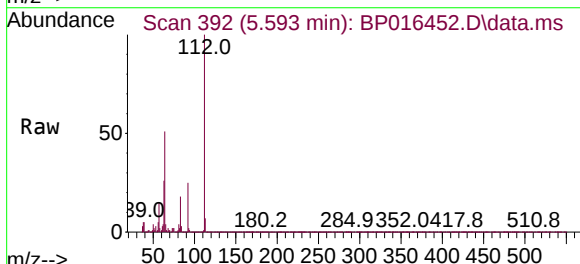


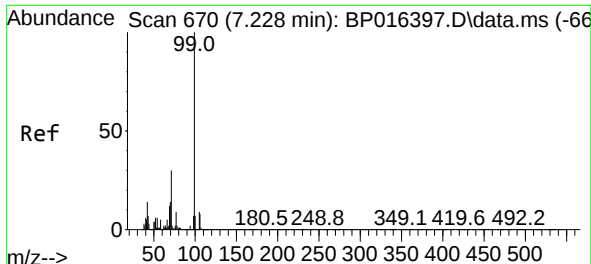

#7
Phenol-d6
Concen: 164.492 ng
RT: 7.216 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47




Instrument :
BNA_P
ClientSampleId :
SB-21-16-18-20230719


Tgt Ion: 99 Resp: 5923585
Ion Ratio Lower Upper
99 100
42 14.2 11.6 17.4
71 30.4 24.3 36.5

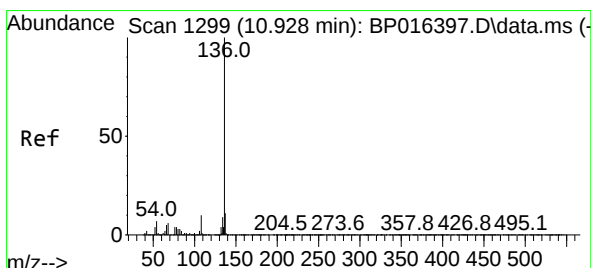

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.910 min Scan# 1296
Delta R.T. -0.018 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47

Tgt Ion:136 Resp: 1868534
Ion Ratio Lower Upper
136 100
137 11.2 8.6 13.0
54 7.2 5.6 8.4
68 6.2 4.6 6.8


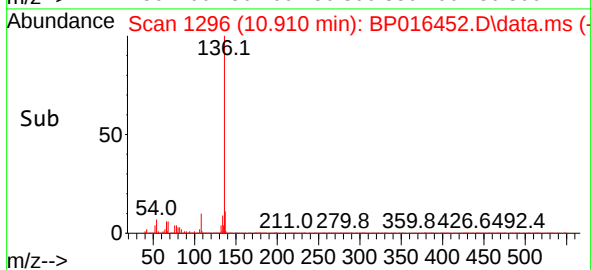

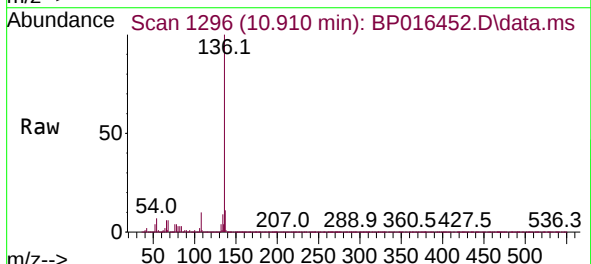




#23
Nitrobenzene-d5
Concen: 106.498 ng
RT: 9.275 min Scan# 1018
Delta R.T. -0.018 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47




Instrument :
BNA_P
ClientSampleId :
SB-21-16-18-20230719


Tgt Ion: 82 Resp: 3554847
Ion Ratio Lower Upper
82 100
128 44.5 36.6 55.0
54 43.4 34.5 51.7

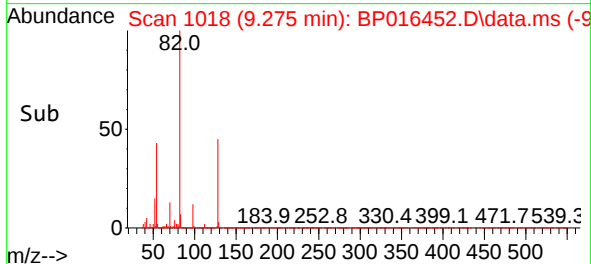

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.728 min Scan# 1945
Delta R.T. -0.006 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47

Tgt Ion: 164 Resp: 1151589
Ion Ratio Lower Upper
164 100
162 100.2 81.0 121.6
160 45.1 36.6 55.0


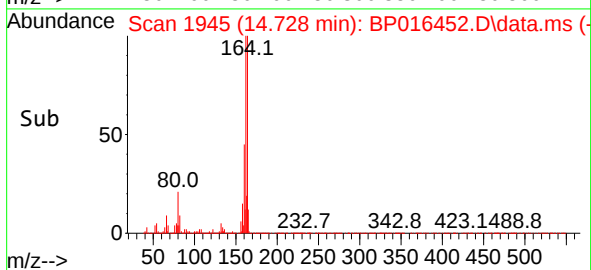

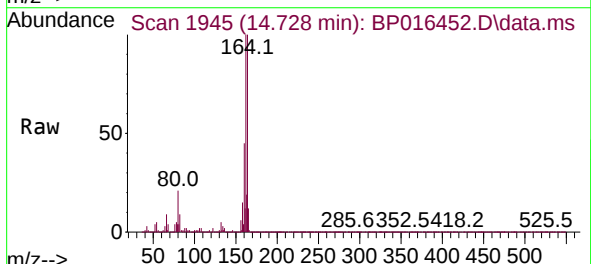




#42
2,4,6-Tribromophenol
Concen: 95.474 ng
RT: 16.222 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47




Instrument :
BNA_P
ClientSampleId :
SB-21-16-18-20230719


Tgt Ion:330 Resp: 1617474
Ion Ratio Lower Upper
330 100
332 96.8 77.8 116.8
141 33.9 22.6 34.0

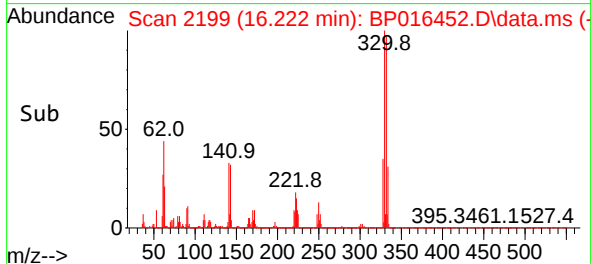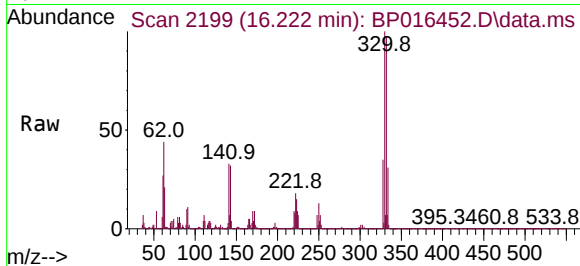

#45
2-Fluorobiphenyl
Concen: 100.101 ng
RT: 13.351 min Scan# 1711
Delta R.T. -0.012 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47

Tgt Ion:172 Resp: 8040577
Ion Ratio Lower Upper
172 100
171 35.7 28.2 42.2
170 24.1 19.1 28.7


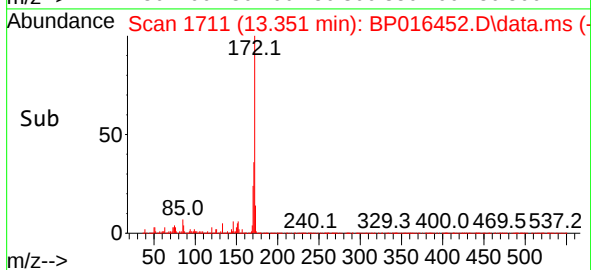

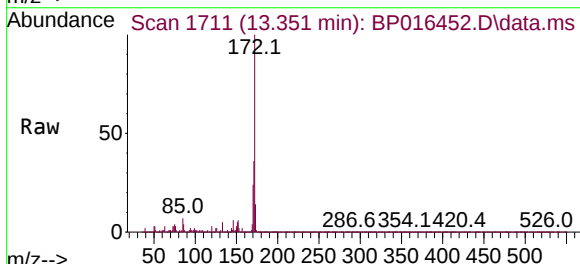


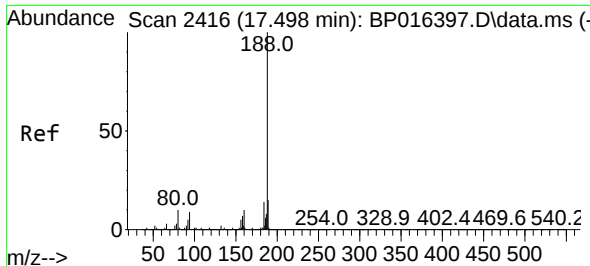

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.492 min Scan# 2416
Delta R.T. -0.006 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47




Instrument :
BNA_P
ClientSampleId :
SB-21-16-18-20230719


Tgt Ion:188 Resp: 2477462
Ion Ratio Lower Upper
188 100
94 10.2 7.4 11.0
80 10.9 7.8 11.8

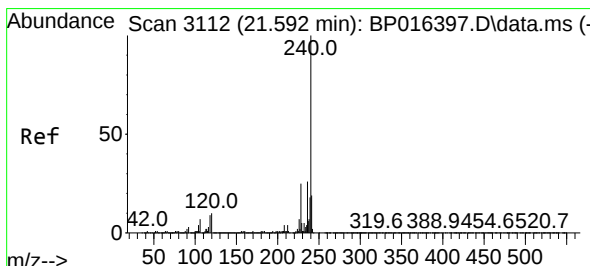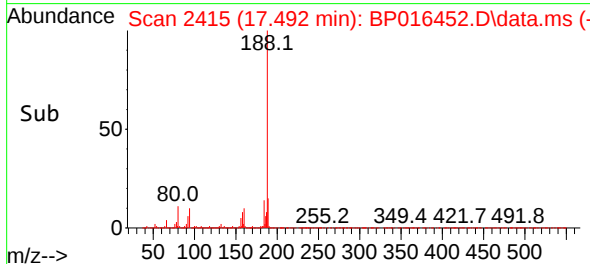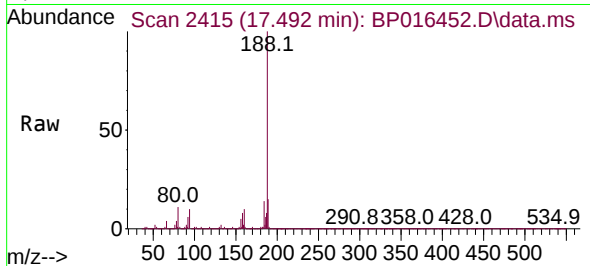

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.592 min Scan# 3112
Delta R.T. -0.000 min
Lab File: BP016452.D
Acq: 01 Aug 2023 12:47

Tgt Ion:240 Resp: 1816989
Ion Ratio Lower Upper
240 100
120 11.4 7.9 11.9
236 26.1 21.1 31.7

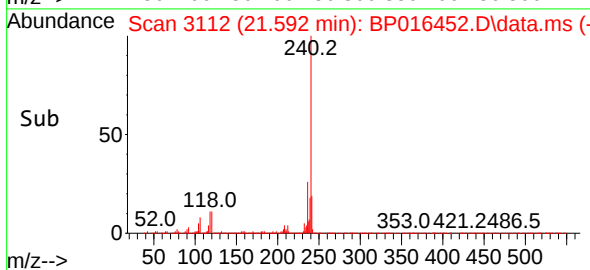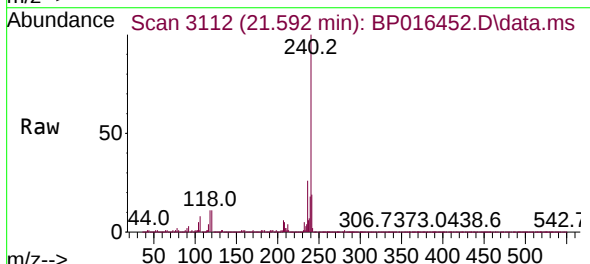

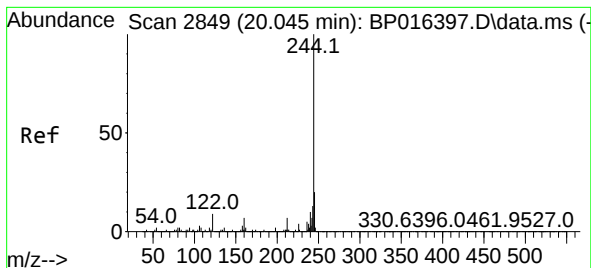

#79

Terphenyl-d14

Concen: 131.975 ng

RT: 20.045 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP016452.D

Acq: 01 Aug 2023 12:47

Instrument :

BNA_P

ClientSampleId :

SB-21-16-18-20230719





Tgt Ion:244 Resp:11351760

Ion Ratio Lower Upper

244 100

212 7.4 5.6 8.4

122 10.6 7.4 11.2

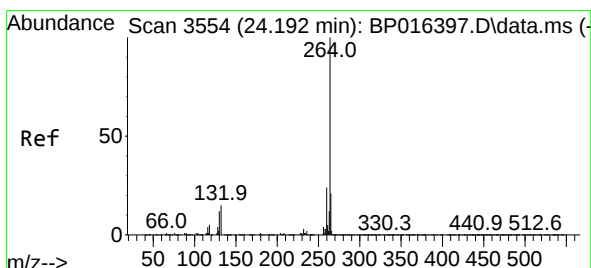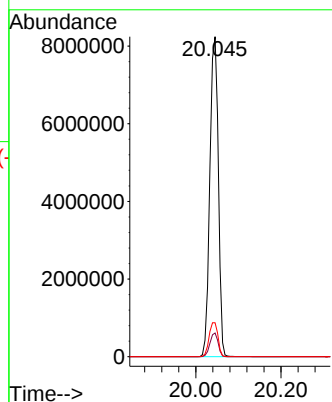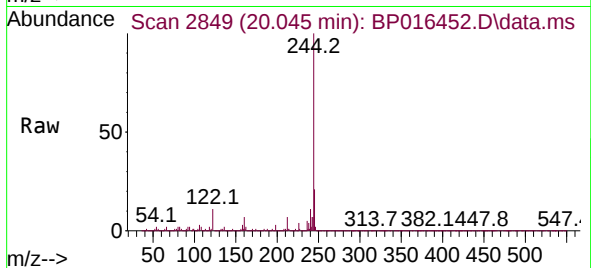

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.186 min Scan# 3553

Delta R.T. -0.006 min

Lab File: BP016452.D

Acq: 01 Aug 2023 12:47

Tgt Ion:264 Resp: 1749009

Ion Ratio Lower Upper

264 100

260 24.1 19.3 28.9

265 22.0 17.4 26.0

