

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
 Data File : BP016445.D
 Acq On : 01 Aug 2023 08:38
 Operator : MA/JU
 Sample : PB154002BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB154002BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.593	384	392	406	rBV	7103714	10593570	39.77%	9.485%
2	7.216	660	668	681	rBV	7140165	11394753	42.78%	10.202%
3	8.075	807	814	824	rVB	1211710	1934809	7.26%	1.732%
4	9.275	1009	1018	1029	rBV	4241802	6856502	25.74%	6.139%
5	10.910	1287	1296	1305	rBV	1797196	2972824	11.16%	2.662%
6	13.351	1702	1711	1722	rBV	11485108	16906092	63.47%	15.137%
7	14.728	1936	1945	1953	rBV	2882263	4101621	15.40%	3.672%
8	16.222	2191	2199	2228	rBV	8617555	12262155	46.04%	10.979%
9	17.492	2408	2415	2425	rBV	3876201	5387955	20.23%	4.824%
10	20.045	2843	2849	2854	rBV	20622052	26634630	100.00%	23.847%
11	21.592	3106	3112	3119	rBV	4598002	6224600	23.37%	5.573%
12	24.192	3546	3554	3566	rVB2	3020355	6419376	24.10%	5.748%




Sum of corrected areas: 111688887

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016445.D
Acq On : 01 Aug 2023 08:38
Operator : MA/JU
Sample : PB154002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154002BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

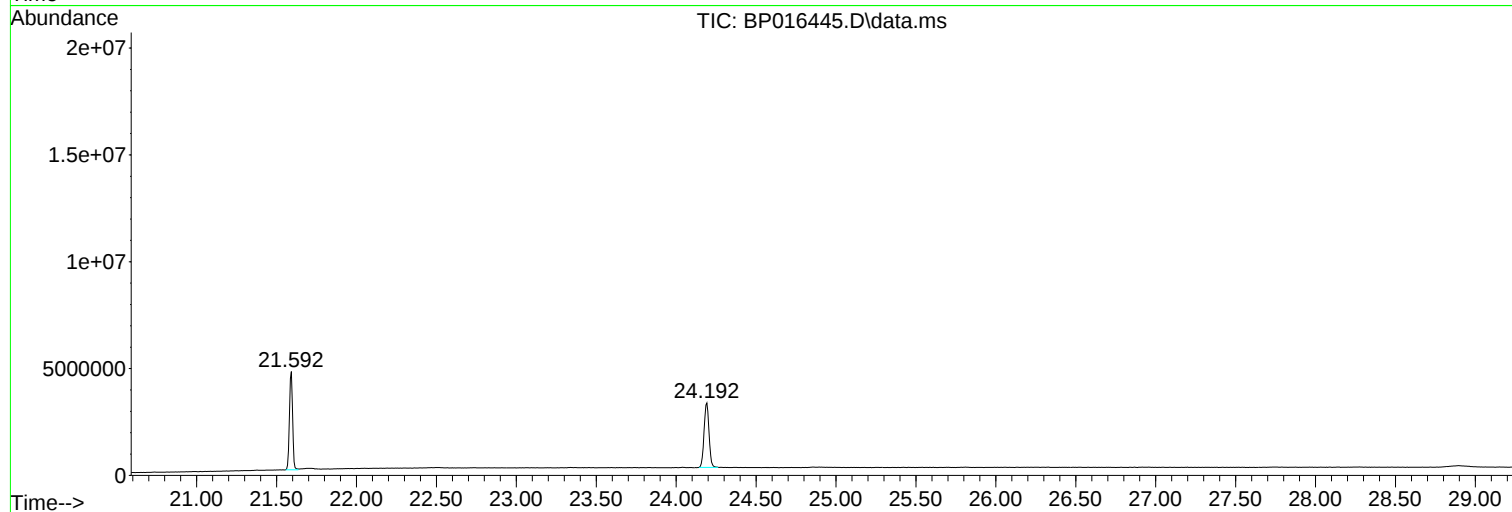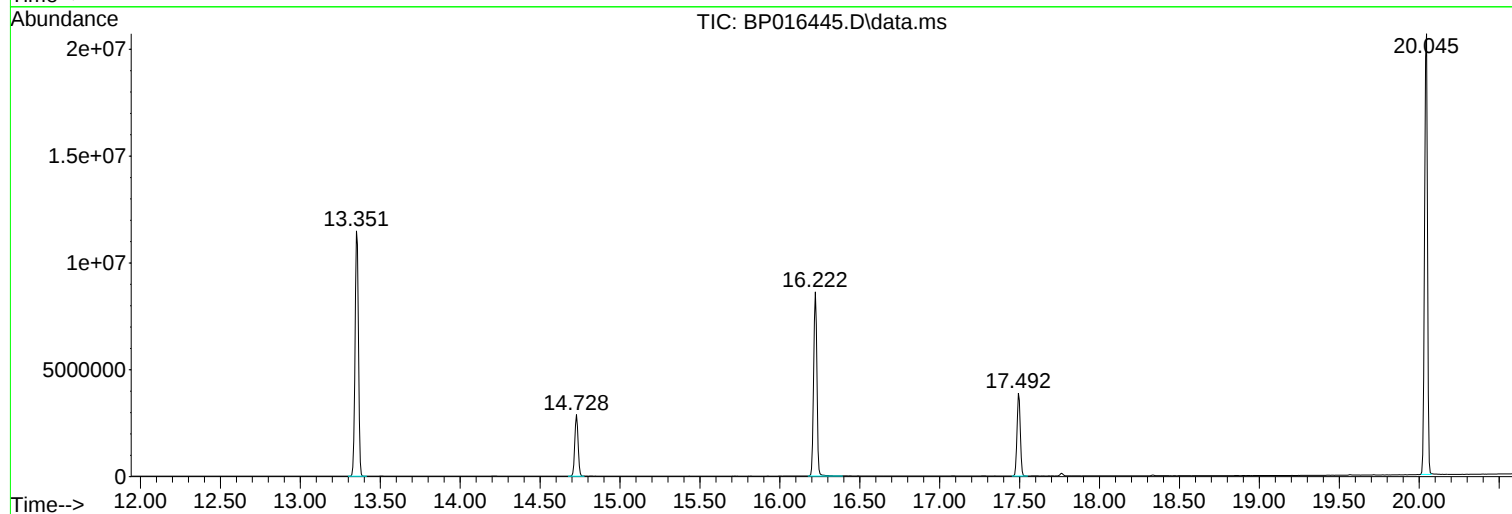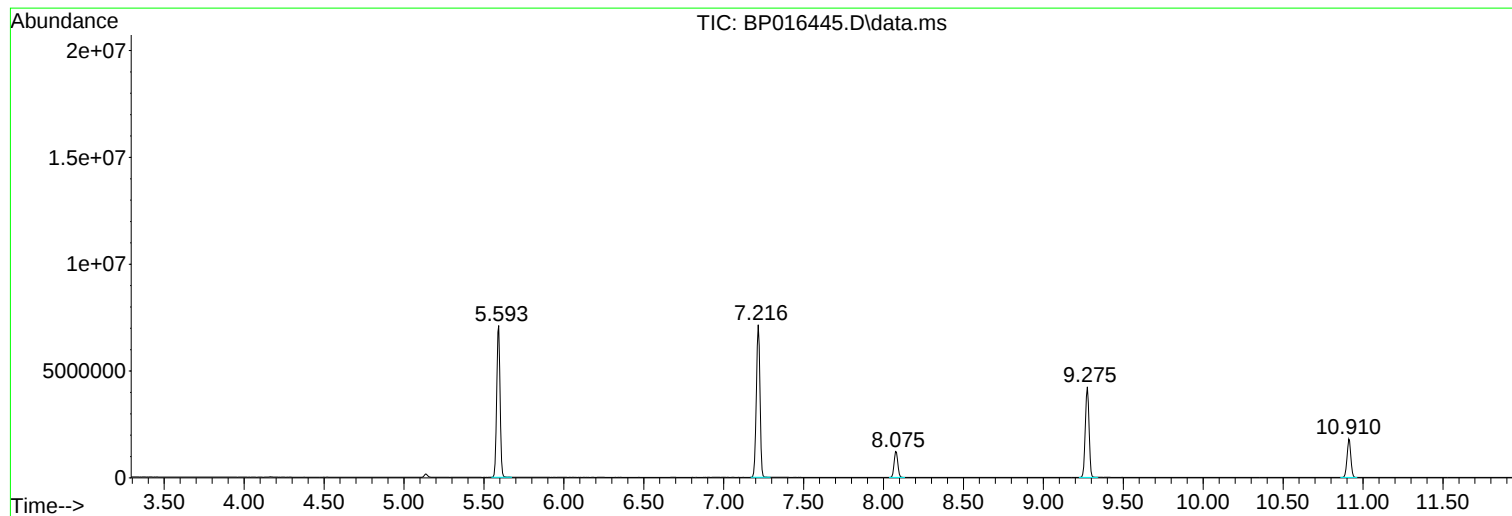

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016445.D
Acq On : 01 Aug 2023 08:38
Operator : MA/JU
Sample : PB154002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154002BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016445.D
Acq On : 01 Aug 2023 08:38
Operator : MA/JU
Sample : PB154002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154002BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------