
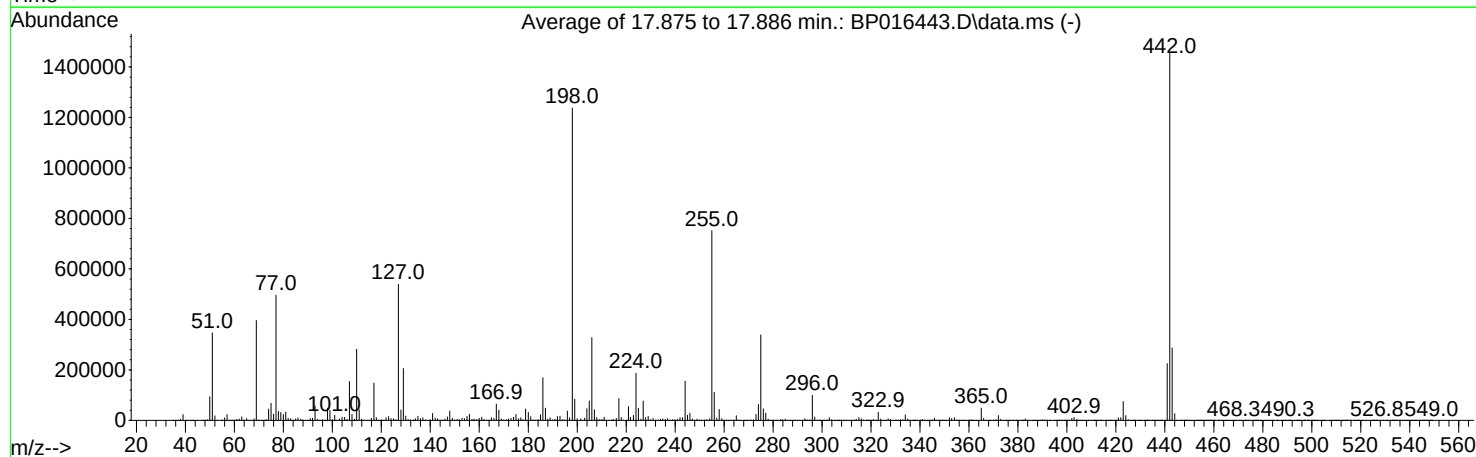


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
 Data File : BP016443.D
 Acq On : 01 Aug 2023 07:31
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 28 01:48:25 2023

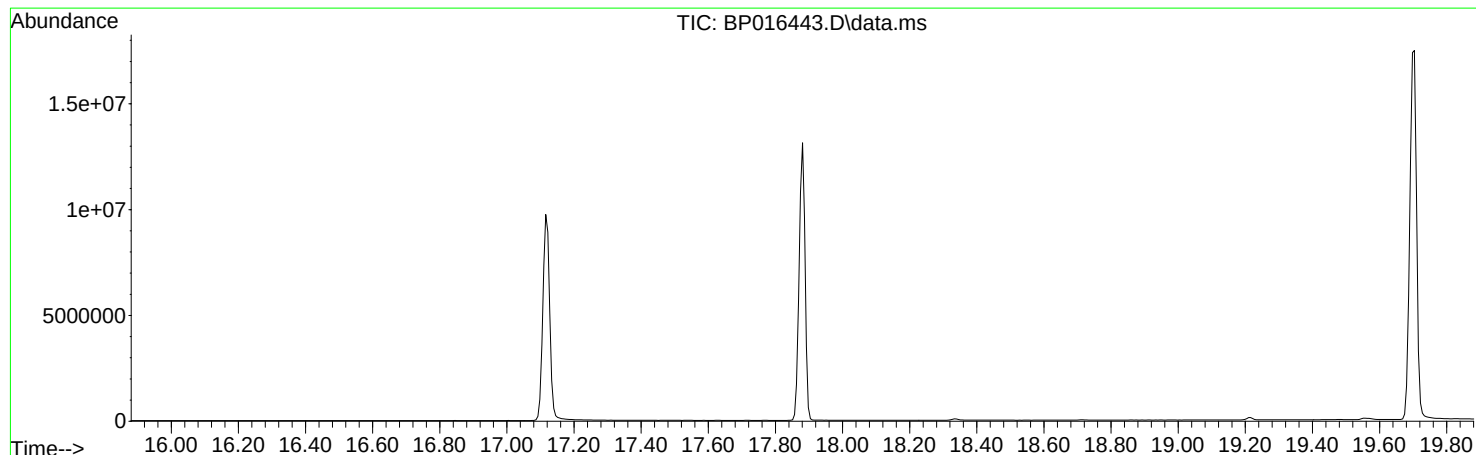

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	346626	PASS
68	69	0.00	2	1.6	6422	PASS
69	198	0.00	100	32.0	395599	PASS
70	69	0.00	2	0.5	1887	PASS
127	198	10	80	43.6	539092	PASS
197	198	0.00	2	0.8	9900	PASS
198	198	100	100	100.0	1237436	PASS
199	198	5	9	6.8	84019	PASS
275	198	10	60	27.4	338491	PASS
365	198	1	100	3.9	48206	PASS
441	198	0.01	100	18.2	225360	PASS
442	442	100	100	100.0	1457323	PASS
443	442	15	24	19.7	287040	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/1/2023	BNA_P	<u>BP016443.D</u>
Compound Name	Response	Retention Time
DDT	4178945	20.874
DDD	57334	20.486
DDE	1804	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
59138	4238083	1.40

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016443.D
Acq On : 01 Aug 2023 07:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 02 05:55:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

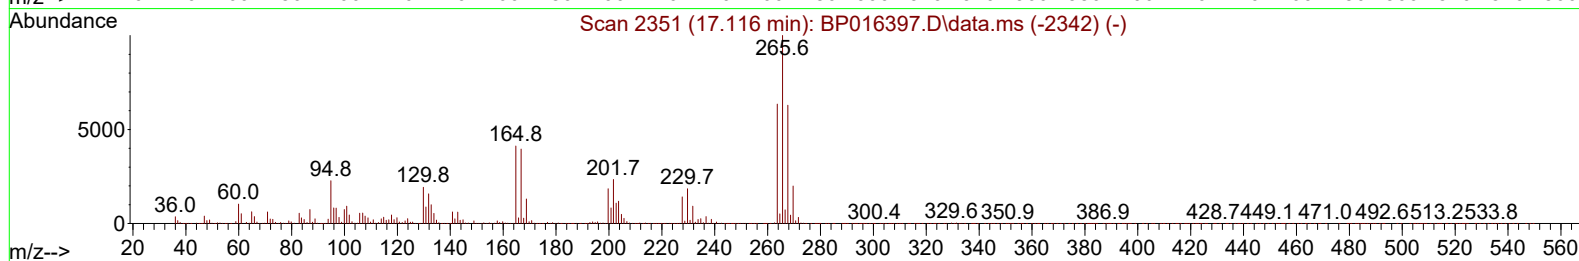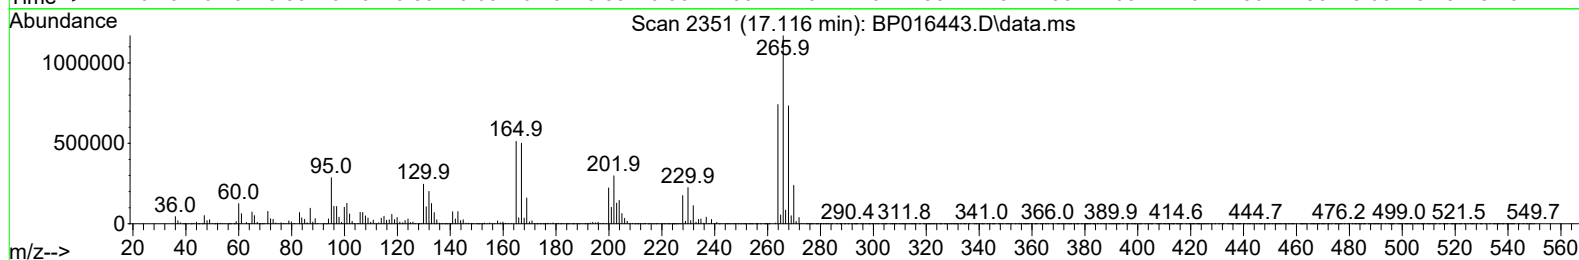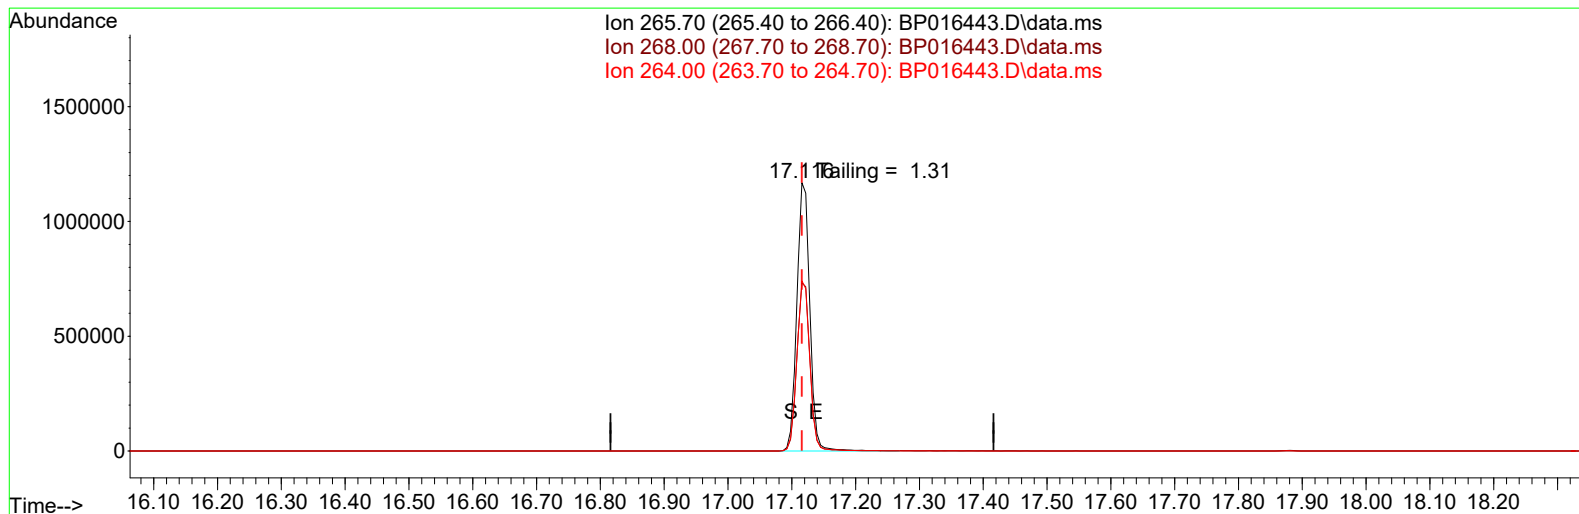

TIC: BP016443.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.000) 329825.30 ng




response 1657549

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	62.74
264.00	68.60	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080123\
Data File : BP016443.D
Acq On : 01 Aug 2023 07:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 02 05:55:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

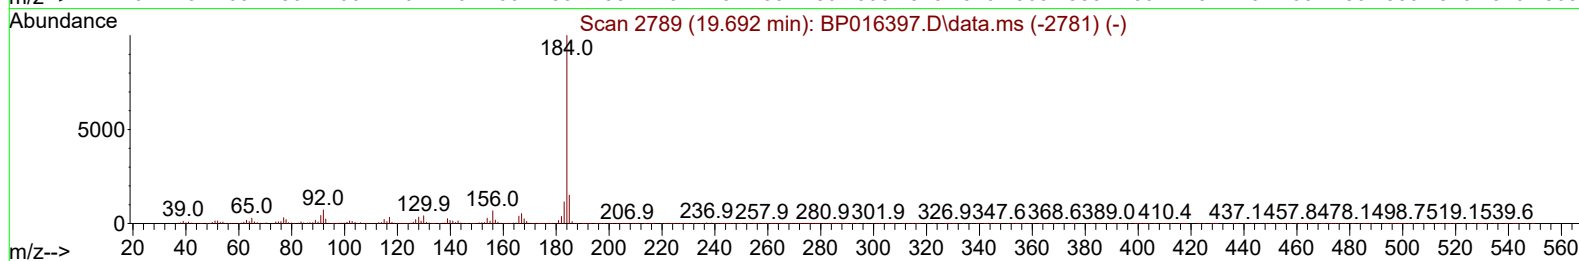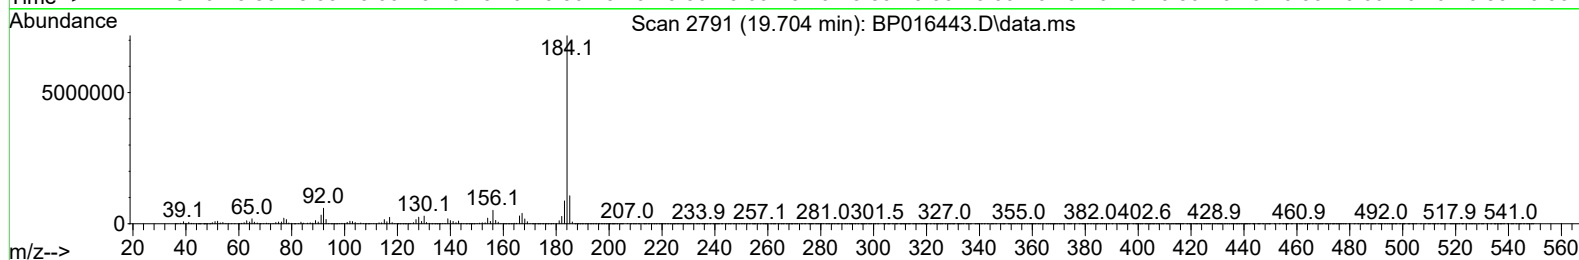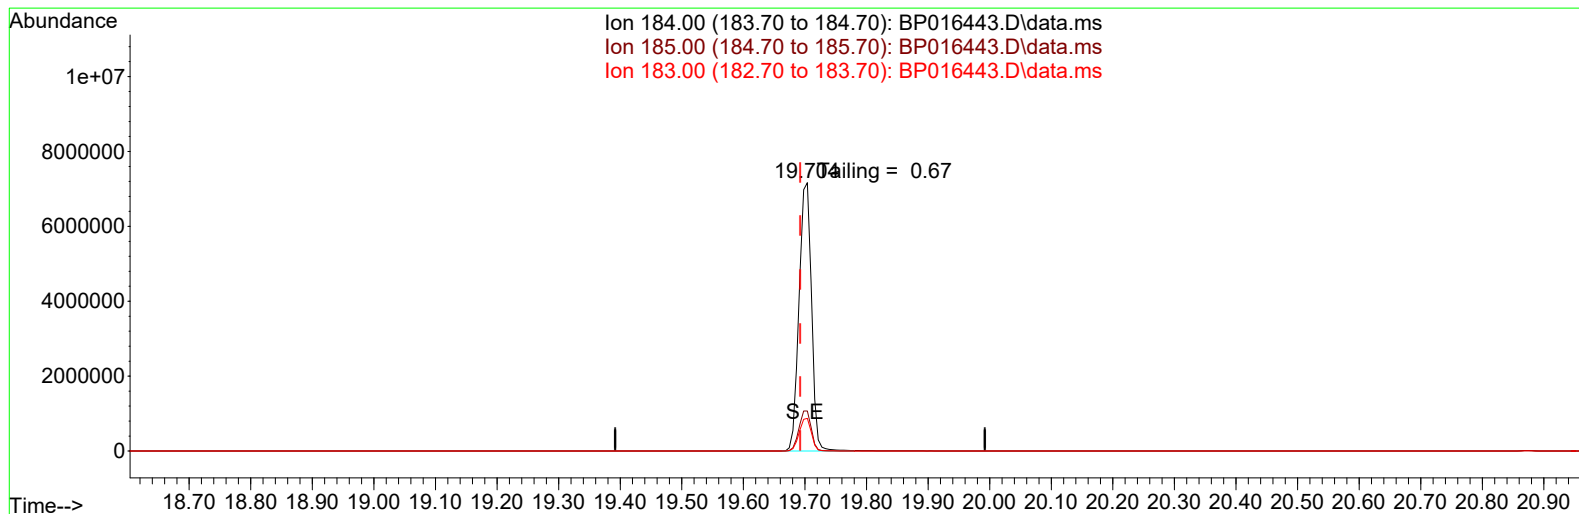

TIC: BP016443.D\data.ms

(77) Benzidine

19.704min (+ 0.012) 468872.07 ng

response 10096428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.90
183.00	11.50	12.21
0.00	0.00	0.00