

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
Data File : BP016465.D
Acq On : 02 Aug 2023 12:59
Operator : MA/JU
Sample : PB154596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154596BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	384	391	400	rBV	8237966	12176417	38.60%	9.193%
2	7.216	659	668	679	rBV	7762876	12645849	40.09%	9.548%
3	8.075	805	814	821	rBV	1736814	2672374	8.47%	2.018%
4	9.269	1009	1017	1026	rBV	4802735	7978927	25.30%	6.024%
5	10.904	1287	1295	1303	rBV	2218288	3753243	11.90%	2.834%
6	13.345	1701	1710	1721	rBV	12975961	19633589	62.25%	14.824%
7	14.722	1937	1944	1954	rBV	3515666	5213967	16.53%	3.937%
8	16.216	2187	2198	2215	rBV	11095615	16777986	53.19%	12.668%
9	17.492	2408	2415	2424	rBV	4794855	6740639	21.37%	5.089%
10	20.039	2842	2848	2853	rBV	24052740	31541661	100.00%	23.815%
11	21.586	3106	3111	3118	rBV	5631045	7353919	23.31%	5.552%
12	24.180	3545	3552	3563	rVB	2783753	5957925	18.89%	4.498%




Sum of corrected areas: 132446496

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
Data File : BP016465.D
Acq On : 02 Aug 2023 12:59
Operator : MA/JU
Sample : PB154596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154596BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

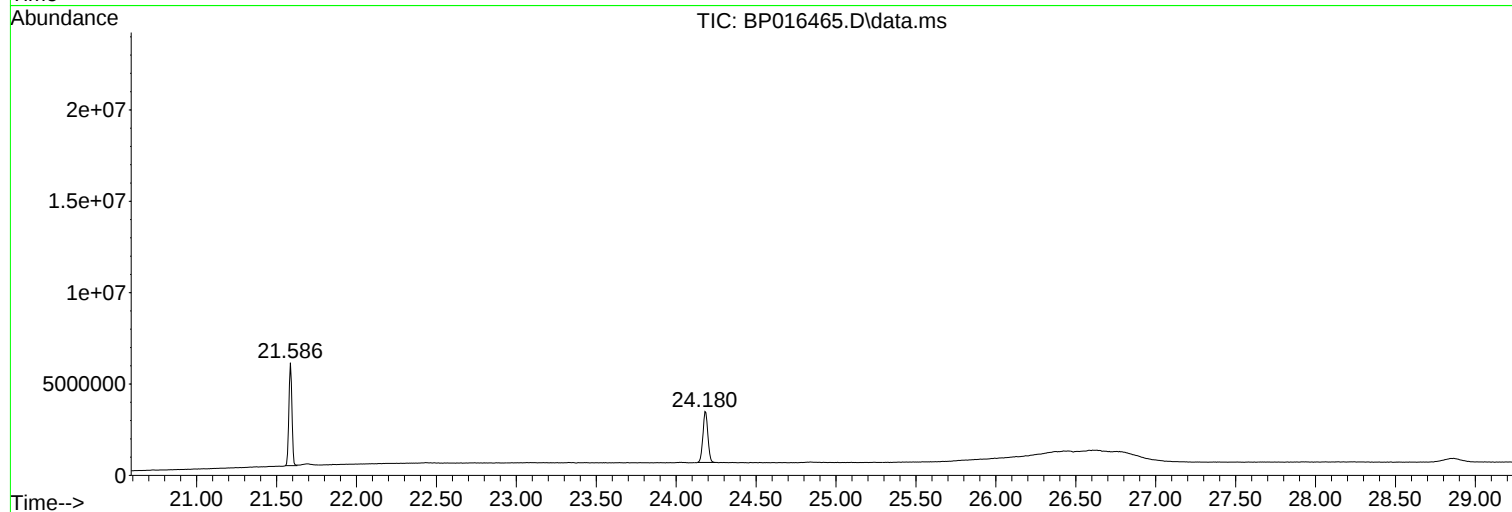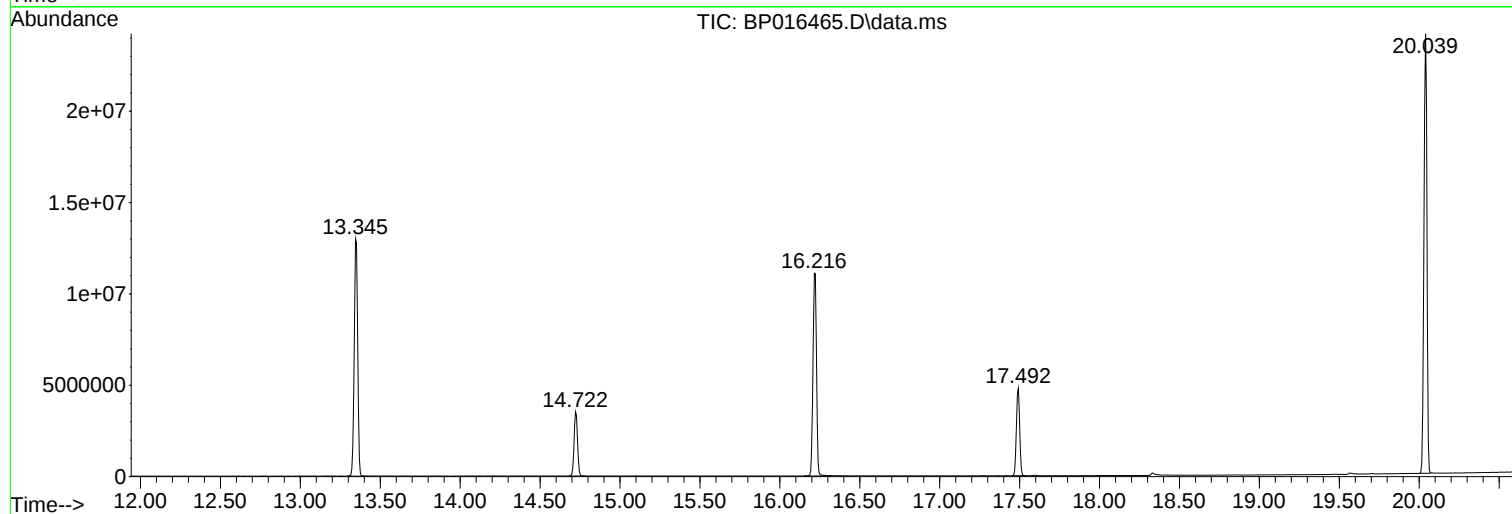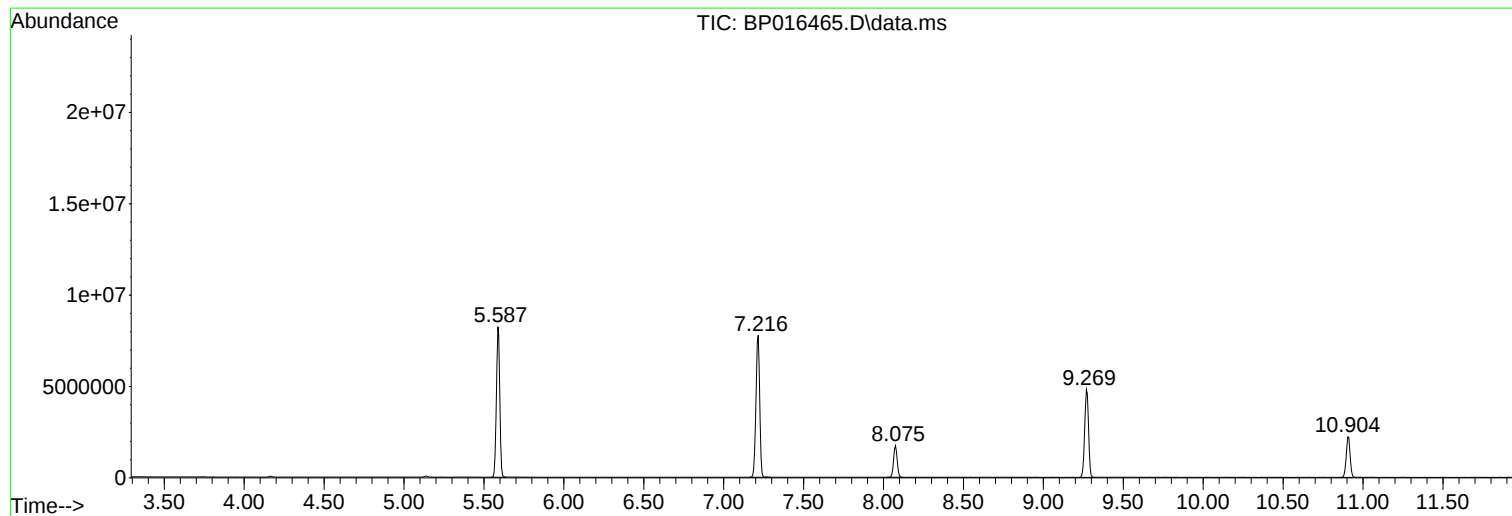

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
Data File : BP016465.D
Acq On : 02 Aug 2023 12:59
Operator : MA/JU
Sample : PB154596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154596BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
Data File : BP016465.D
Acq On : 02 Aug 2023 12:59
Operator : MA/JU
Sample : PB154596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154596BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------