
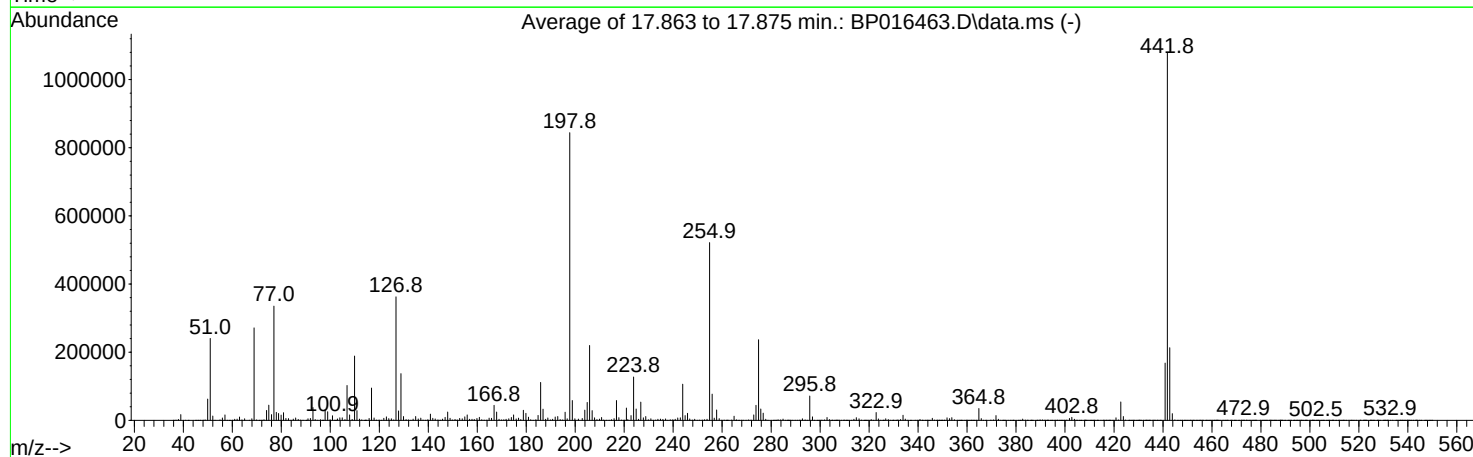


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
 Data File : BP016463.D
 Acq On : 02 Aug 2023 11:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 28 01:48:25 2023

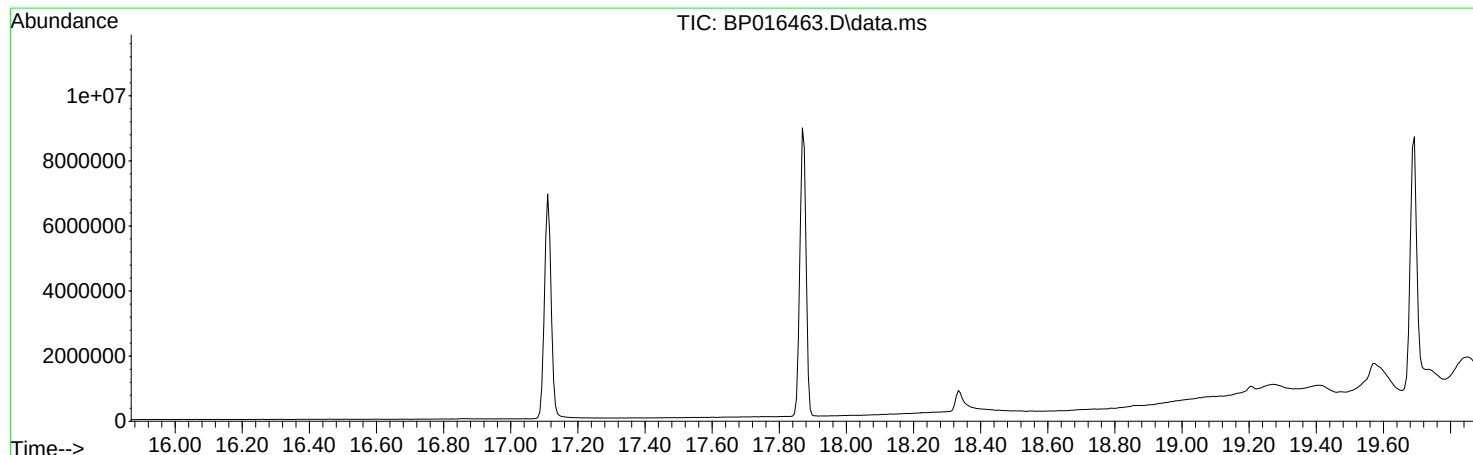




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	240283	PASS
68	69	0.00	2	1.7	4536	PASS
69	198	0.00	100	32.1	271209	PASS
70	69	0.00	2	0.5	1342	PASS
127	198	10	80	43.0	362656	PASS
197	198	0.00	2	0.6	4805	PASS
198	198	100	100	100.0	844136	PASS
199	198	5	9	6.9	58077	PASS
275	198	10	60	28.0	236672	PASS
365	198	1	100	4.1	34968	PASS
441	198	0.01	100	19.9	167875	PASS
442	442	100	100	100.0	1079509	PASS
443	442	15	24	19.7	213153	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
Data File : BP016463.D
Acq On : 02 Aug 2023 11:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 02 23:38:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

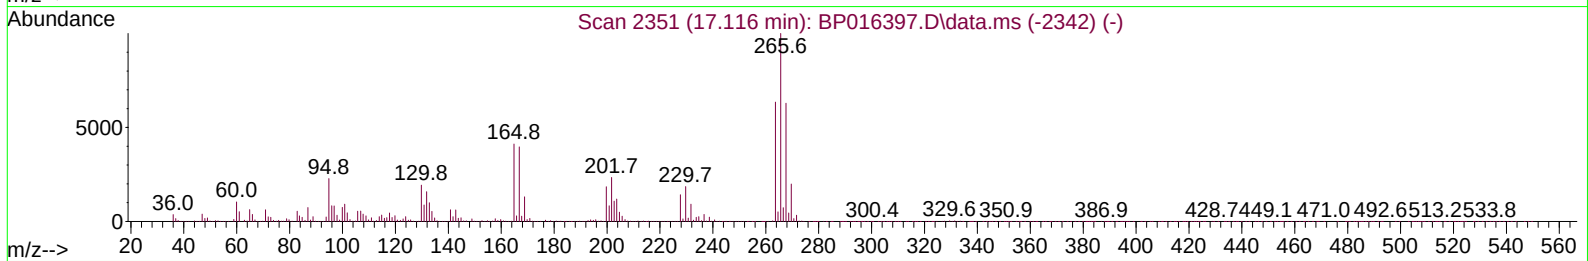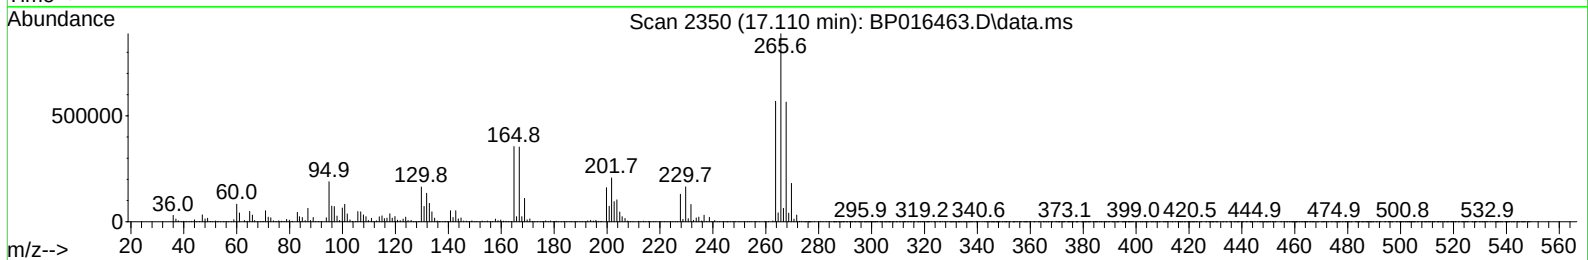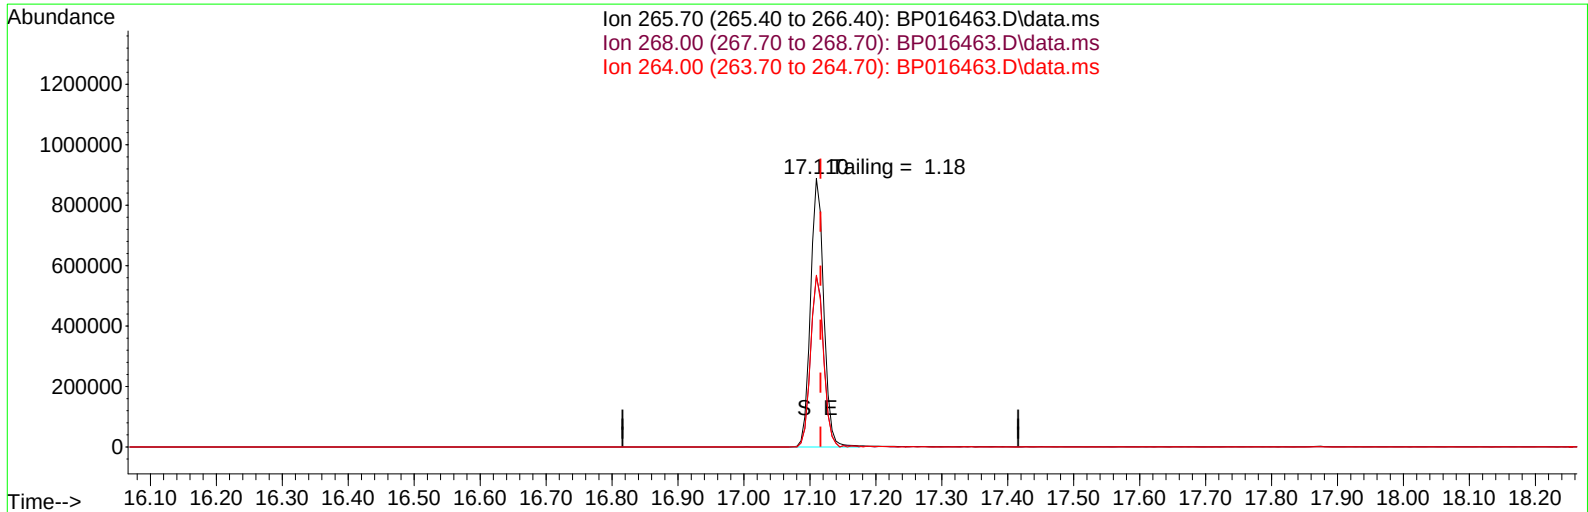

TIC: BP016463.D\data.ms

(70) Pentachlorophenol (C)

17.110min (-0.006) 1906096.18 ng




response 1246069

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	68.13
264.00	68.60	68.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080223\
Data File : BP016463.D
Acq On : 02 Aug 2023 11:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 02 23:38:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

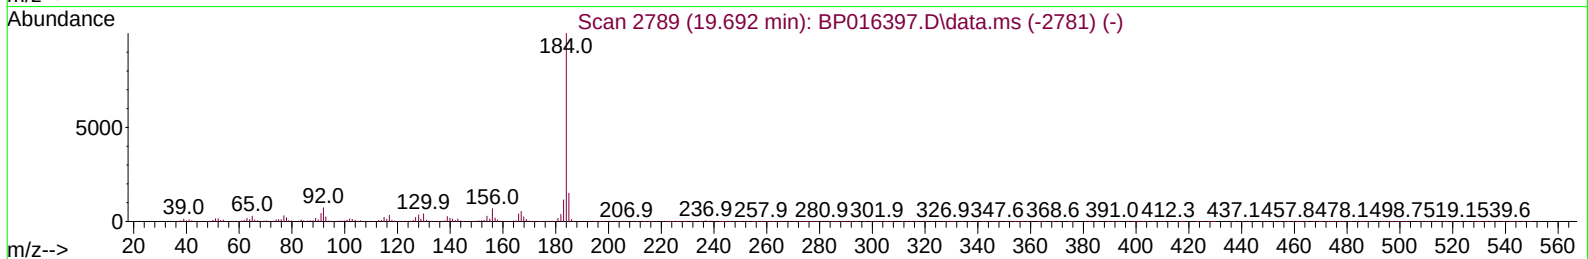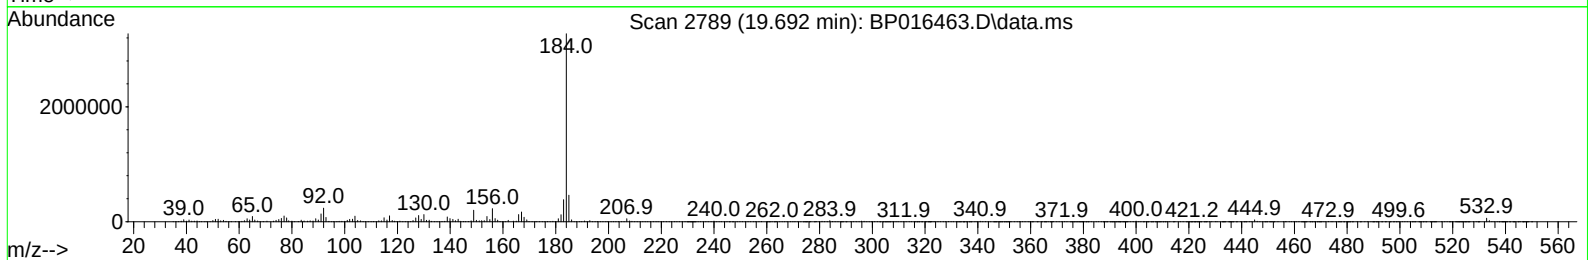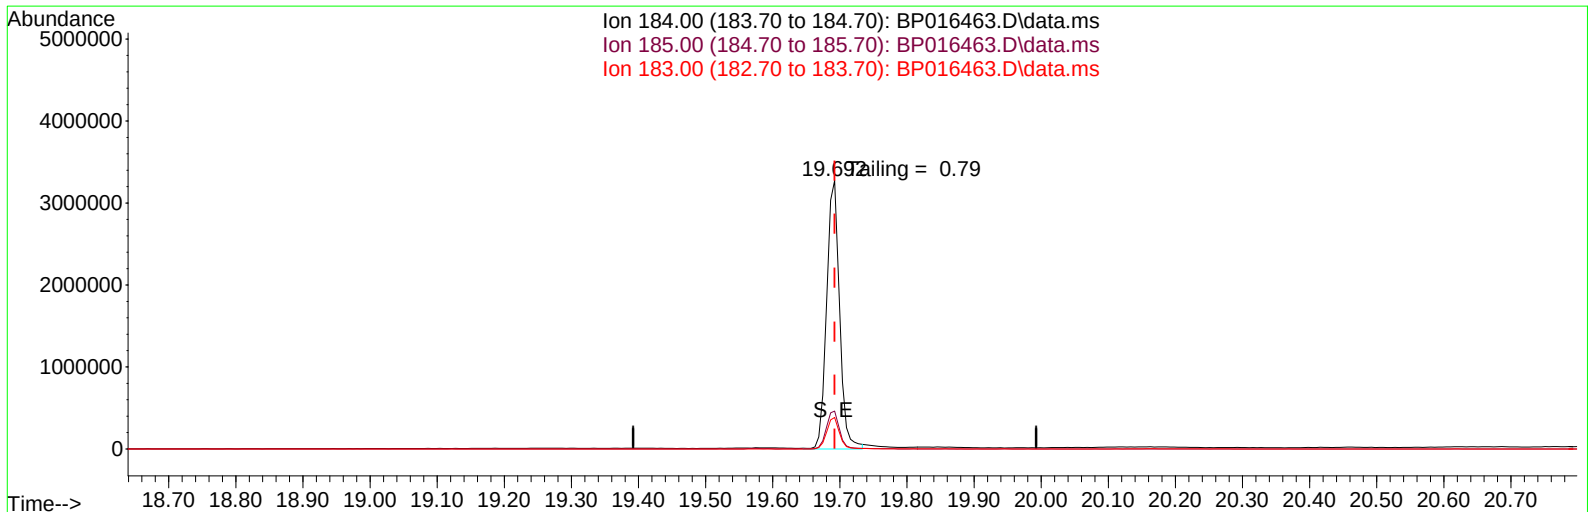

TIC: BP016463.D\data.ms

(77) Benzidine

19.692min (-0.000) 0.00 ng

response 4435777

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.10
183.00	11.50	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_P	<u>BP016463.D</u>
Compound Name	Response	Retention Time
DDT	2240361	20.874
DDD	65737	20.486
DDE	0	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65737	2306098	2.85

Instrument :
BNA_P
ClientSampleId :
DFTPP