
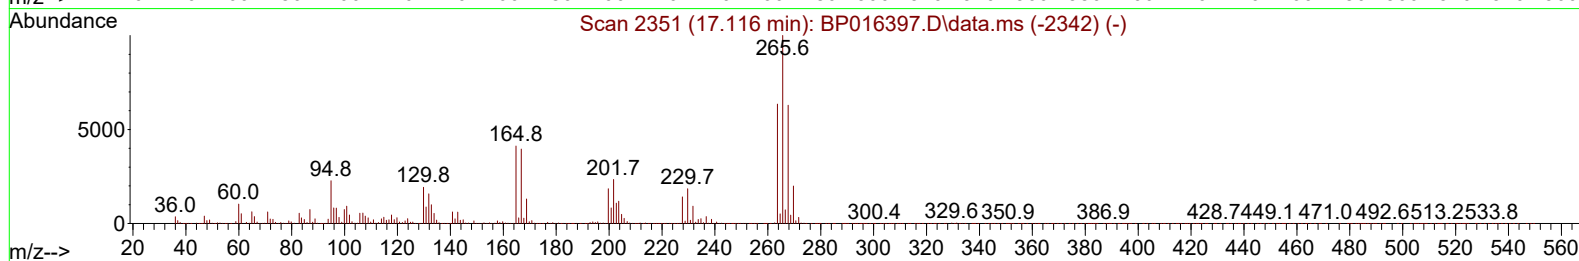
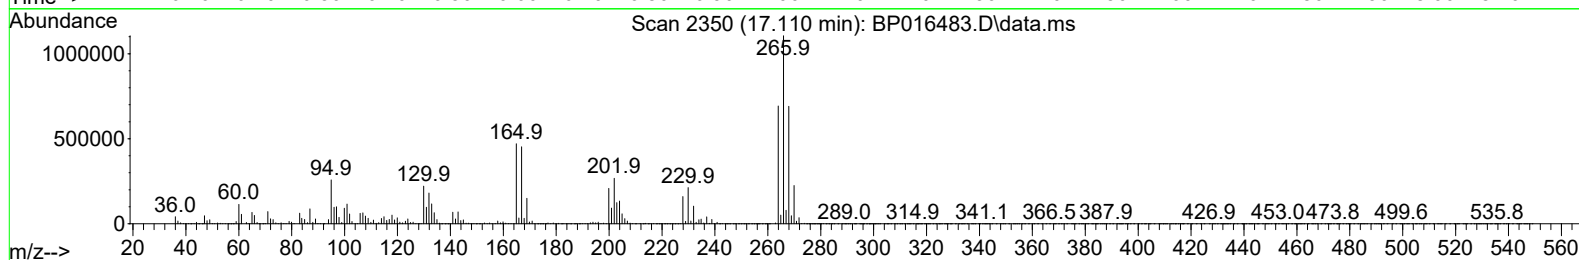


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016483.D
Acq On : 03 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 11:41:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

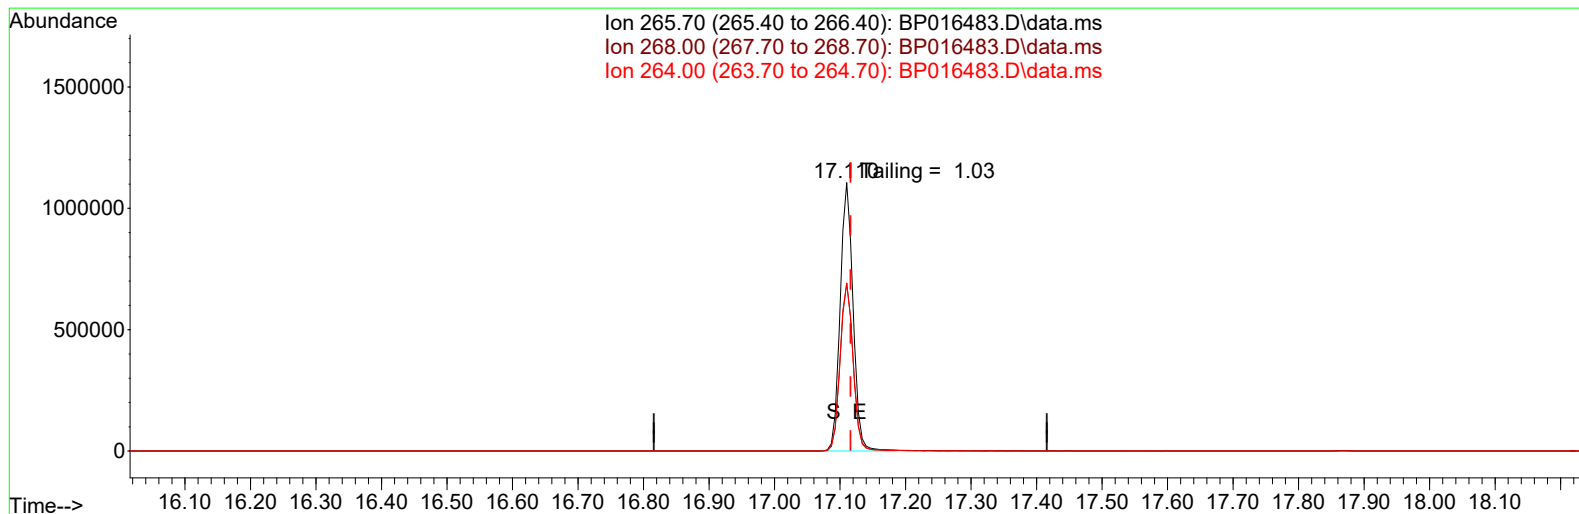

TIC: BP016483.D\data.ms

(70) Pentachlorophenol (C)




17.110min (-0.006) 2807126.76 ng

response 1513956

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	62.47
264.00	68.60	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
 Data File : BP016483.D
 Acq On : 03 Aug 2023 08:44
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 11:41:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 01:48:25 2023
 Response via : Initial Calibration

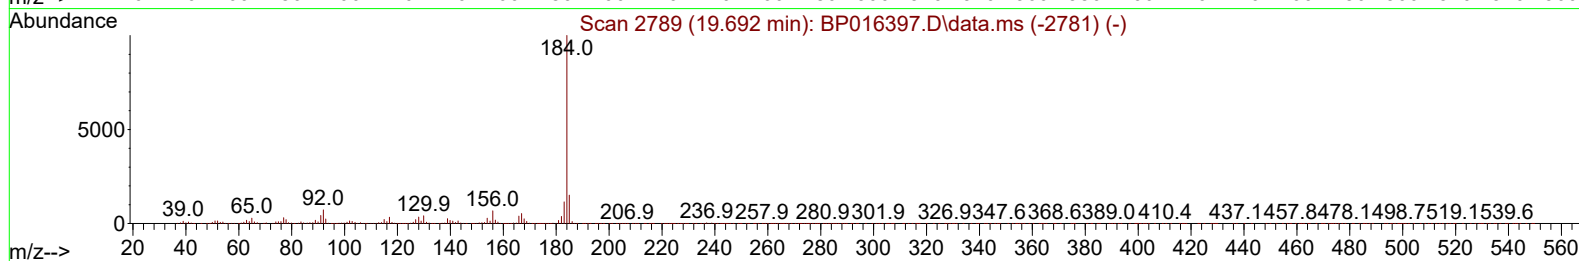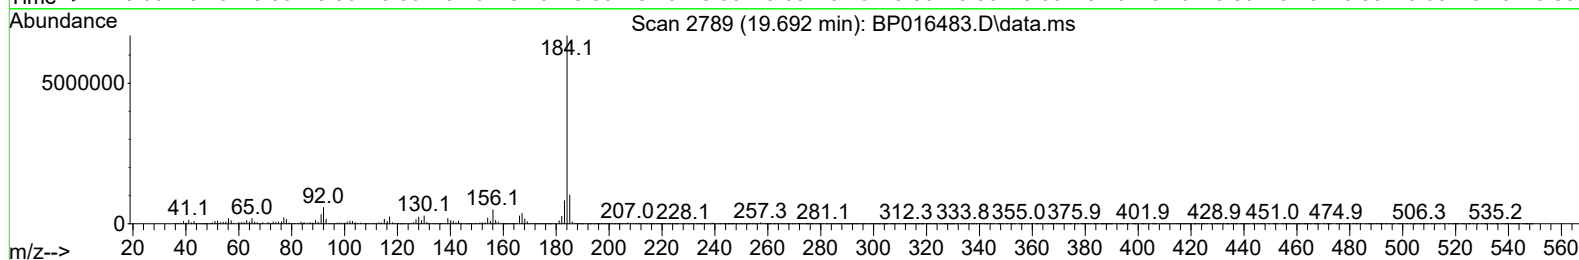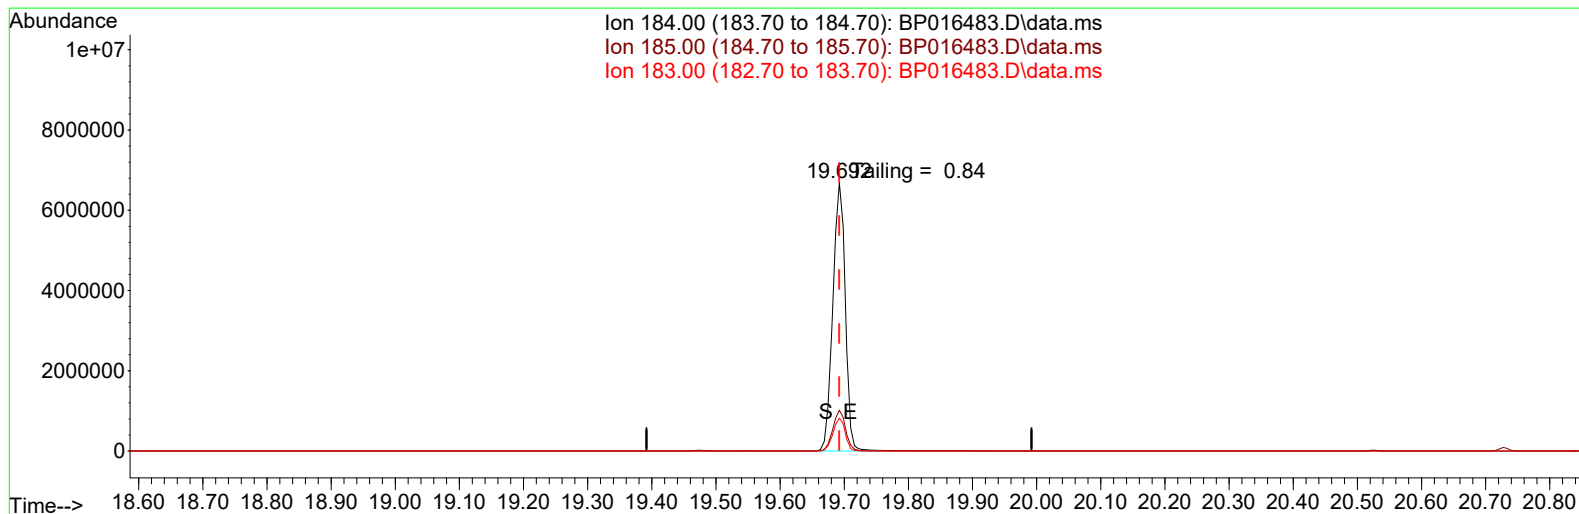

TIC: BP016483.D\data.ms

(77) Benzidine

19.692min (+ 0.000) 9861556.54 ng

response 9061772

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.23
183.00	11.50	12.30
0.00	0.00	0.00