

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
 Data File : BP016485.D
 Acq On : 03 Aug 2023 11:08
 Operator : MA/JU
 Sample : PB154495BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB154495BL

Quant Time: Aug 03 18:12:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 03 18:07:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.069	152	396102	20.000	ng	0.00
21) Naphthalene-d8	10.904	136	1533564	20.000	ng	0.00
39) Acenaphthene-d10	14.716	164	849502	20.000	ng	0.00
64) Phenanthrene-d10	17.486	188	1798810	20.000	ng	0.00
76) Chrysene-d12	21.580	240	1560630	20.000	ng	# 0.00
86) Perylene-d12	24.174	264	1775300	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.587	112	3596996	148.148	ng	0.00
7) Phenol-d6	7.210	99	4441419	133.458	ng	0.00
23) Nitrobenzene-d5	9.269	82	2632643	96.097	ng	0.00
42) 2,4,6-Tribromophenol	16.216	330	1510185	120.840	ng	0.00
45) 2-Fluorobiphenyl	13.345	172	5546506	93.606	ng	0.00
79) Terphenyl-d14	20.033	244	7810252	105.717	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016485.D
Acq On : 03 Aug 2023 11:08
Operator : MA/JU
Sample : PB154495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154495BL

Quant Time: Aug 03 18:12:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 18:07:40 2023
Response via : Initial Calibration




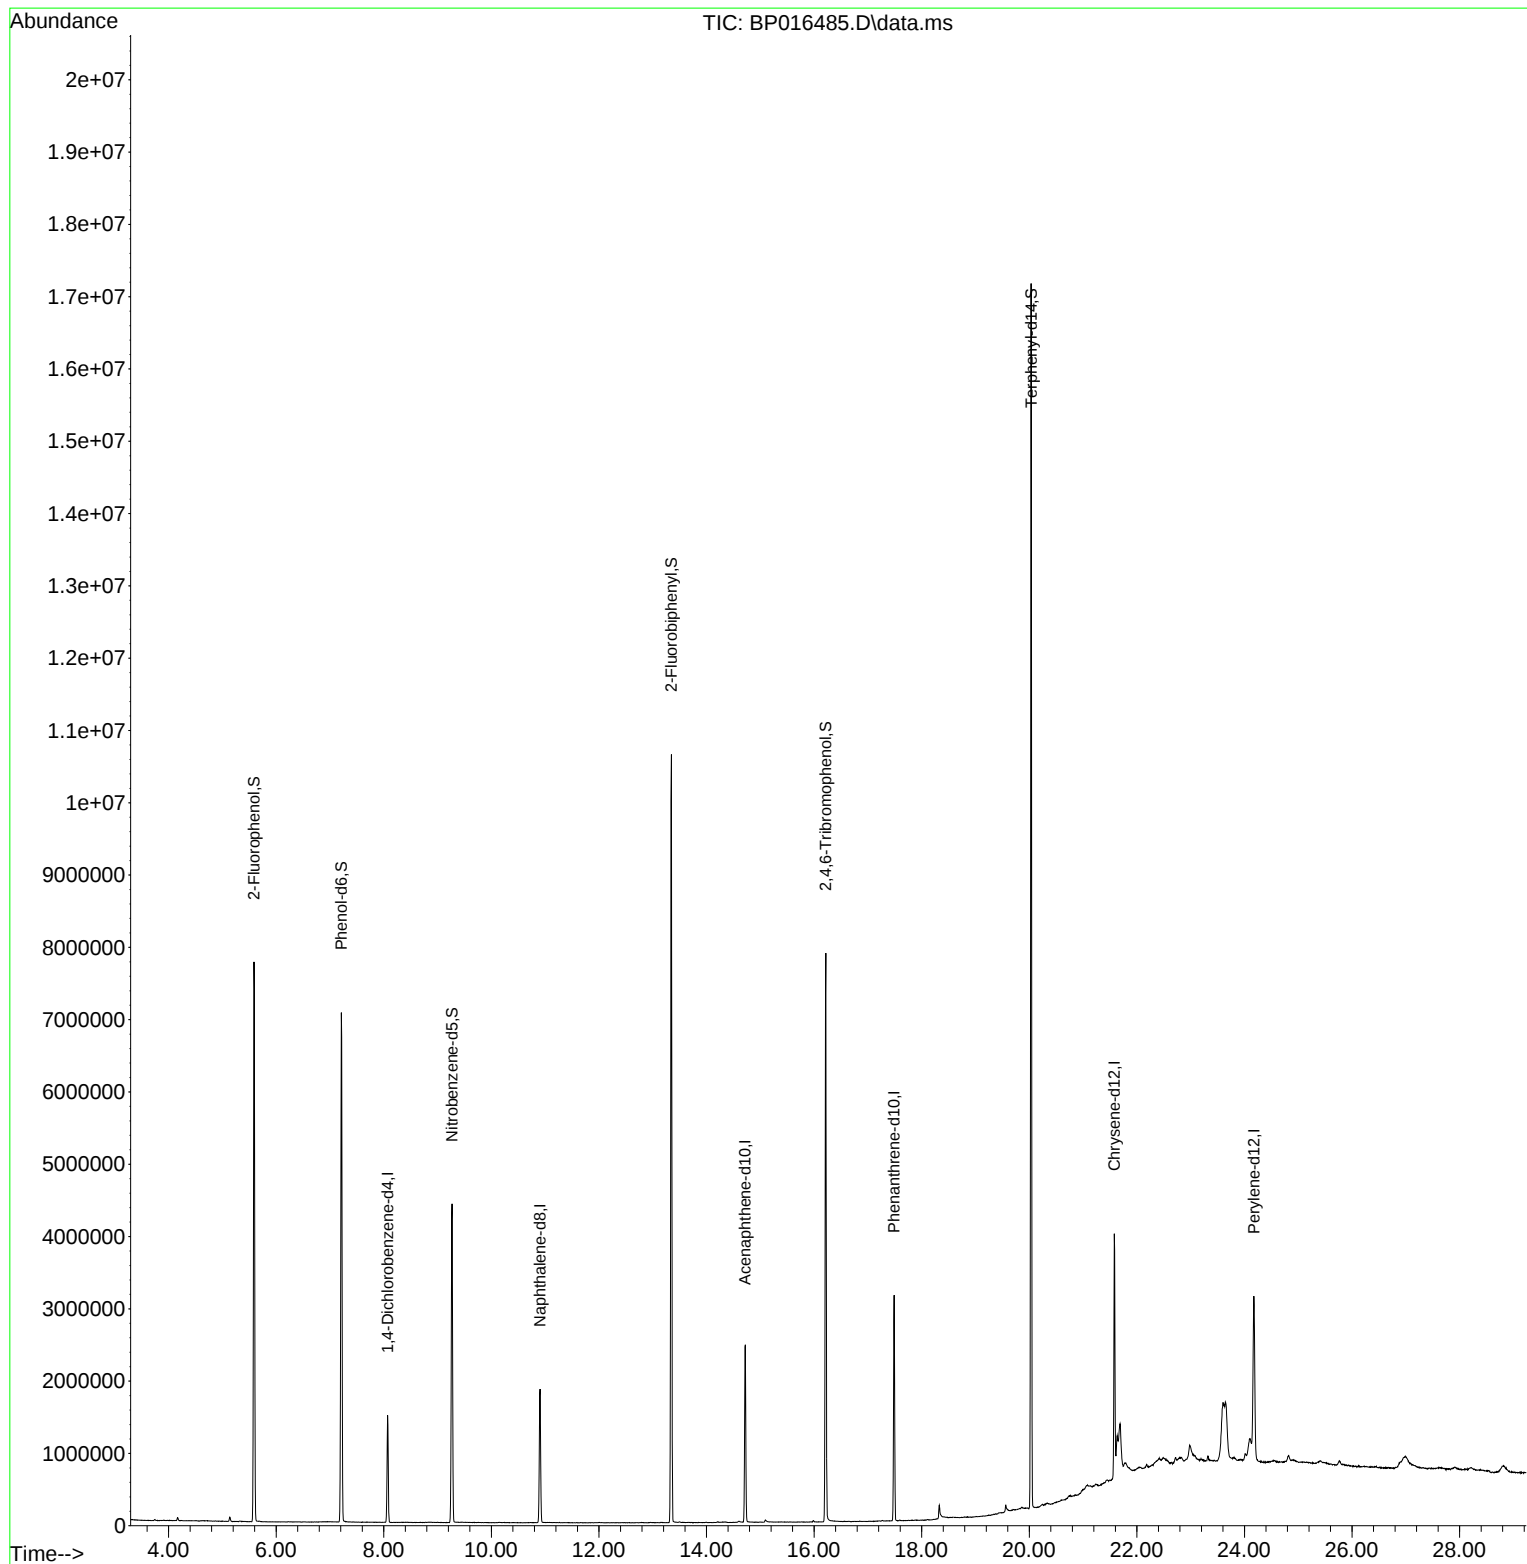




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.069 min Scan# 81
Delta R.T. 0.000 min
Lab File: BP016485.D
Acq: 03 Aug 2023 11:08




Instrument :
BNA_P
ClientSampleId :
PB154495BL


Tgt Ion:152 Resp: 396102
Ion Ratio Lower Upper
152 100
150 160.7 124.9 187.3
115 60.2 46.8 70.2

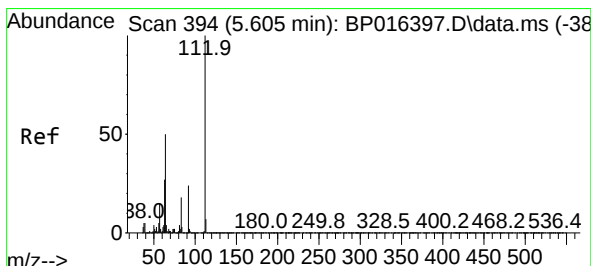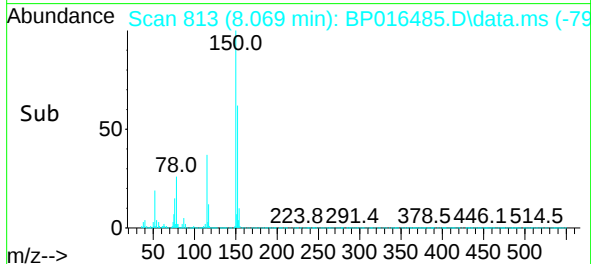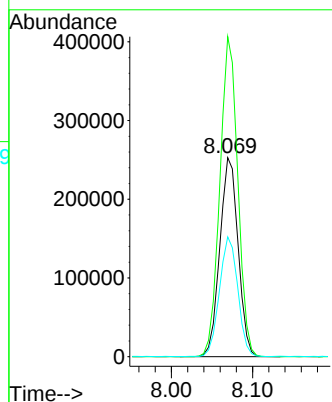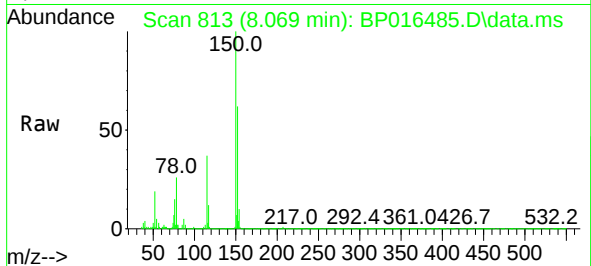

#5
2-Fluorophenol
Concen: 148.148 ng
RT: 5.587 min Scan# 391
Delta R.T. 0.006 min
Lab File: BP016485.D
Acq: 03 Aug 2023 11:08

Tgt Ion:112 Resp: 3596996
Ion Ratio Lower Upper
112 100
64 52.5 40.0 60.0
63 27.0 21.2 31.8


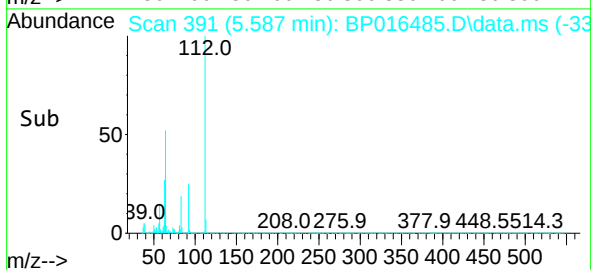
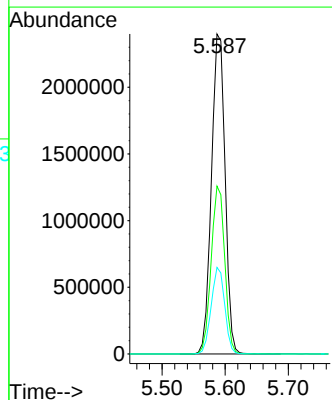
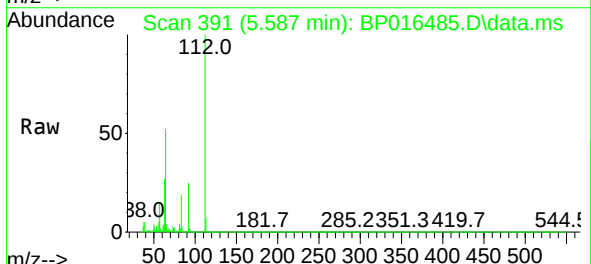


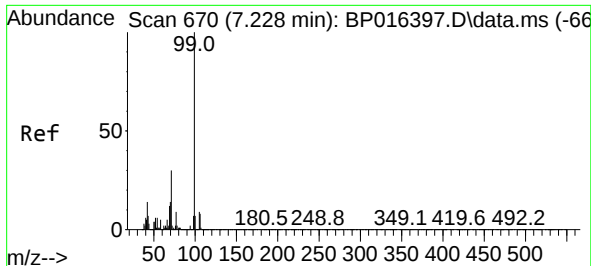

#7
Phenol-d6
Concen: 133.458 ng
RT: 7.210 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP016485.D
Acq: 03 Aug 2023 11:08




Instrument :
BNA_P
ClientSampleId :
PB154495BL


Tgt Ion: 99 Resp: 4441419
Ion Ratio Lower Upper
99 100
42 14.5 11.6 17.4
71 30.9 24.3 36.5

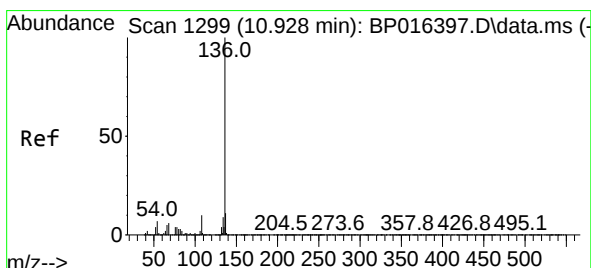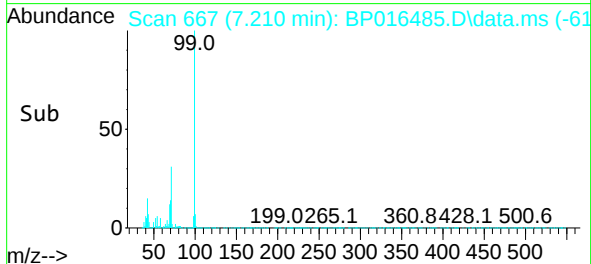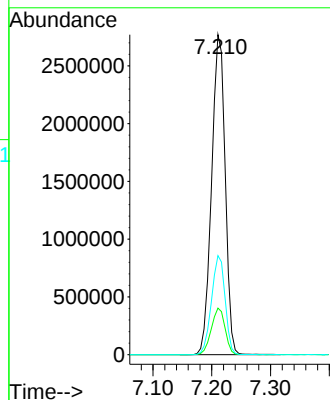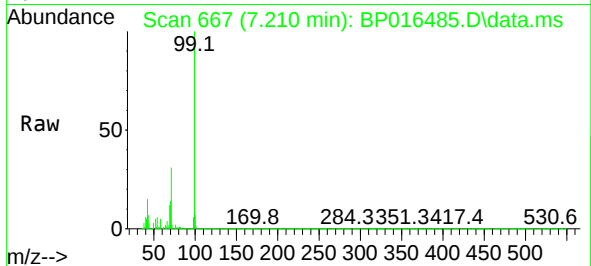

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.904 min Scan# 1295
Delta R.T. -0.000 min
Lab File: BP016485.D
Acq: 03 Aug 2023 11:08

Tgt Ion:136 Resp: 1533564
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 7.1 5.6 8.4
68 6.2 4.6 6.8

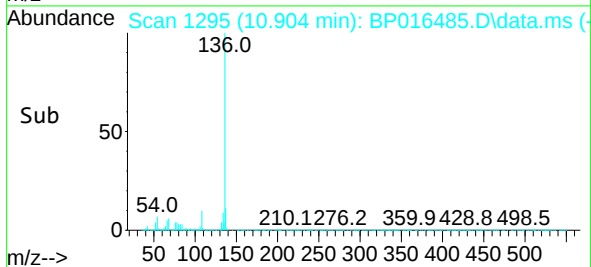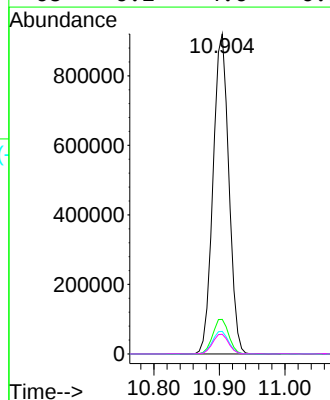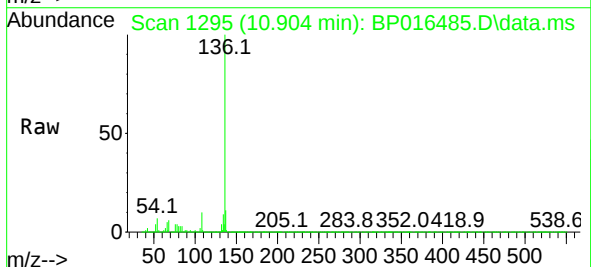

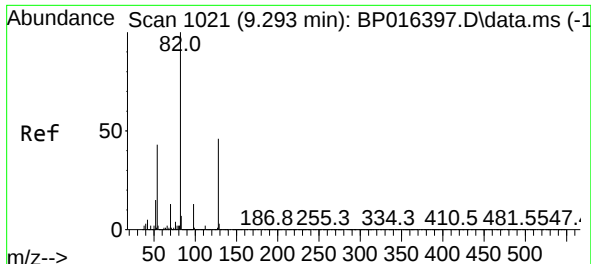

#23

Nitrobenzene-d5

Concen: 96.097 ng

RT: 9.269 min Scan# 1021

Delta R.T. -0.000 min

Lab File: BP016485.D

Acq: 03 Aug 2023 11:08

Instrument :

BNA_P

ClientSampleId :

PB154495BL





Tgt Ion: 82 Resp: 2632643

Ion Ratio Lower Upper

82 100

128 44.7 36.6 55.0

54 42.4 34.5 51.7

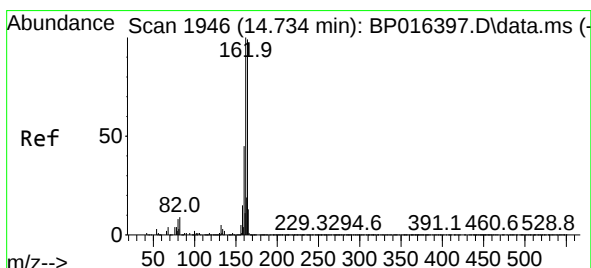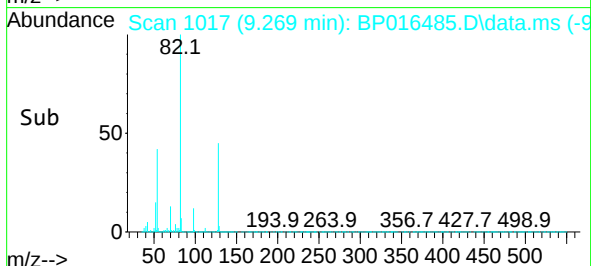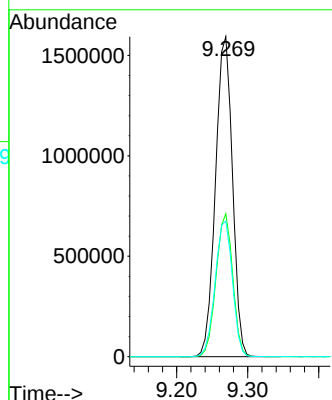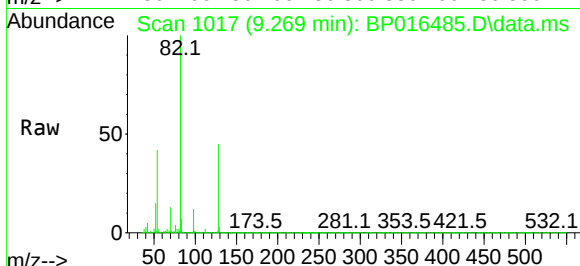

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.716 min Scan# 1943

Delta R.T. -0.006 min

Lab File: BP016485.D

Acq: 03 Aug 2023 11:08




Tgt Ion: 164 Resp: 849502


Ion Ratio Lower Upper

164 100

162 99.1 81.0 121.6

160 44.5 36.6 55.0


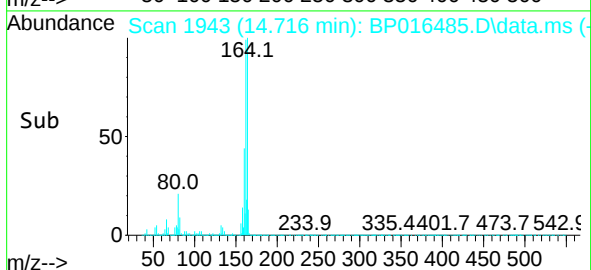
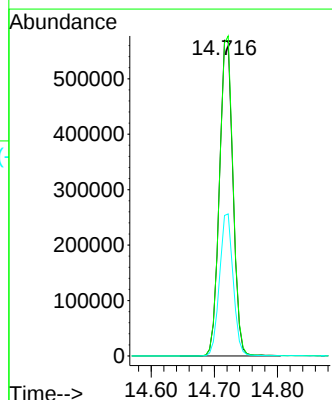
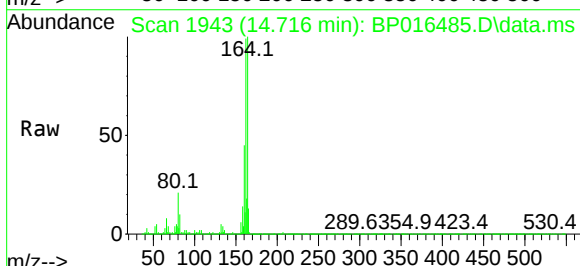


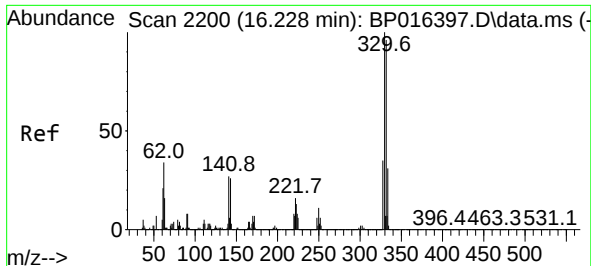

#42
2,4,6-Tribromophenol
Concen: 120.840 ng
RT: 16.216 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP016485.D
Acq: 03 Aug 2023 11:08




Instrument :
BNA_P
ClientSampleId :
PB154495BL


Tgt Ion:330 Resp: 1510185
Ion Ratio Lower Upper
330 100
332 96.8 77.8 116.8
141 33.0 22.6 34.0

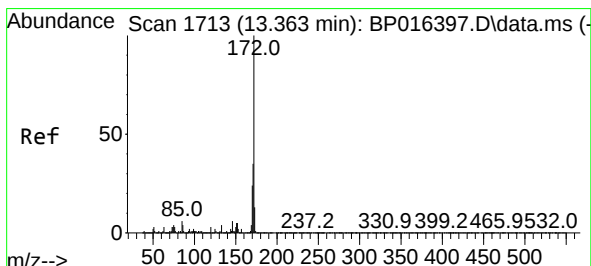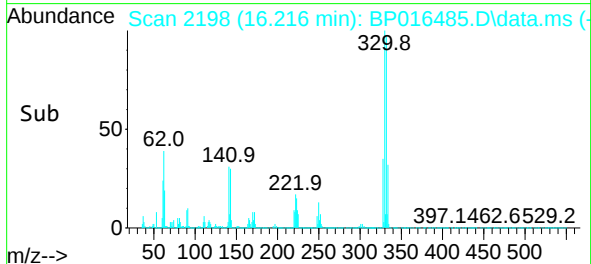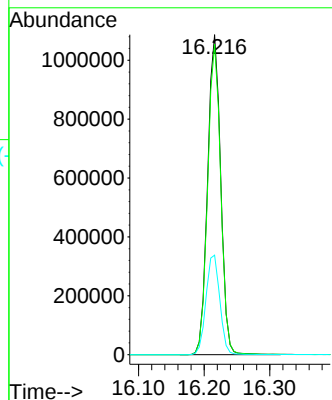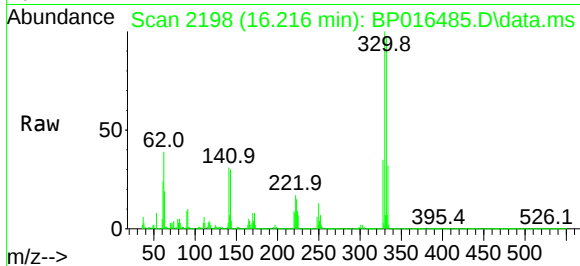

#45
2-Fluorobiphenyl
Concen: 93.606 ng
RT: 13.345 min Scan# 1710
Delta R.T. -0.000 min
Lab File: BP016485.D
Acq: 03 Aug 2023 11:08

Tgt Ion:172 Resp: 5546506
Ion Ratio Lower Upper
172 100
171 35.4 28.2 42.2
170 23.3 19.1 28.7

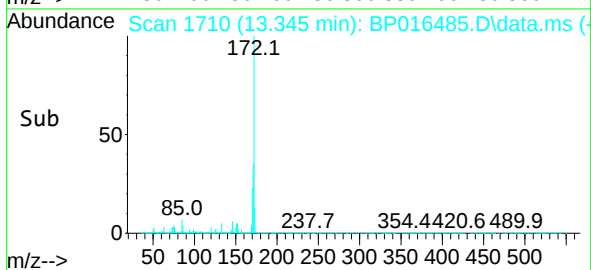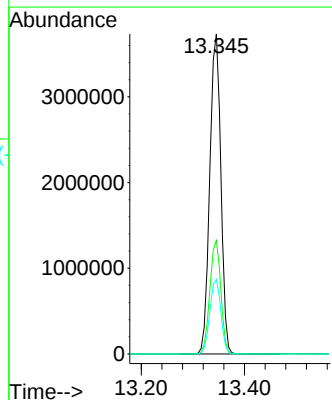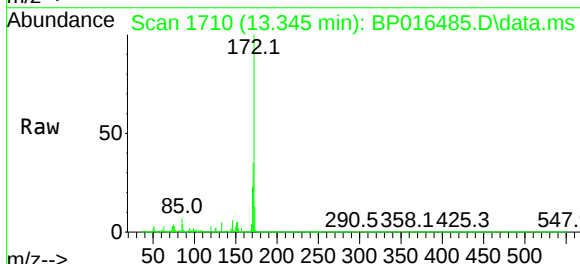

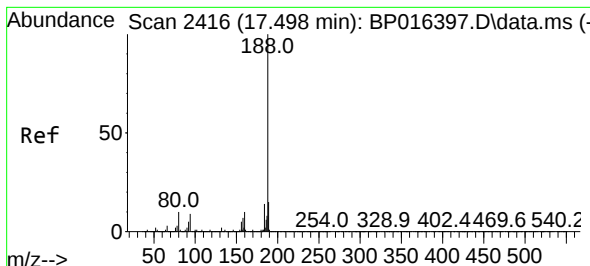

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.486 min Scan# 2416

Delta R.T. -0.000 min

Lab File: BP016485.D

Acq: 03 Aug 2023 11:08

Instrument :

BNA_P

ClientSampleId :

PB154495BL





Tgt Ion:188 Resp: 1798810

Ion Ratio Lower Upper

188 100

94 9.6 7.4 11.0

80 10.8 7.8 11.8

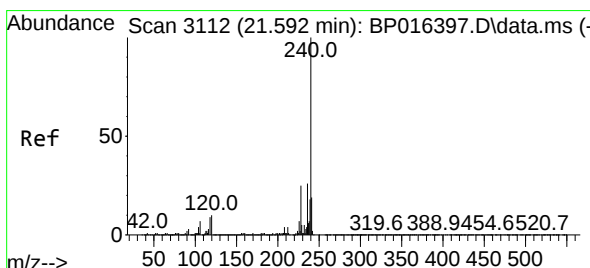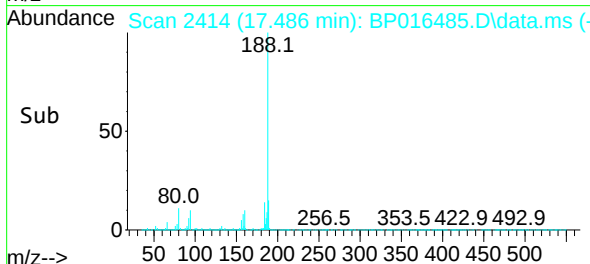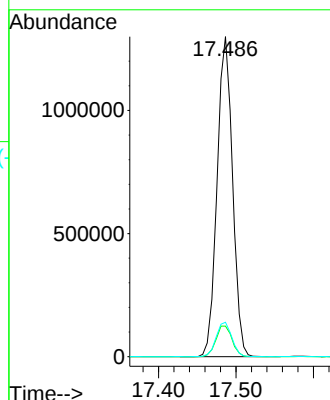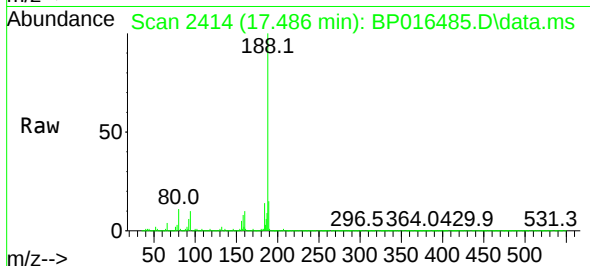

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.580 min Scan# 3110

Delta R.T. -0.006 min

Lab File: BP016485.D

Acq: 03 Aug 2023 11:08




Tgt Ion:240 Resp: 1560630


Ion Ratio Lower Upper

240 100

120 12.1 7.9 11.9#

236 25.4 21.1 31.7


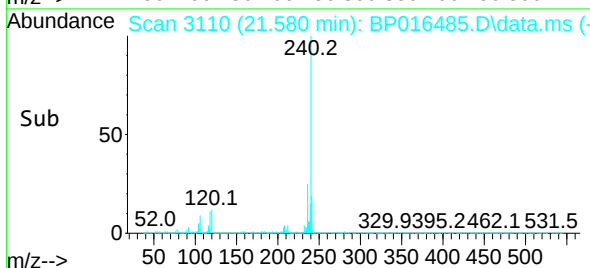
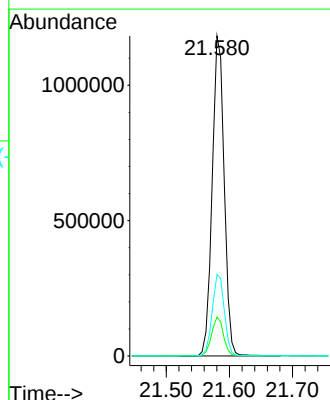
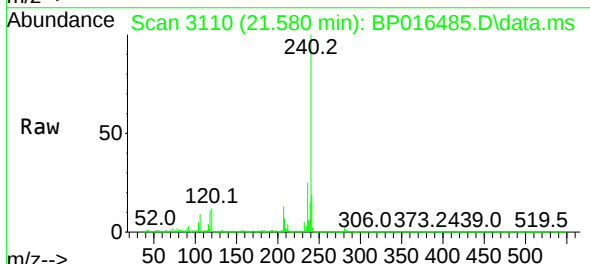


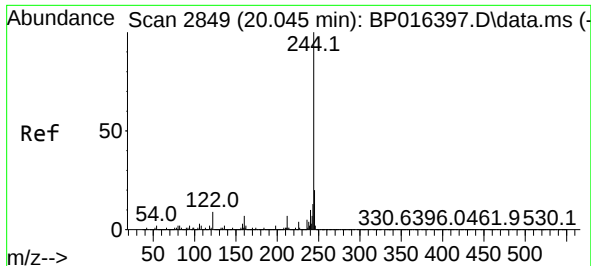

#79
 Terphenyl-d14
 Concen: 105.717 ng
 RT: 20.033 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP016485.D
 Acq: 03 Aug 2023 11:08

Instrument :
 BNA_P
 ClientSampleId :
 PB154495BL

Tgt Ion:244 Resp: 7810252
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.6 8.4
 122 11.3 7.4 11.2#

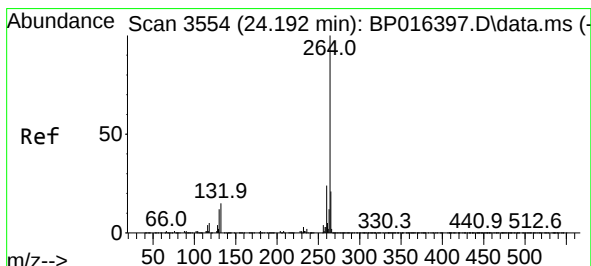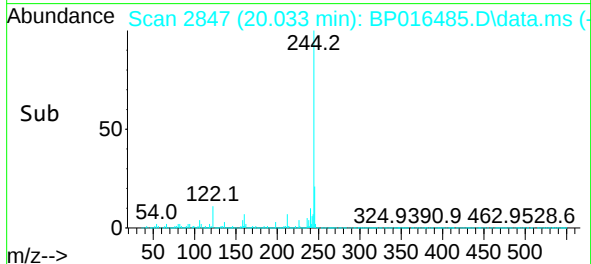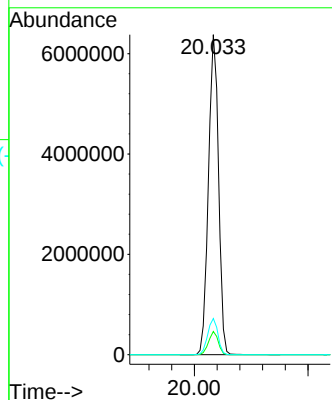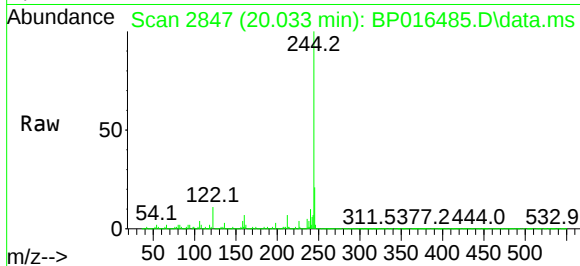

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.174 min Scan# 3551
 Delta R.T. -0.006 min
 Lab File: BP016485.D
 Acq: 03 Aug 2023 11:08

Tgt Ion:264 Resp: 1775300
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.3 28.9
 265 22.1 17.4 26.0

