

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
 Data File : BP016485.D
 Acq On : 03 Aug 2023 11:08
 Operator : MA/JU
 Sample : PB154495BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB154495BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	384	391	402	rBV	7742389	11542849	55.82%	11.284%
2	7.210	659	667	679	rBV	7044926	11492708	55.57%	11.235%
3	8.069	805	813	823	rVB	1481723	2304589	11.14%	2.253%
4	9.269	1008	1017	1027	rBV	4408954	7356709	35.57%	7.192%
5	10.904	1286	1295	1306	rBV	1847021	3102800	15.00%	3.033%
6	13.345	1702	1710	1723	rBV	10624190	15868533	76.73%	15.513%
7	14.722	1937	1944	1952	rBV	2453290	3706624	17.92%	3.624%
8	16.216	2190	2198	2215	rBV	7868713	11542484	55.81%	11.284%
9	17.486	2407	2414	2422	rBV	3121862	4376401	21.16%	4.278%
10	18.328	2552	2557	2568	rBV	188975	399947	1.93%	0.391%
11	20.033	2841	2847	2852	rBV	16937686	20679898	100.00%	20.216%
12	21.580	3105	3110	3115	rBV	3378348	4707065	22.76%	4.602%
13	24.174	3545	3551	3566	rVB	2287888	5212309	25.20%	5.095%




Sum of corrected areas: 102292916

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016485.D
Acq On : 03 Aug 2023 11:08
Operator : MA/JU
Sample : PB154495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154495BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

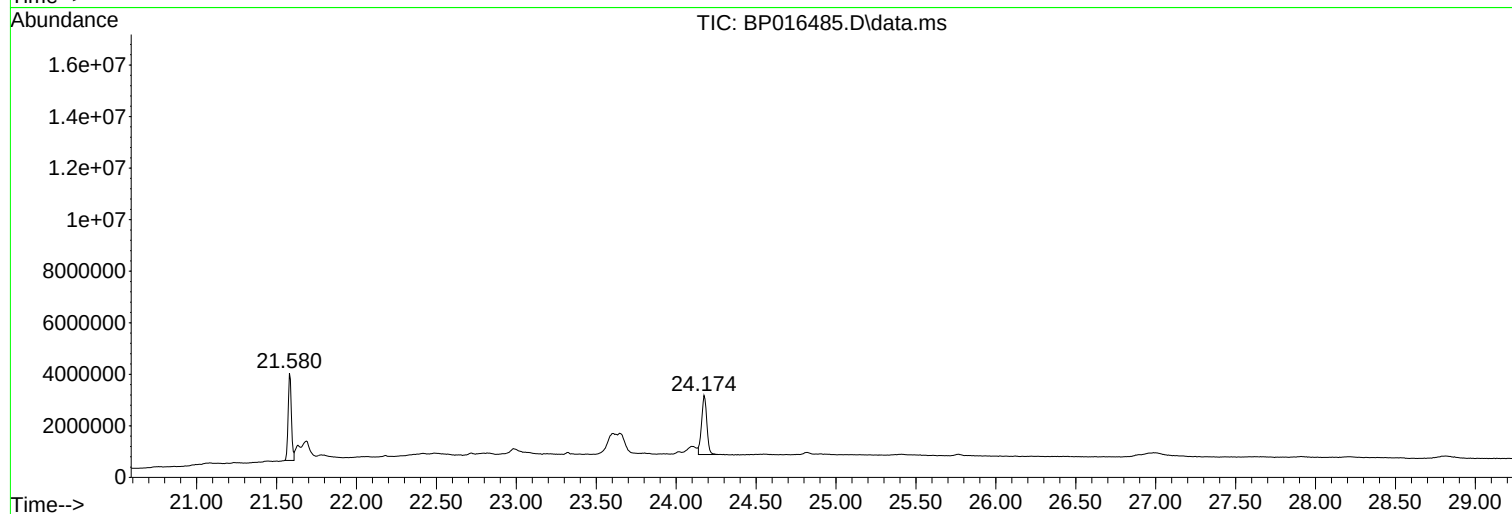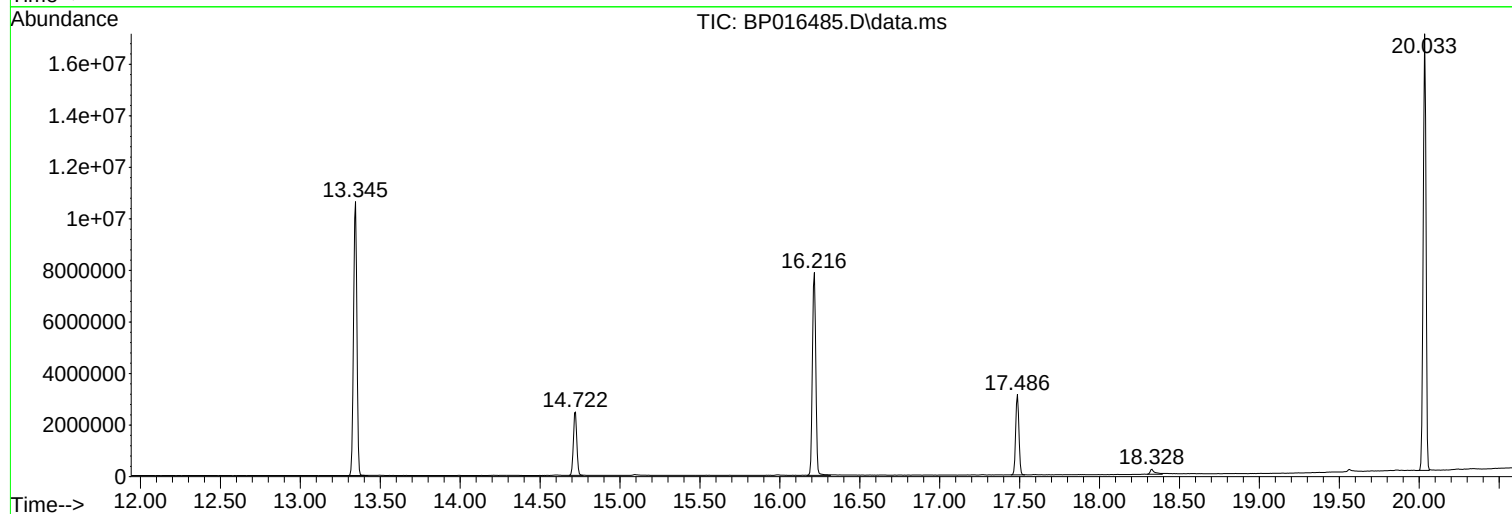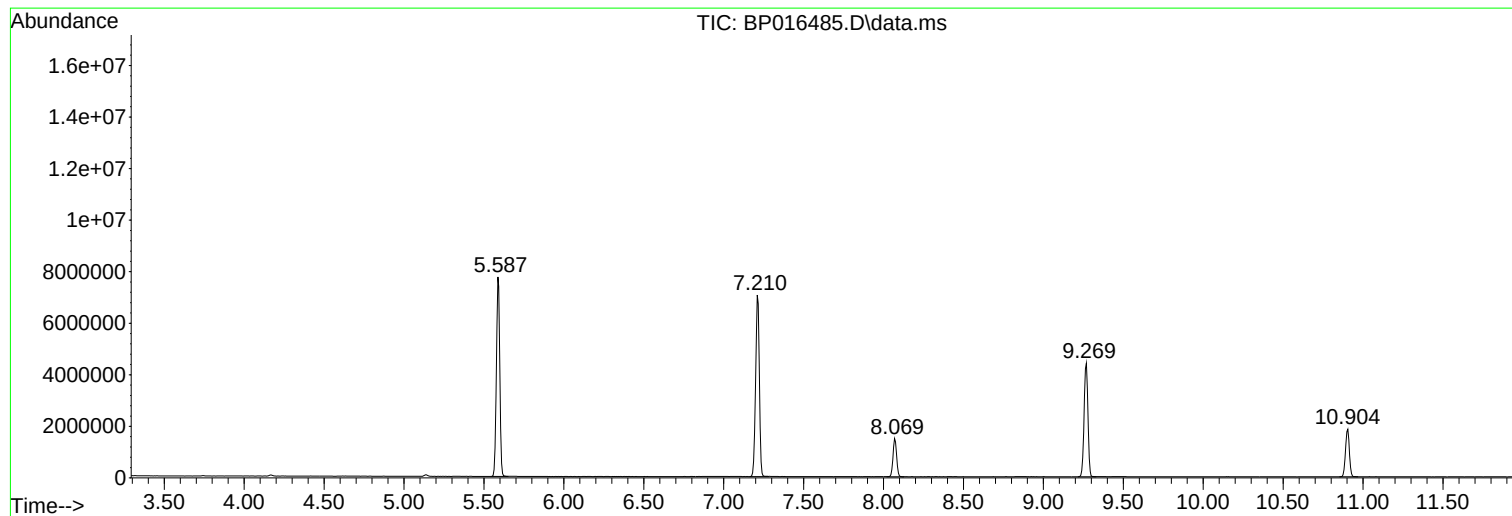

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016485.D
Acq On : 03 Aug 2023 11:08
Operator : MA/JU
Sample : PB154495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154495BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016485.D
Acq On : 03 Aug 2023 11:08
Operator : MA/JU
Sample : PB154495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154495BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------