

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016492.D
Acq On : 03 Aug 2023 15:07
Operator : MA/JU
Sample : PB154350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154350BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	384	391	401	rBV	7238493	10446310	58.20%	11.799%
2	7.211	659	667	684	rBV	6572178	10402346	57.96%	11.749%
3	8.069	806	813	823	rBV	1319625	2046065	11.40%	2.311%
4	9.269	1007	1017	1032	rBV	4026878	6671376	37.17%	7.535%
5	10.905	1286	1295	1304	rBV	1609689	2718791	15.15%	3.071%
6	13.340	1702	1709	1721	rBV	9293815	14285376	79.59%	16.135%
7	14.716	1937	1943	1952	rBV	2167615	3175652	17.69%	3.587%
8	16.216	2190	2198	2211	rBV	6432806	9617486	53.58%	10.863%
9	17.487	2407	2414	2423	rBV	2665042	3661247	20.40%	4.135%
10	20.033	2841	2847	2852	rBV	14661052	17948742	100.00%	20.273%
11	21.580	3105	3110	3117	rBV	2846750	3758137	20.94%	4.245%
12	24.174	3544	3551	3560	rVB	1792756	3805326	21.20%	4.298%




Sum of corrected areas: 88536854

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016492.D
Acq On : 03 Aug 2023 15:07
Operator : MA/JU
Sample : PB154350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154350BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

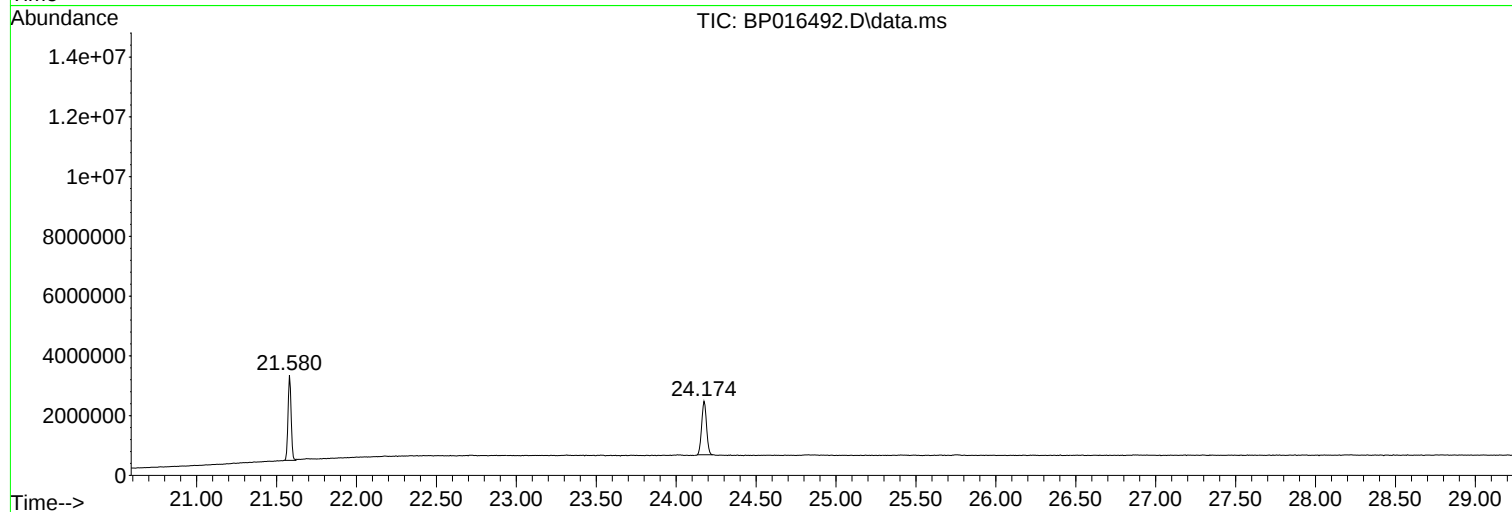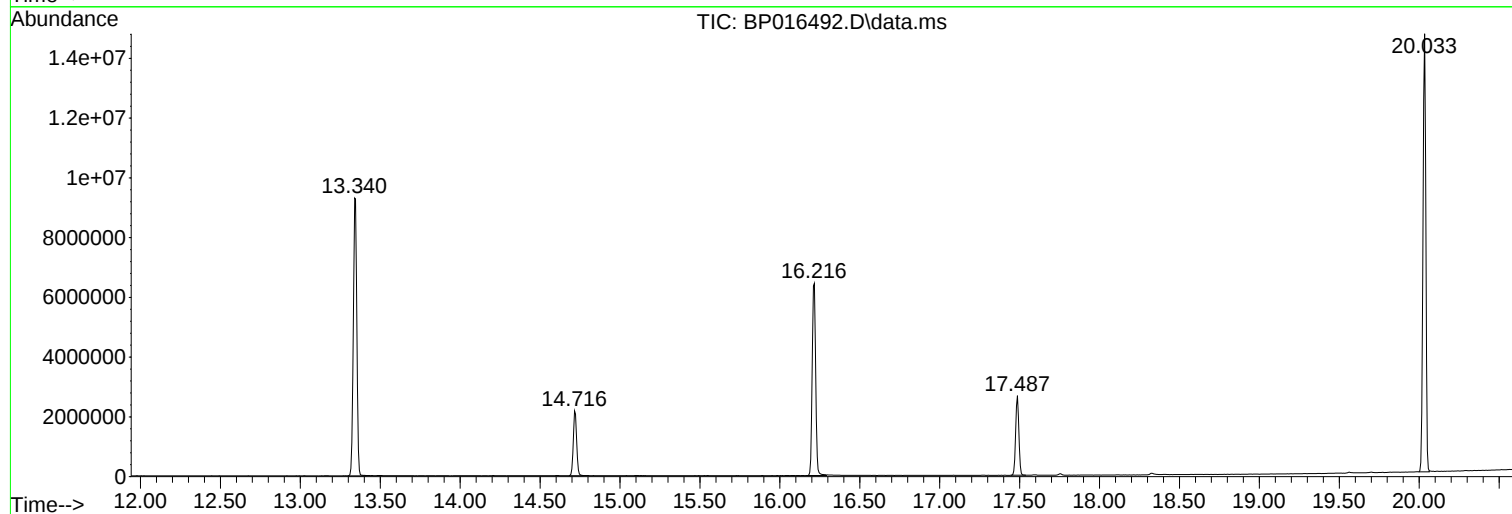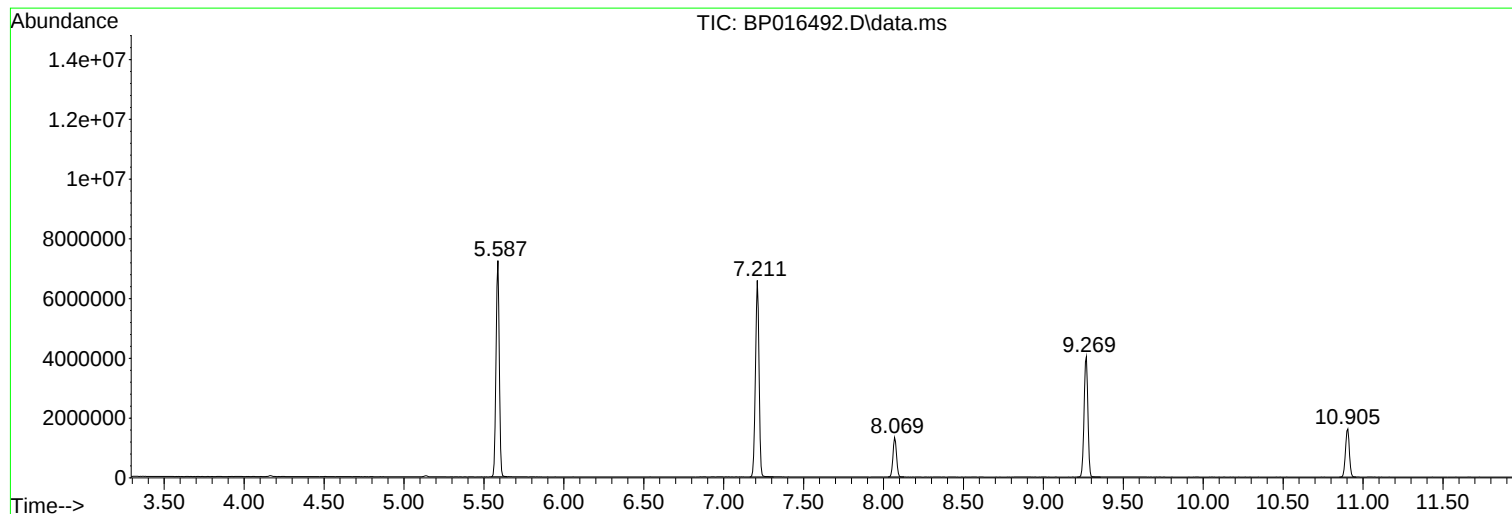

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016492.D
Acq On : 03 Aug 2023 15:07
Operator : MA/JU
Sample : PB154350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154350BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016492.D
Acq On : 03 Aug 2023 15:07
Operator : MA/JU
Sample : PB154350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154350BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------