
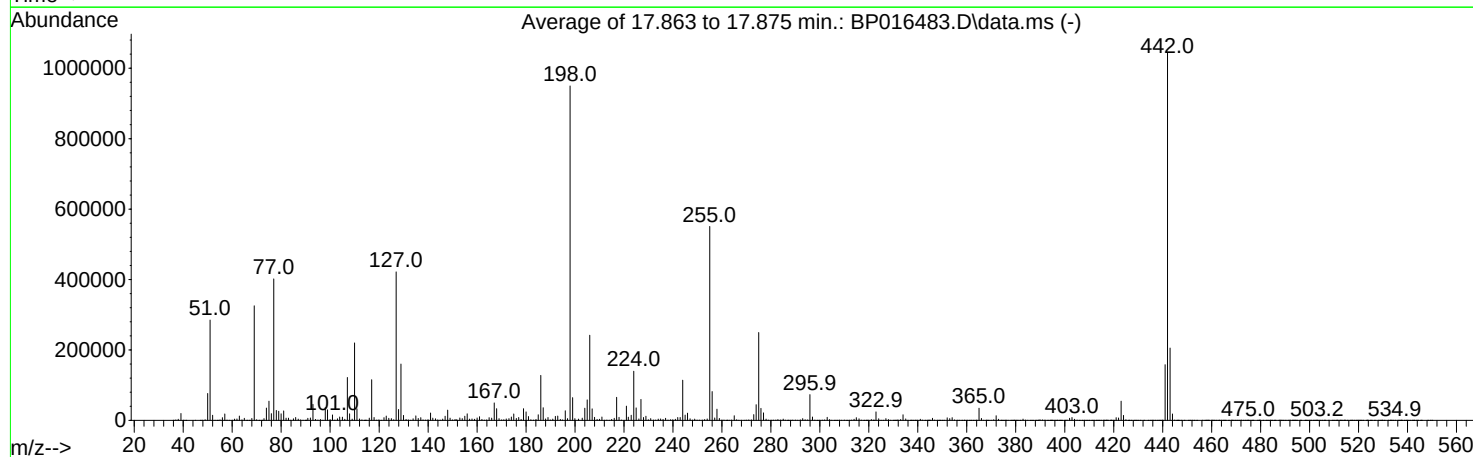


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016483.D
Acq On : 03 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 03 18:07:40 2023

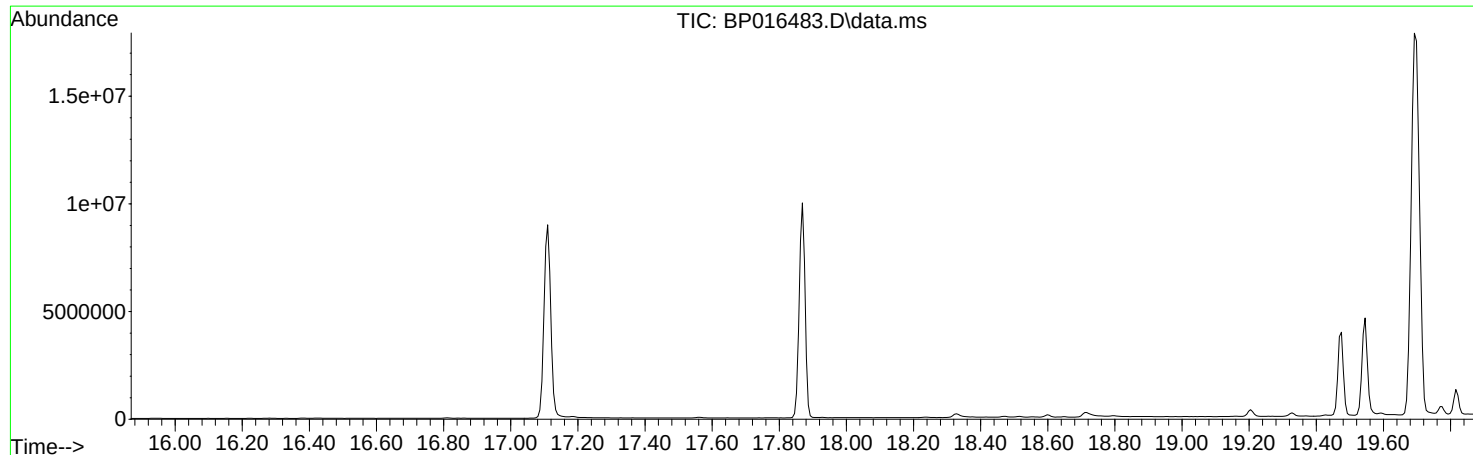




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	285164	PASS
68	69	0.00	2	1.7	5518	PASS
69	198	0.00	100	34.3	325587	PASS
70	69	0.00	2	0.5	1765	PASS
127	198	10	80	44.4	421823	PASS
197	198	0.00	2	0.5	5050	PASS
198	198	100	100	100.0	949891	PASS
199	198	5	9	6.8	64430	PASS
275	198	10	60	26.3	249557	PASS
365	198	1	100	3.7	34743	PASS
441	198	0.01	100	16.7	158339	PASS
442	442	100	100	100.0	1044774	PASS
443	442	15	24	19.6	205291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016483.D
Acq On : 03 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 03 11:41:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

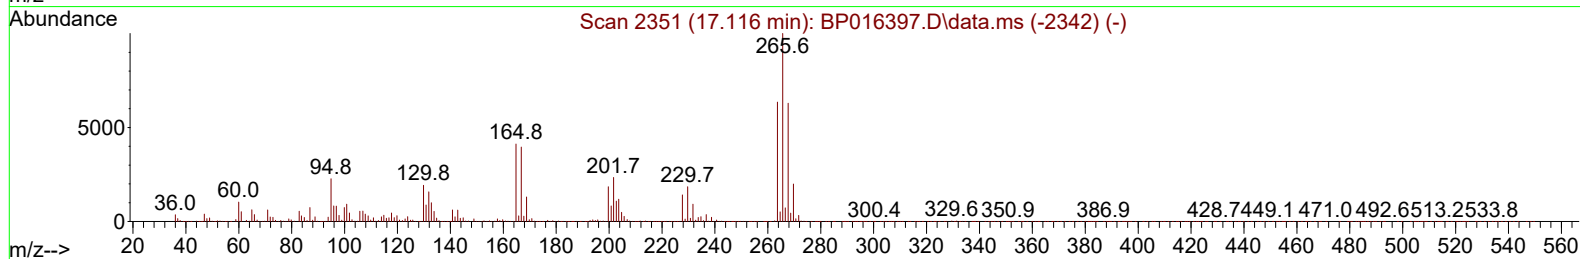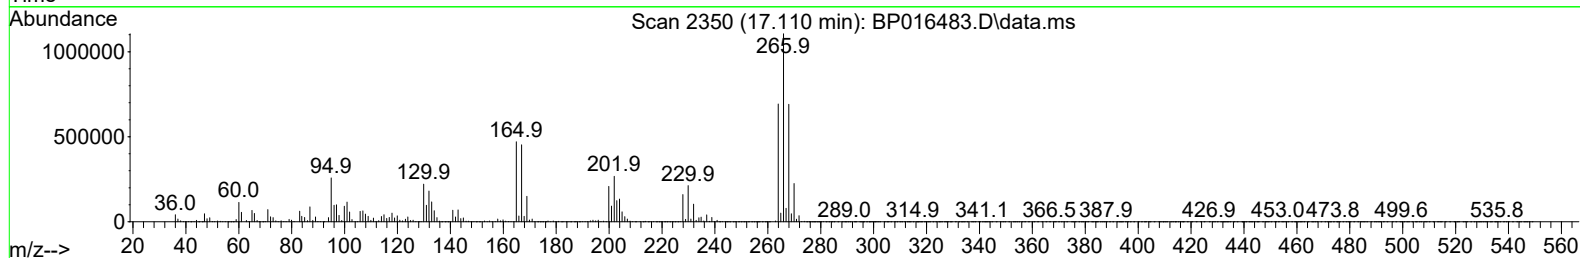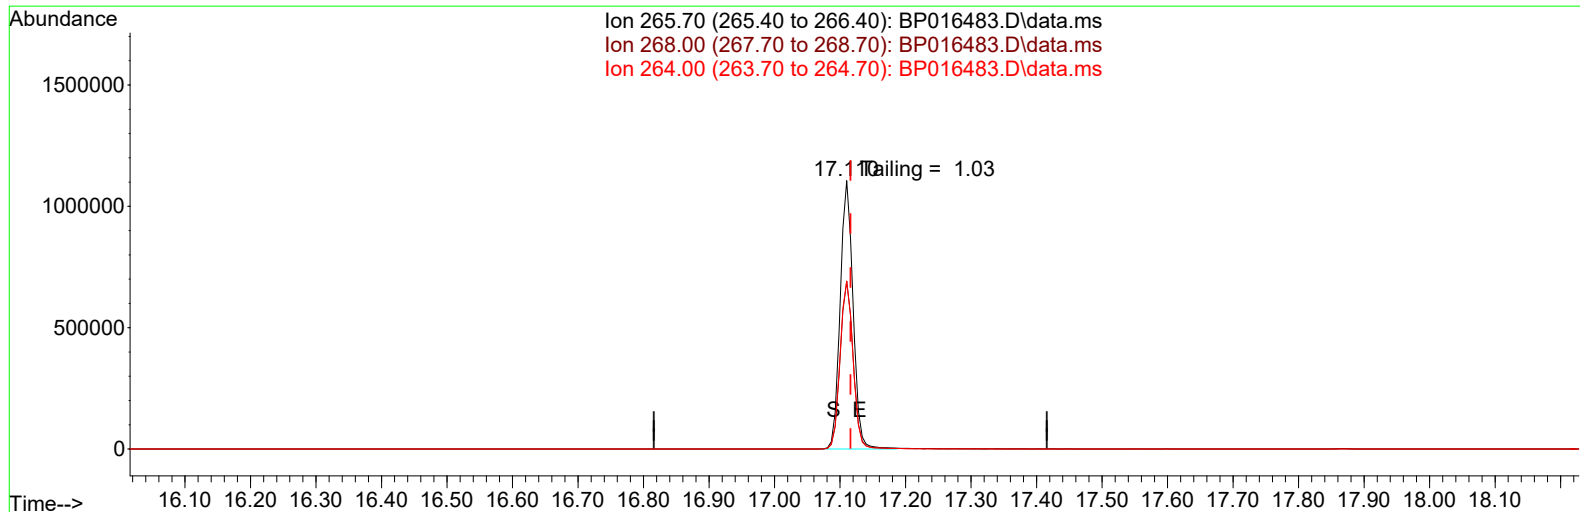

TIC: BP016483.D\data.ms

(70) Pentachlorophenol (C)

17.110min (-0.006) 2807126.76 ng




response 1513956

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	62.47
264.00	68.60	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080323\
Data File : BP016483.D
Acq On : 03 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 03 11:41:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

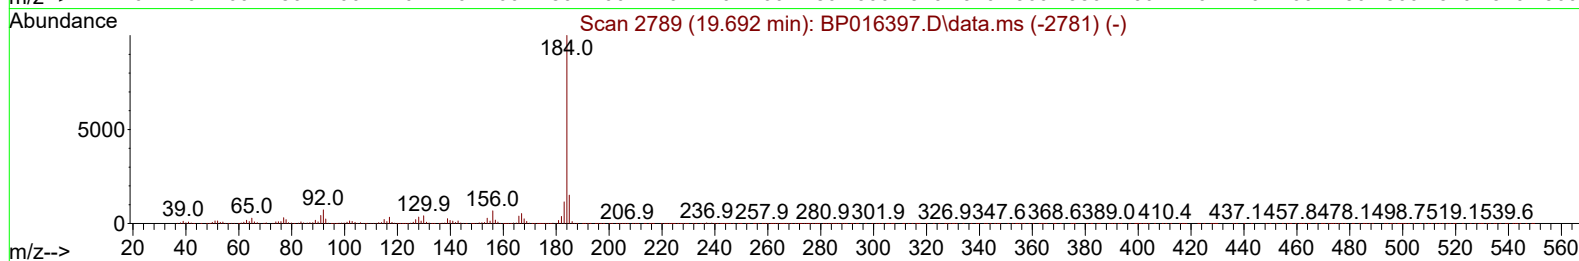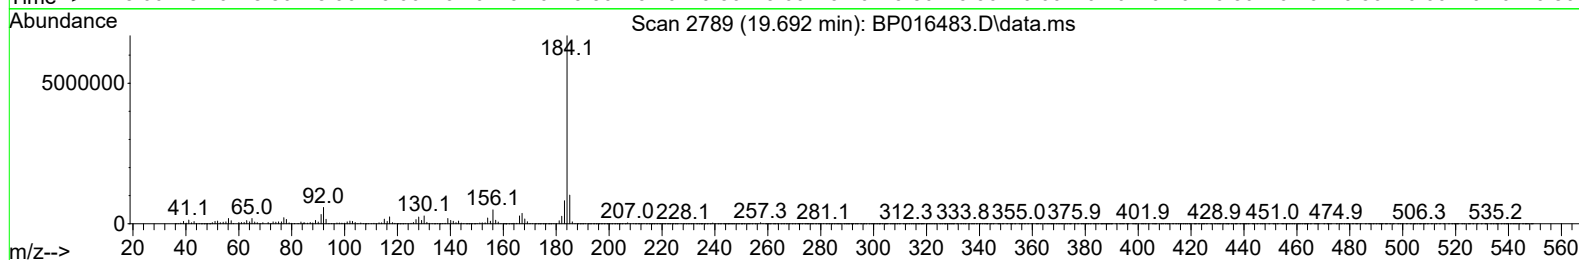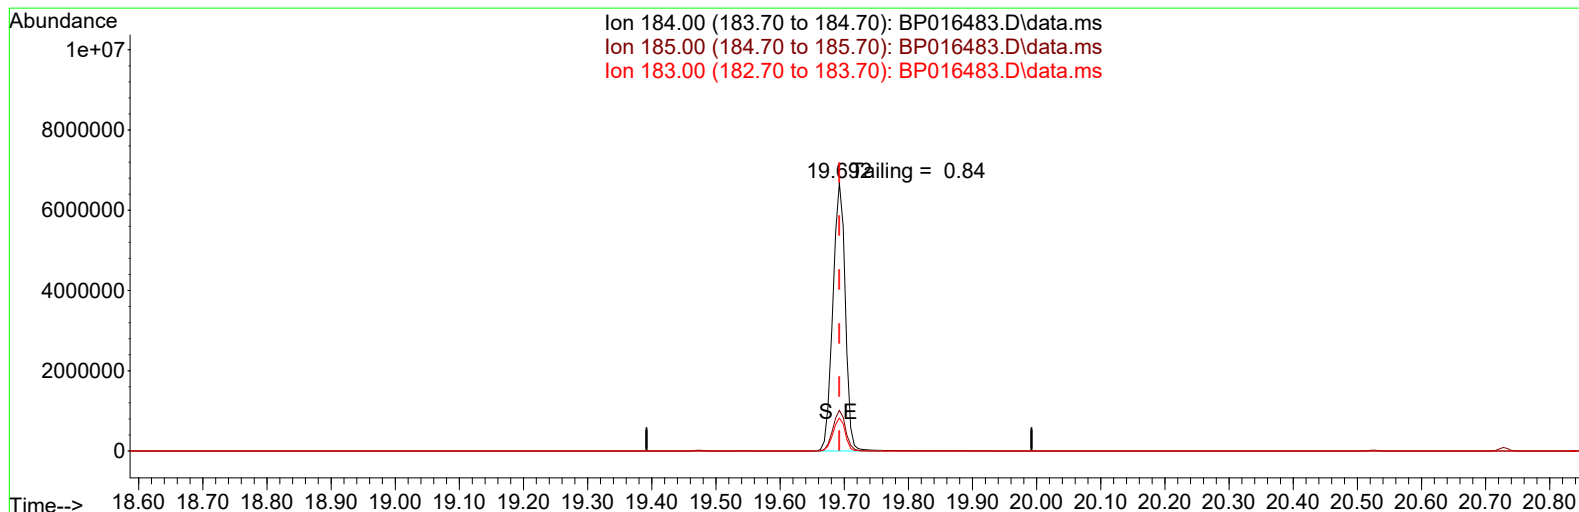

TIC: BP016483.D\data.ms

(77) Benzidine

19.692min (+ 0.000) 9861556.54 ng

response 9061772

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.23
183.00	11.50	12.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2023	BNA_P	<u>BP016483.D</u>
Compound Name	Response	Retention Time
DDT	4193936	20.863
DDD	65380	20.481
DDE	1917	19.928
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
67297	4261233	1.58

Instrument :
BNA_P
ClientSampleId :
DFTPP