

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080423\
 Data File : BP016504.D
 Acq On : 04 Aug 2023 15:46
 Operator : MA/JU
 Sample : PB154583BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK583

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	17	21	28	rVB	146901	205058	1.96%	0.187%
2	3.840	90	94	122	rBV	1824570	2923918	27.92%	2.672%
3	4.170	145	150	157	rVB	23997	42923	0.41%	0.039%
4	4.599	219	223	227	rBV3	6366	13561	0.13%	0.012%
5	4.805	256	258	264	rVB7	8560	10801	0.10%	0.010%
6	5.681	400	407	409	rBV5	10635	17330	0.17%	0.016%
7	6.517	544	549	552	rBV6	9054	16375	0.16%	0.015%
8	7.205	657	666	679	rBV	2169909	3416797	32.63%	3.123%
9	7.405	693	700	711	rVB	1809901	2807486	26.81%	2.566%
10	7.587	723	731	744	rBV	2187247	3430994	32.76%	3.136%
11	8.069	806	813	821	rBV	1373643	2152895	20.56%	1.968%
12	8.269	842	847	849	rBV6	6367	10674	0.10%	0.010%
13	8.769	924	932	946	rBV	2546137	4136942	39.50%	3.781%
14	9.263	1008	1016	1031	rBV	1976863	3186548	30.43%	2.912%
15	9.981	1129	1138	1153	rBV	1522989	2460419	23.50%	2.249%
16	10.505	1219	1227	1241	rBV	2417302	3977259	37.98%	3.635%
17	10.899	1285	1294	1302	rBV	1836313	3041717	29.05%	2.780%
18	11.052	1312	1320	1334	rBV	2492445	4193799	40.05%	3.833%
19	12.475	1558	1562	1569	rBV2	48545	73431	0.70%	0.067%
20	13.569	1741	1748	1754	rBV2	41732	68929	0.66%	0.063%
21	13.687	1763	1768	1773	rVB7	7737	13924	0.13%	0.013%
22	14.128	1833	1843	1855	rBV	4087764	5531337	52.82%	5.056%
23	14.222	1855	1859	1867	rVB	7283	17587	0.17%	0.016%
24	14.416	1885	1892	1910	rBV	4857287	7024119	67.07%	6.420%
25	14.716	1937	1943	1953	rVB	2690204	3824380	36.52%	3.495%
26	14.910	1969	1976	1989	rBV	1860917	2773904	26.49%	2.535%
27	15.710	2105	2112	2119	rBV	6063787	8485051	81.03%	7.755%
28	15.822	2125	2131	2141	rBV	1357771	1867296	17.83%	1.707%
29	15.945	2148	2152	2157	rVB2	26244	35981	0.34%	0.033%
30	16.498	2242	2246	2249	rVB4	8500	12772	0.12%	0.012%
31	17.110	2342	2350	2352	rBV8	5643	12733	0.12%	0.012%
32	17.151	2353	2357	2362	rVB8	10359	16349	0.16%	0.015%
33	17.269	2373	2377	2385	rVB6	8785	19184	0.18%	0.018%
34	17.481	2404	2413	2420	rBV	3188661	4472313	42.71%	4.088%
35	17.581	2424	2430	2446	rVV	6271189	8881217	84.81%	8.117%
36	18.322	2552	2556	2563	rBV3	72488	125268	1.20%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080423\
Data File : BP016504.D
Acq On : 04 Aug 2023 15:46
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Title : SVOA CALIBRATION

37	19.386	2733	2737	2741	rBV	78178	101648	0.97%	0.093%
38	19.451	2744	2748	2752	rVV	75236	95366	0.91%	0.087%
39	19.557	2763	2766	2771	rBV7	37013	60461	0.58%	0.055%
40	19.810	2804	2809	2822	rBV	7410218	10102385	96.47%	9.233%
41	21.580	3105	3110	3115	rBV	3281445	4486594	42.84%	4.101%
42	24.004	3514	3522	3535	rBV2	4995123	10472063	100.00%	9.571%
43	24.174	3544	3551	3562	rVB	2226852	4791698	45.76%	4.380%




Sum of corrected areas: 109411486

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080423\
Data File : BP016504.D
Acq On : 04 Aug 2023 15:46
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

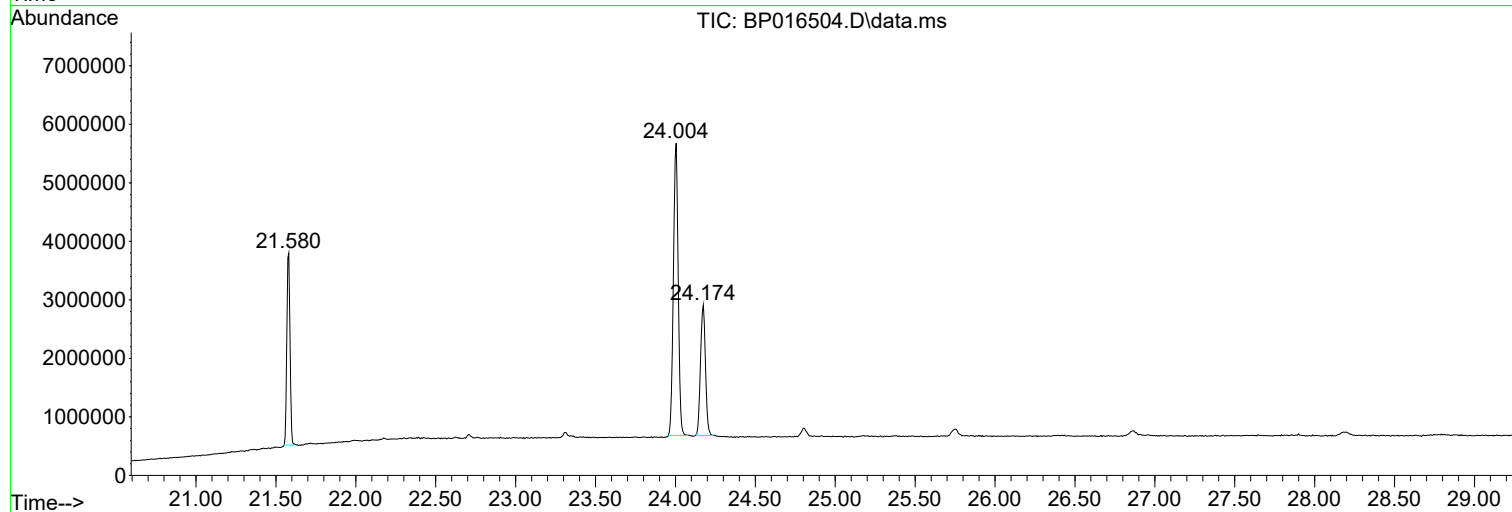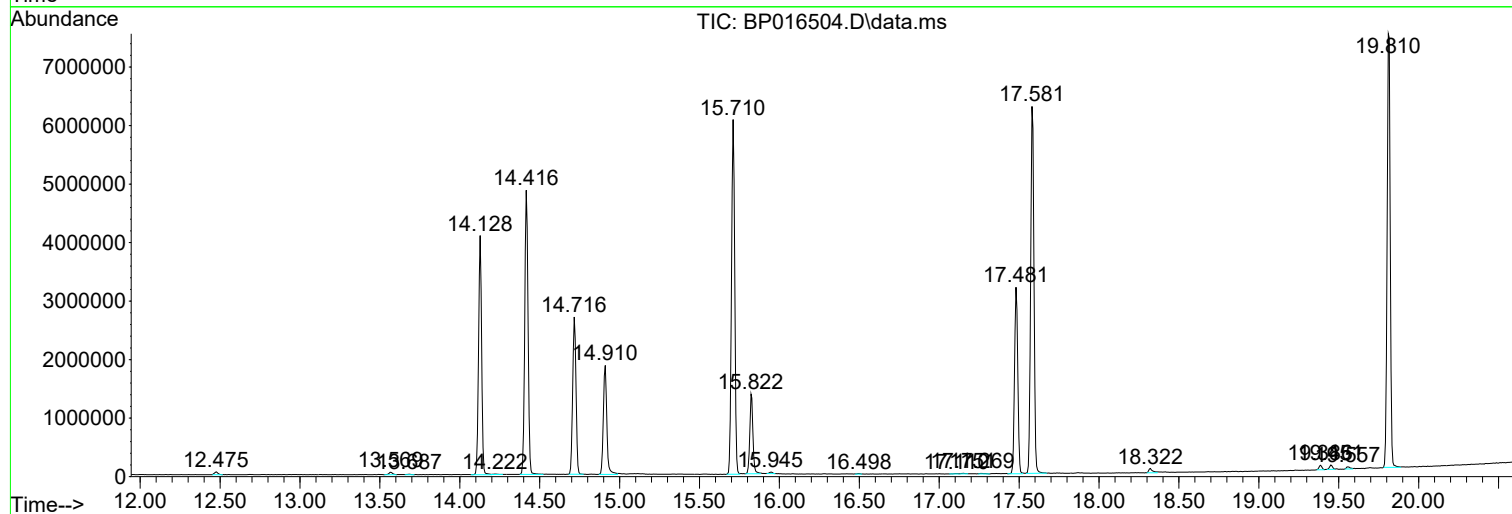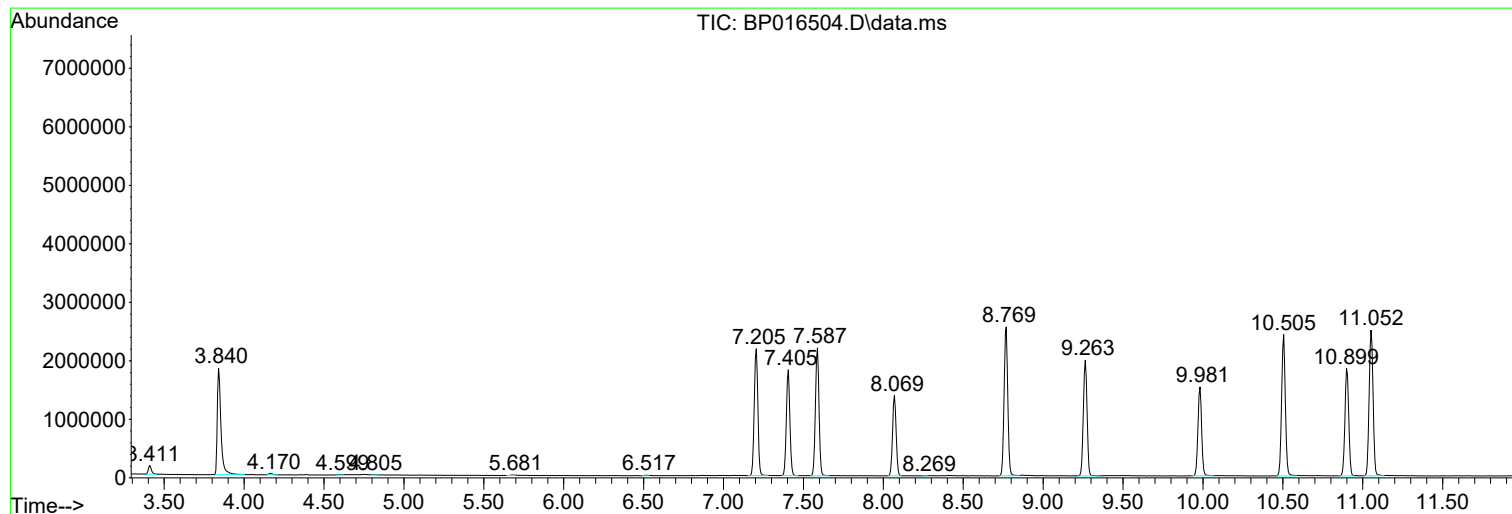

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080423\
Data File : BP016504.D
Acq On : 04 Aug 2023 15:46
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080423\
Data File : BP016504.D
Acq On : 04 Aug 2023 15:46
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------