

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011289.D
 Acq On : 05 Aug 2022 21:16
 Operator : CG/JU
 Sample : N4026-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Aug 05 23:04:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	101194	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	397440	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.269	164	234511	20.000	ng/ul	# 0.00
64) Phenanthrene-d10	17.039	188	484607	20.000	ng/ul	0.00
79) Chrysene-d12	21.163	240	662577	20.000	ng/ul	-0.01
88) Perylene-d12	23.474	264	693258	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.087	96	3031	2.422	ng/uL	0.00
4) Pyridine-d5	3.505	84	25887	7.668	ng/ul	0.00
7) Phenol-d5	6.781	99	28762	3.411	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	197642	32.479	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.128	132	119613	17.401	ng/ul	-0.01
15) 4-Methylphenol-d8	8.316	113	59875	8.629	ng/ul	-0.01
21) Nitrobenzene-d5	8.763	128	143185	50.088	ng/ul	0.00
24) 2-Nitrophenol-d4	9.481	143	90895	33.921	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.016	165	127794	25.009	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131	94425	11.945	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	510996	31.815	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	819389	40.547	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.498	143	7687	2.814	ng/ul	0.00
60) Fluorene-d10	15.269	176	705231	51.602	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.404	200	69457	30.867	ng/ul	-0.01
73) Anthracene-d10	17.139	188	1316351	61.806	ng/ul	0.00
81) Pyrene-d10	19.398	212	1575999	47.045	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.327	264	1583112	45.826	ng/ul	-0.02
Target Compounds						Qvalue
78) Di-n-butylphthalate	18.027	149	260220	8.864	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011289.D
Acq On : 05 Aug 2022 21:16
Operator : CG/JU
Sample : N4026-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Aug 05 23:04:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

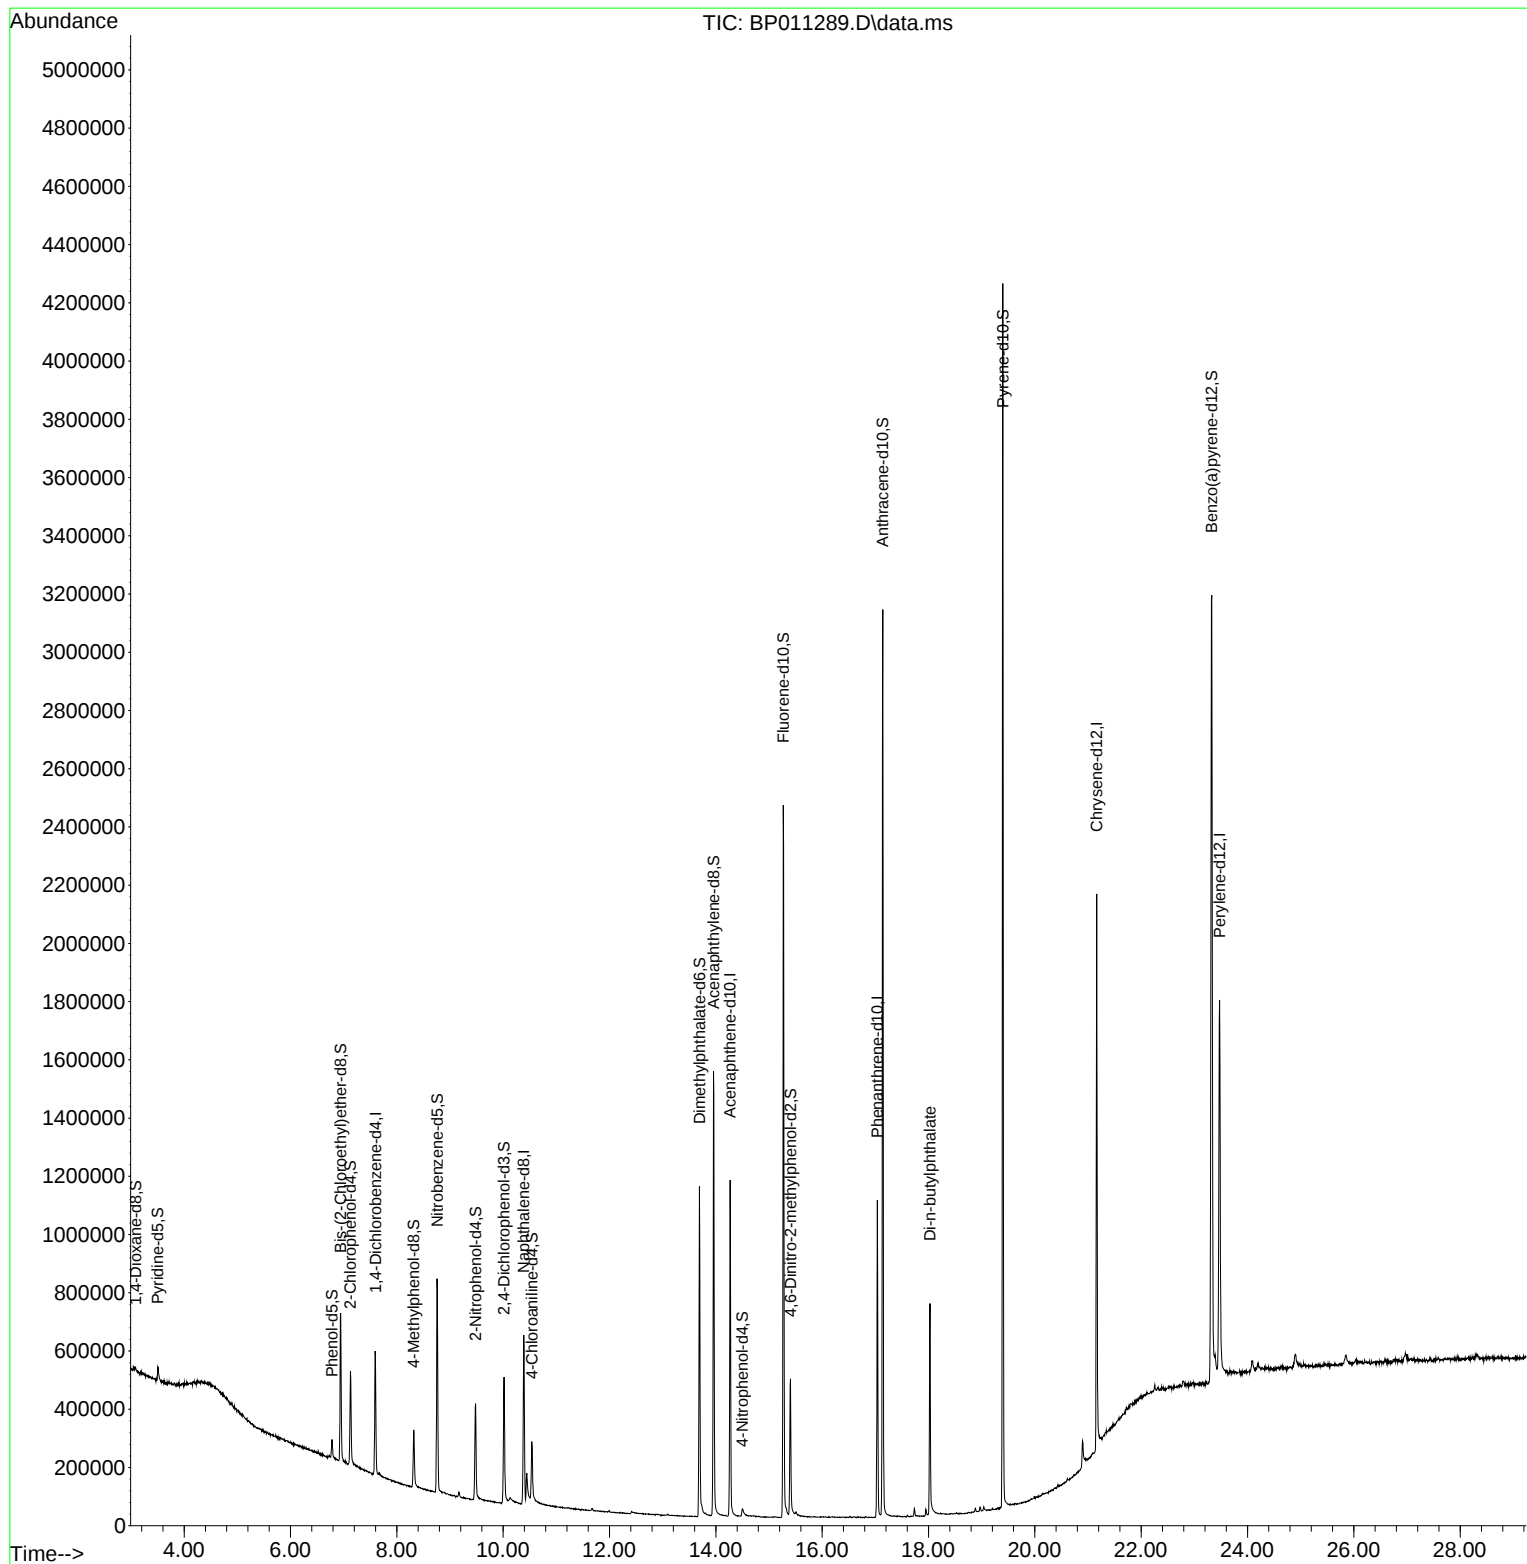

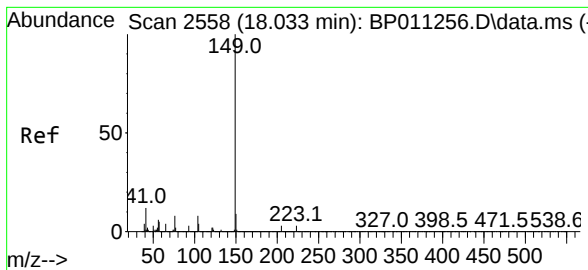

#78
 Di-n-butylphthalate
 Concen: 8.864 ng/ul
 RT: 18.027 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP011289.D
 Acq: 05 Aug 2022 21:16

Instrument :
 BNA_P
 ClientSampleId :

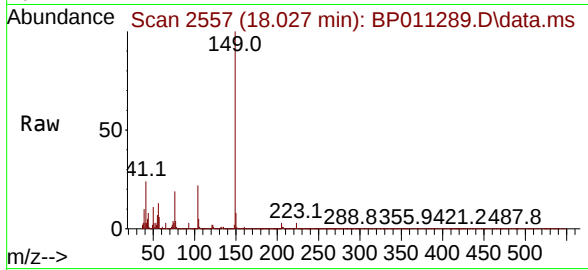

Tgt Ion:149 Resp: 260220
 Ion Ratio Lower Upper
 149 100
 150 8.4 7.4 11.0
 104 22.4 5.1 7.7#

