




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011275.D
Acq On : 05 Aug 2022 12:33
Operator : CG/JU
Sample : N4026-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH1

Manual IntegrationsAPPROVED

Quant Time: Aug 05 23:01:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/08/2022
Supervised By :Sohil Jodhani 08/10/2022

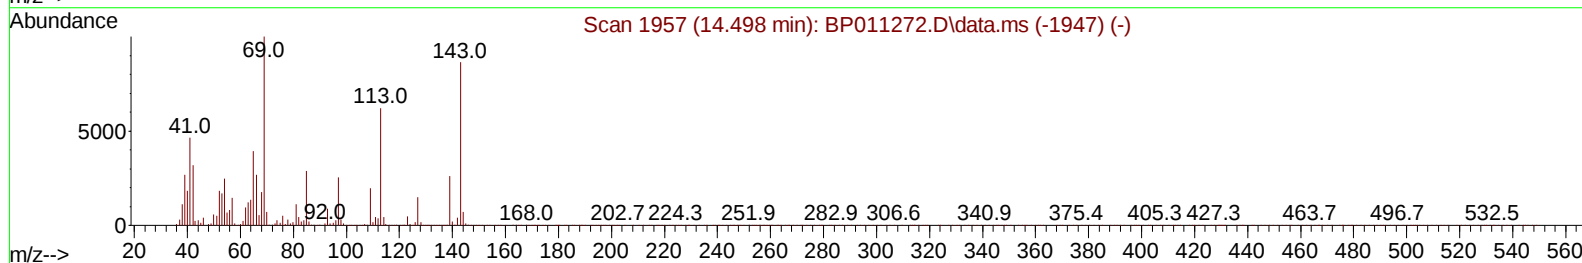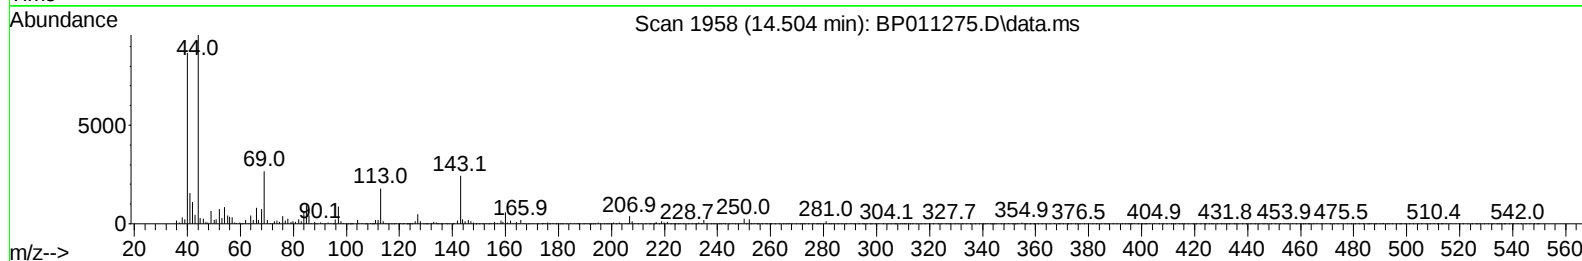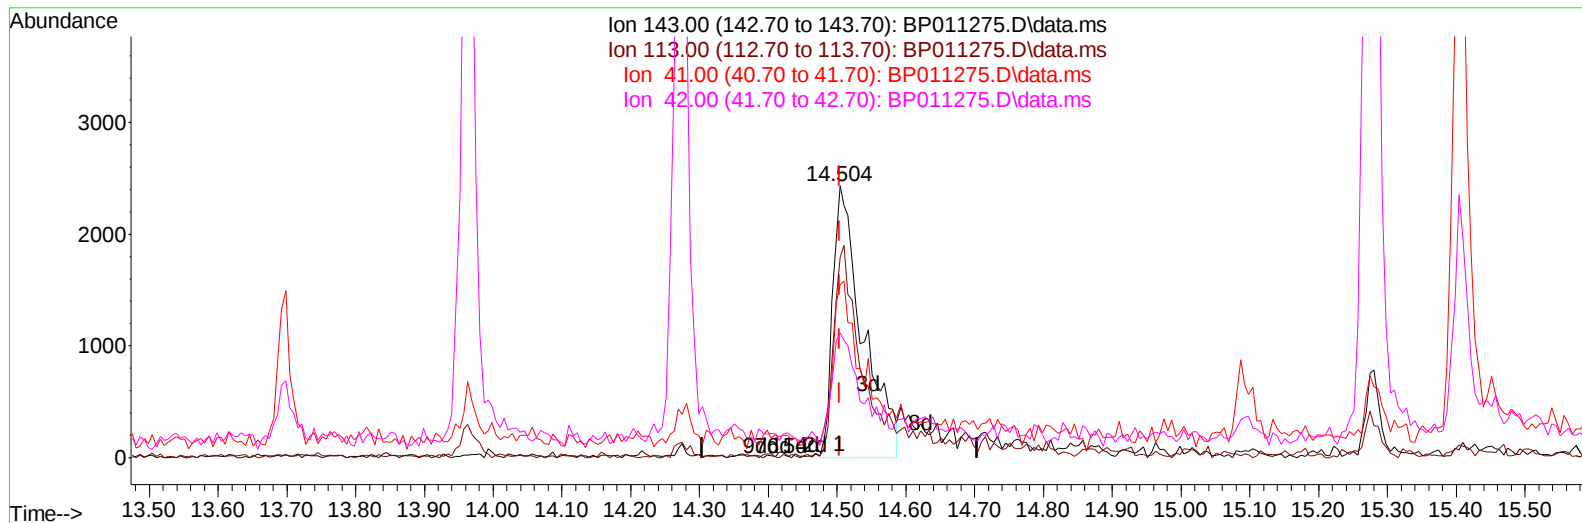

TIC: BP011275.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (0.000) 3.40 ng/ul m

response 7375

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	73.73
41.00	54.40	63.61
42.00	35.50	45.81#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011275.D
 Acq On : 05 Aug 2022 12:33
 Operator : CG/JU
 Sample : N4026-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJH1

Manual IntegrationsAPPROVED

Quant Time: Aug 05 23:01:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/08/2022
 Supervised By :Sohil Jodhani 08/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	87037	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	335056	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	186005	20.000	ng/ul	# 0.00
64) Phenanthrene-d10	17.045	188	388345	20.000	ng/ul	0.00
79) Chrysene-d12	21.169	240	547821	20.000	ng/ul	0.00
88) Perylene-d12	23.486	264	594739	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.087	96	3217	2.988	ng/uL	0.00
4) Pyridine-d5	3.511	84	23112	7.960	ng/ul	0.00
7) Phenol-d5	6.781	99	27040	3.728	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	166733	31.856	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	100946	17.074	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113	43673	7.318	ng/ul	0.00
21) Nitrobenzene-d5	8.763	128	106685	44.268	ng/ul	0.00
24) 2-Nitrophenol-d4	9.481	143	64689	28.636	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	94101	21.844	ng/ul	0.00
31) 4-Chloroaniline-d4	10.546	131	24820	3.724	ng/ul	0.00
46) Dimethylphthalate-d6	13.698	166	365241	28.670	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	558246	34.828	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	7375m	3.404	ng/ul	0.00
60) Fluorene-d10	15.275	176	493881	45.561	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	51721	28.682	ng/ul	0.00
73) Anthracene-d10	17.145	188	769889	45.109	ng/ul	0.00
81) Pyrene-d10	19.404	212	1044057	37.694	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.333	264	1247028	42.077	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011275.D
Acq On : 05 Aug 2022 12:33
Operator : CG/JU
Sample : N4026-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/08/2022
Supervised By :Sohil Jodhani 08/10/2022

Quant Time: Aug 05 23:01:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

