


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011292.D
Acq On : 05 Aug 2022 23:01
Operator : CG/JU
Sample : N4026-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH7

Manual IntegrationsAPPROVED

Quant Time: Aug 06 00:13:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/08/2022
Supervised By :Sohil Jodhani 08/10/2022

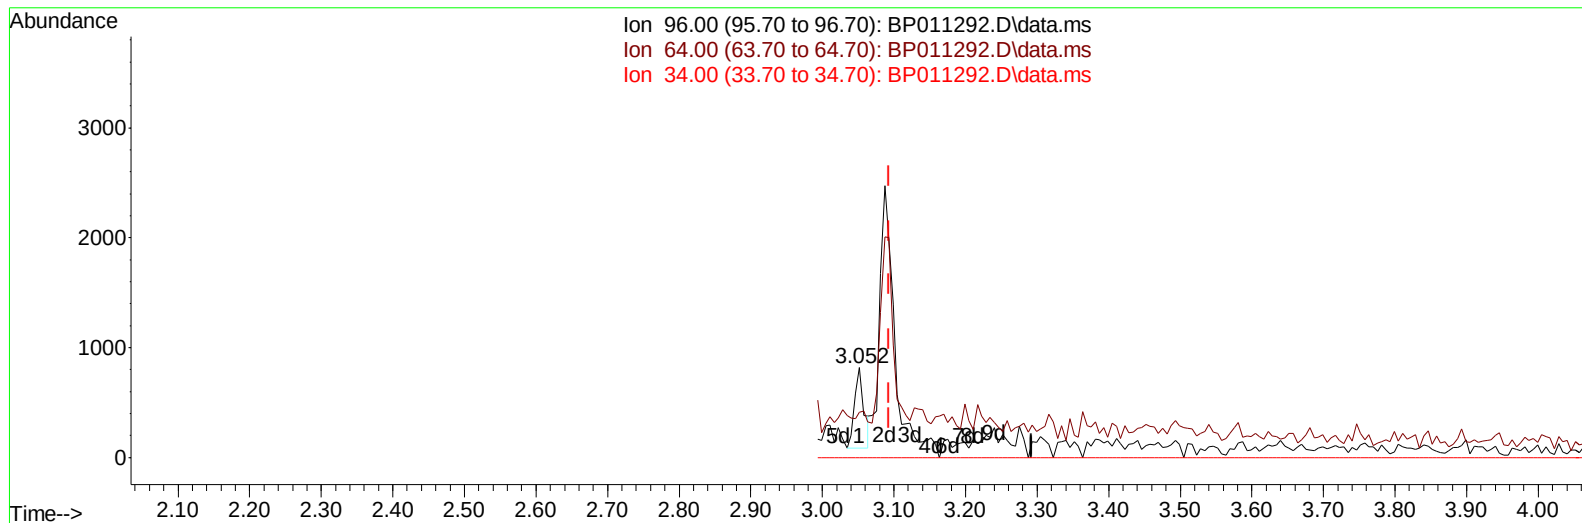




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011292.D
 Acq On : 05 Aug 2022 23:01
 Operator : CG/JU
 Sample : N4026-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJH7

Manual IntegrationsAPPROVED

Quant Time: Aug 06 00:13:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/08/2022
 Supervised By :Sohil Jodhani 08/10/2022

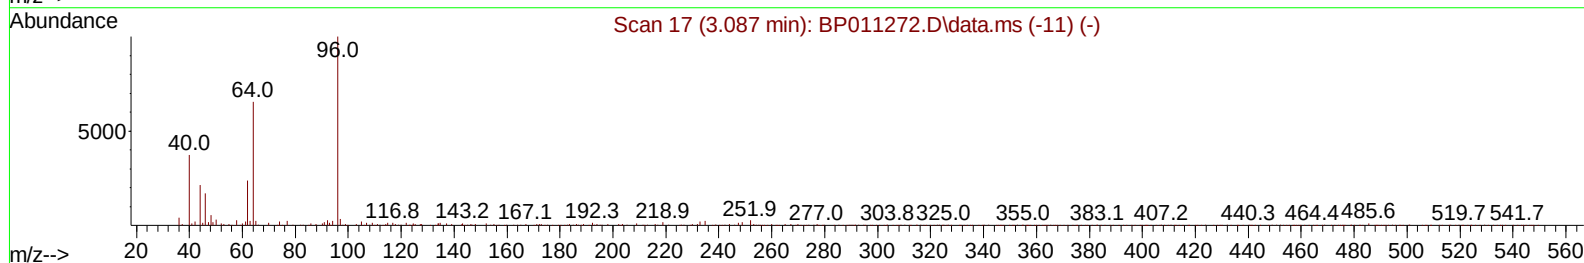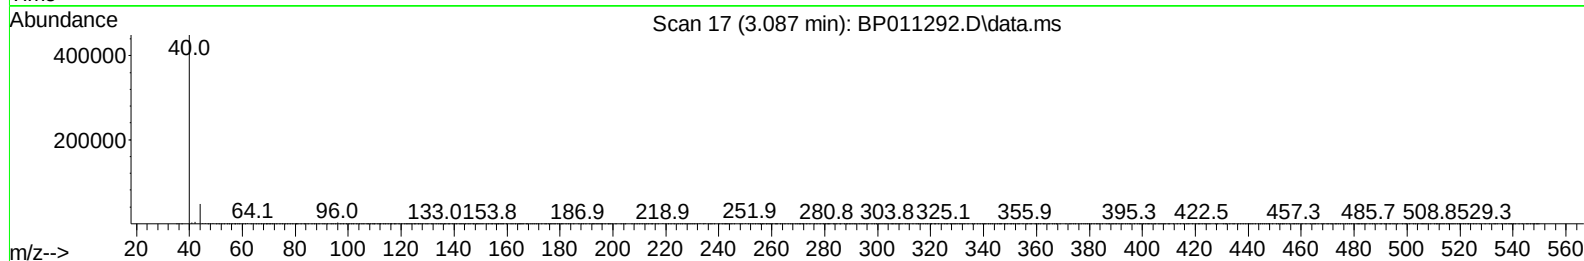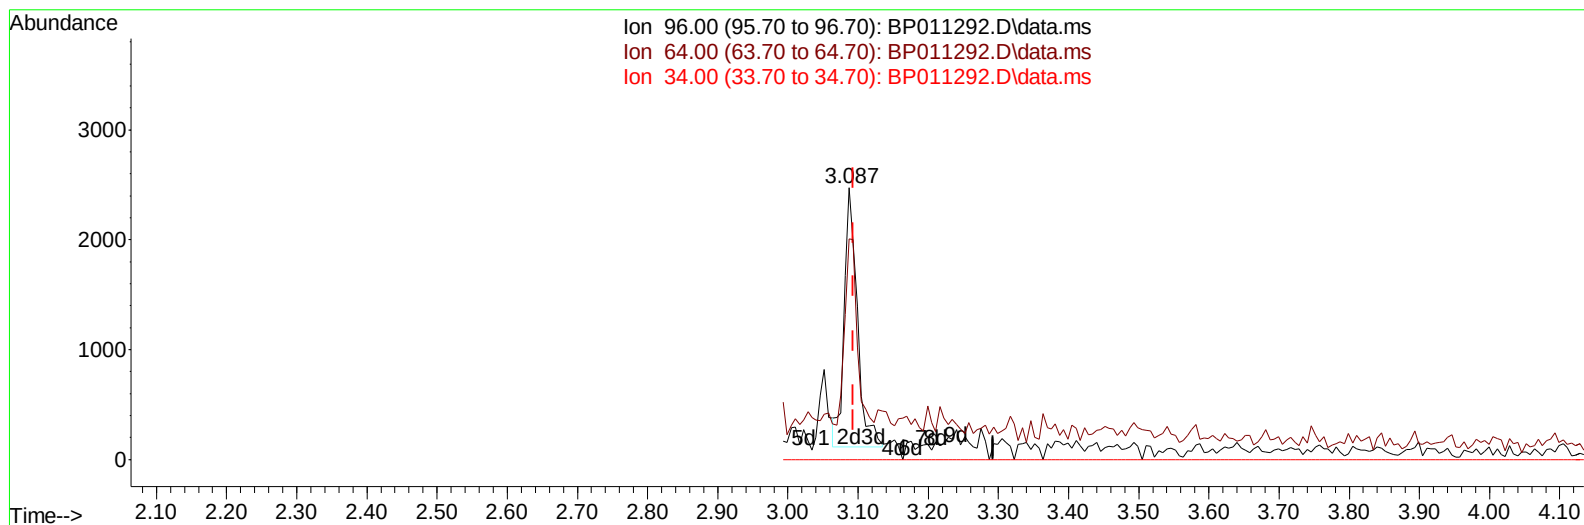

TIC: BP011292.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.087min (-0.006) 2.59 ng/uL m

response 3100

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	81.14#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011292.D
 Acq On : 05 Aug 2022 23:01
 Operator : CG/JU
 Sample : N4026-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJH7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/08/2022
 Supervised By :Sohil Jodhani 08/10/2022

Quant Time: Aug 06 00:13:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	96787	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.387	136	370024	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.269	164	210461	20.000	ng/ul	# 0.00
64) Phenanthrene-d10	17.039	188	411550	20.000	ng/ul	0.00
79) Chrysene-d12	21.163	240	566610	20.000	ng/ul	-0.01
88) Perylene-d12	23.474	264	606299	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.087	96	3100m	2.590	ng/uL	0.00
4) Pyridine-d5	3.505	84	21685	6.716	ng/ul	0.00
7) Phenol-d5	6.781	99	26288	3.259	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	176675	30.355	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.128	132	110418	16.795	ng/ul	-0.01
15) 4-Methylphenol-d8	8.316	113	54967	8.282	ng/ul	-0.01
21) Nitrobenzene-d5	8.757	128	131944	49.575	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.481	143	83467	33.457	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.016	165	114044	23.972	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131	57352	7.792	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	406431	28.196	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	670650	36.979	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.498	143	6362	2.595	ng/ul	0.00
60) Fluorene-d10	15.269	176	602767	49.145	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.404	200	73506	38.465	ng/ul	-0.01
73) Anthracene-d10	17.133	188	1209265	66.857	ng/ul	-0.01
81) Pyrene-d10	19.398	212	1344892	46.945	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.321	264	1351547	44.734	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011292.D
Acq On : 05 Aug 2022 23:01
Operator : CG/JU
Sample : N4026-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/08/2022
Supervised By :Sohil Jodhani 08/10/2022

Quant Time: Aug 06 00:13:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

