

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011278.D
 Acq On : 05 Aug 2022 14:51
 Operator : CG/JU
 Sample : N4026-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJH4

Quant Time: Aug 05 23:02:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	91370	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	350707	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	189976	20.000	ng/u1	# 0.00
64) Phenanthrene-d10	17.045	188	395419	20.000	ng/u1	0.00
79) Chrysene-d12	21.169	240	556104	20.000	ng/u1	0.00
88) Perylene-d12	23.486	264	629447	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	4088	3.618	ng/uL	0.00
4) Pyridine-d5	3.499	84	76571	25.121	ng/u1	0.00
7) Phenol-d5	6.781	99	185866	24.410	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	184912	33.654	ng/u1	0.00
11) 2-Chlorophenol-d4	7.134	132	157820	25.428	ng/u1	0.00
15) 4-Methylphenol-d8	8.322	113	154353	24.636	ng/u1	0.00
21) Nitrobenzene-d5	8.763	128	118524	46.986	ng/u1	0.00
24) 2-Nitrophenol-d4	9.481	143	79606	33.667	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	128679	28.538	ng/u1	0.00
31) 4-Chloroaniline-d4	10.546	131	67077	9.616	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	439773	33.799	ng/u1	0.00
49) Acenaphthylene-d8	13.963	160	648148	39.592	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	64970	29.364	ng/u1	0.00
60) Fluorene-d10	15.275	176	589646	53.259	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	69486	37.845	ng/u1	-0.01
73) Anthracene-d10	17.145	188	1148960	66.114	ng/u1	0.00
81) Pyrene-d10	19.404	212	1271267	45.214	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.339	264	1398528	44.587	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.123	88	3641	3.494	ng/uL#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011278.D
Acq On : 05 Aug 2022 14:51
Operator : CG/JU
Sample : N4026-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH4

Quant Time: Aug 05 23:02:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

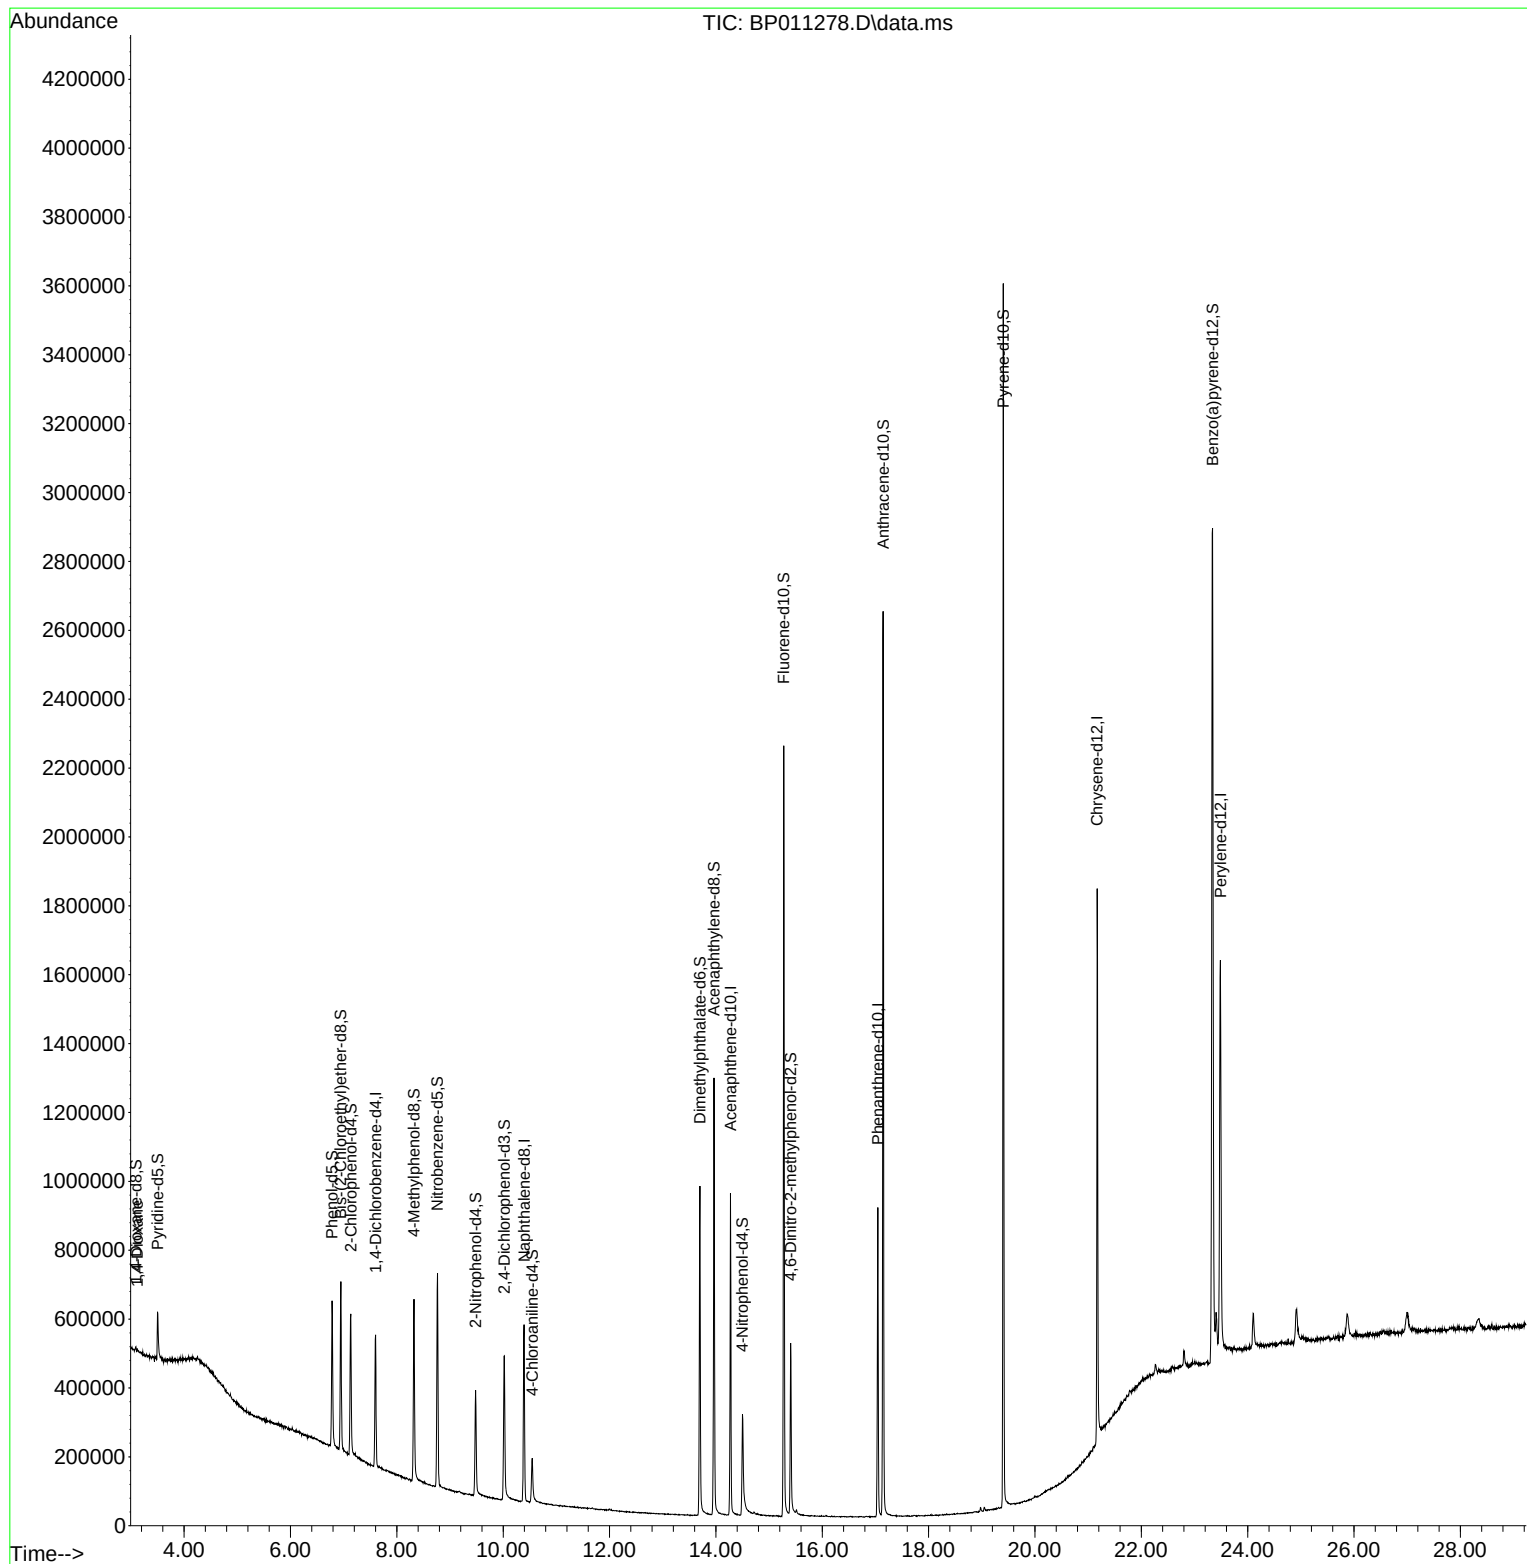

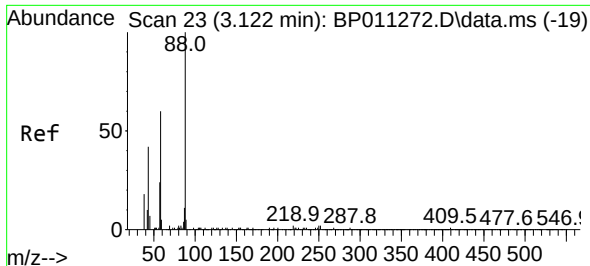

#2
 1,4-Dioxane
 Concen: 3.494 ng/uL
 RT: 3.123 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BP011278.D
 Acq: 05 Aug 2022 14:51

Instrument :
 BNA_P
 ClientSampleId :
 GBJH4

Tgt Ion: 88 Resp: 3641
 Ion Ratio Lower Upper
 88 100
 43 0.0 29.6 44.4#
 58 58.1 49.1 73.7

