

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011274.D
 Acq On : 05 Aug 2022 11:58
 Operator : CG/JU
 Sample : PB146743BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK743

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	85	88	100	rBV	126262	205869	4.28%	0.560%
2	6.781	641	645	658	rVB	526286	783621	16.29%	2.133%
3	6.946	668	673	681	rVB	608514	874926	18.19%	2.381%
4	7.134	700	705	714	rVB	525625	800068	16.63%	2.178%
5	7.599	779	784	793	rVB	482523	729245	15.16%	1.985%
6	8.322	901	907	920	rBV	654046	955823	19.87%	2.602%
7	8.763	976	982	994	rVB	787614	1184283	24.62%	3.223%
8	9.481	1098	1104	1114	rBV	372392	603288	12.54%	1.642%
9	10.022	1189	1196	1214	rBV	530763	926923	19.27%	2.523%
10	10.392	1252	1259	1268	rBV	647662	977095	20.31%	2.660%
11	10.545	1278	1285	1296	rBV	555823	876940	18.23%	2.387%
12	13.698	1814	1821	1834	rBV	1172963	1501488	31.21%	4.087%
13	13.963	1859	1866	1883	rBV	1673587	1998750	41.55%	5.440%
14	14.275	1912	1919	1928	rBV	1178634	1425856	29.64%	3.881%
15	14.504	1951	1958	1979	rBV	342275	723737	15.04%	1.970%
16	15.275	2083	2089	2105	rBV	2492643	2904299	60.37%	7.905%
17	15.410	2105	2112	2125	rVV	483176	753704	15.67%	2.051%
18	15.510	2127	2129	2136	rVB5	14244	23162	0.48%	0.063%
19	16.075	2218	2225	2228	rVB6	3753	8731	0.18%	0.024%
20	17.045	2382	2390	2400	rBV	1118064	1332932	27.71%	3.628%
21	17.139	2400	2406	2427	rVB	2854412	3653873	75.95%	9.945%
22	18.980	2715	2719	2724	rVB4	11523	15503	0.32%	0.042%
23	19.051	2727	2731	2735	rVV3	11077	15665	0.33%	0.043%
24	19.404	2785	2791	2802	rBV	3734882	4134230	85.94%	11.253%
25	21.168	3087	3091	3103	rBV	1809436	2211298	45.97%	6.019%
26	23.339	3453	3460	3470	rBV2	2585264	4810706	100.00%	13.094%
27	23.486	3479	3485	3498	rVB	1218033	2307703	47.97%	6.281%




Sum of corrected areas: 36739718

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011274.D
Acq On : 05 Aug 2022 11:58
Operator : CG/JU
Sample : PB146743BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK743

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

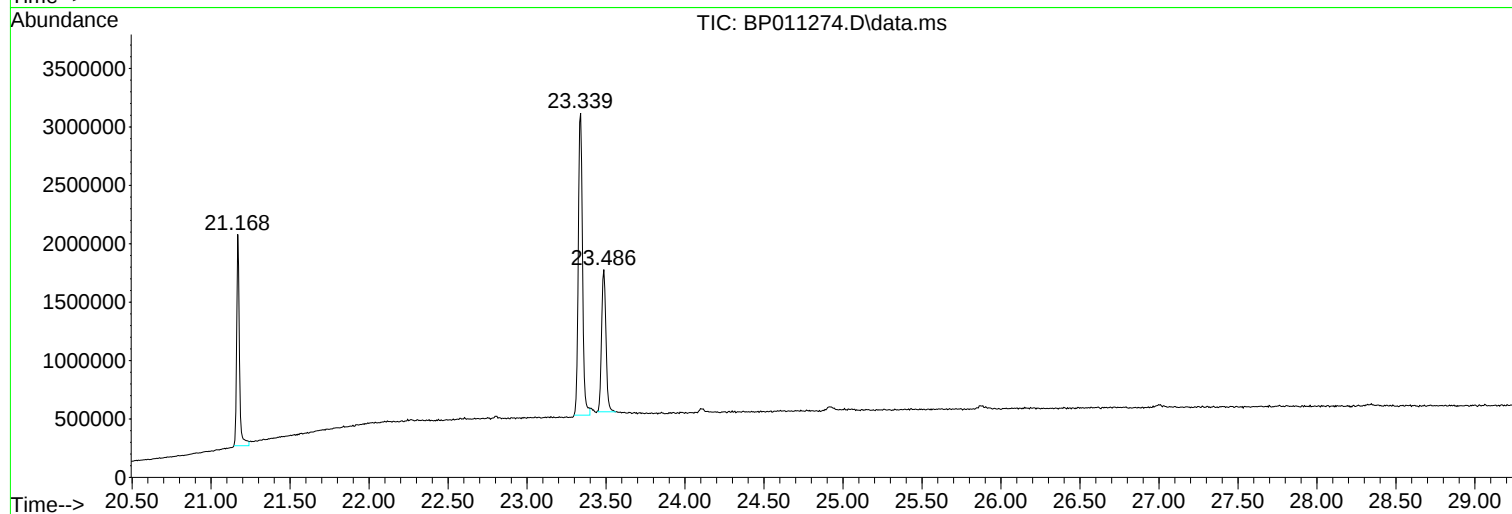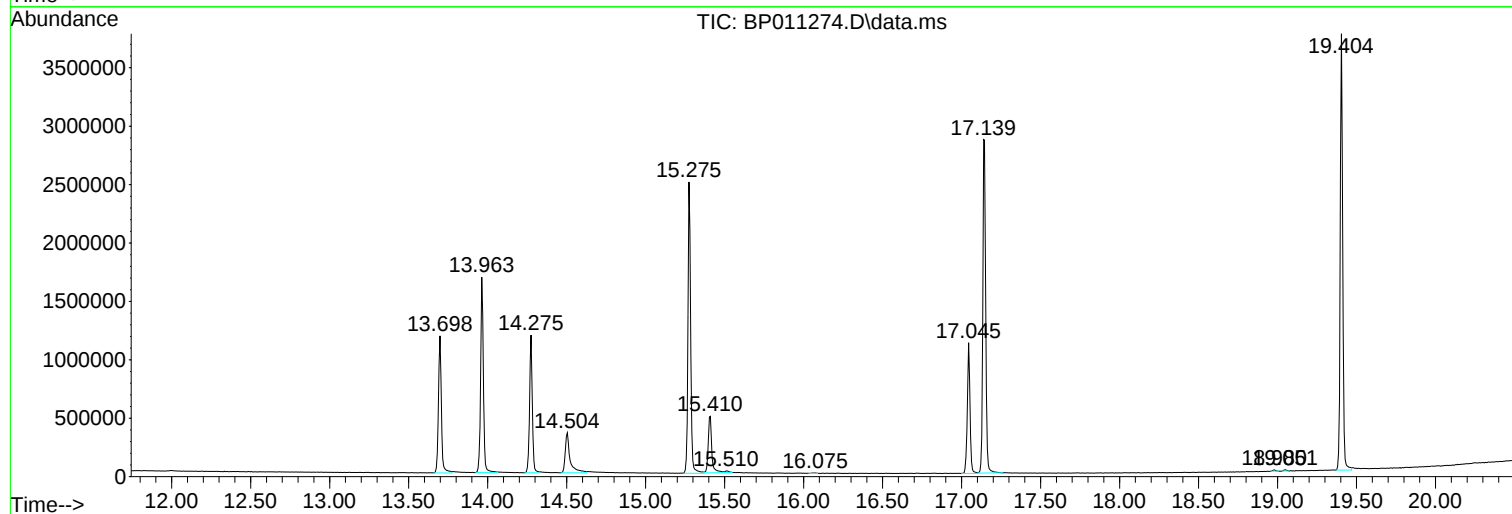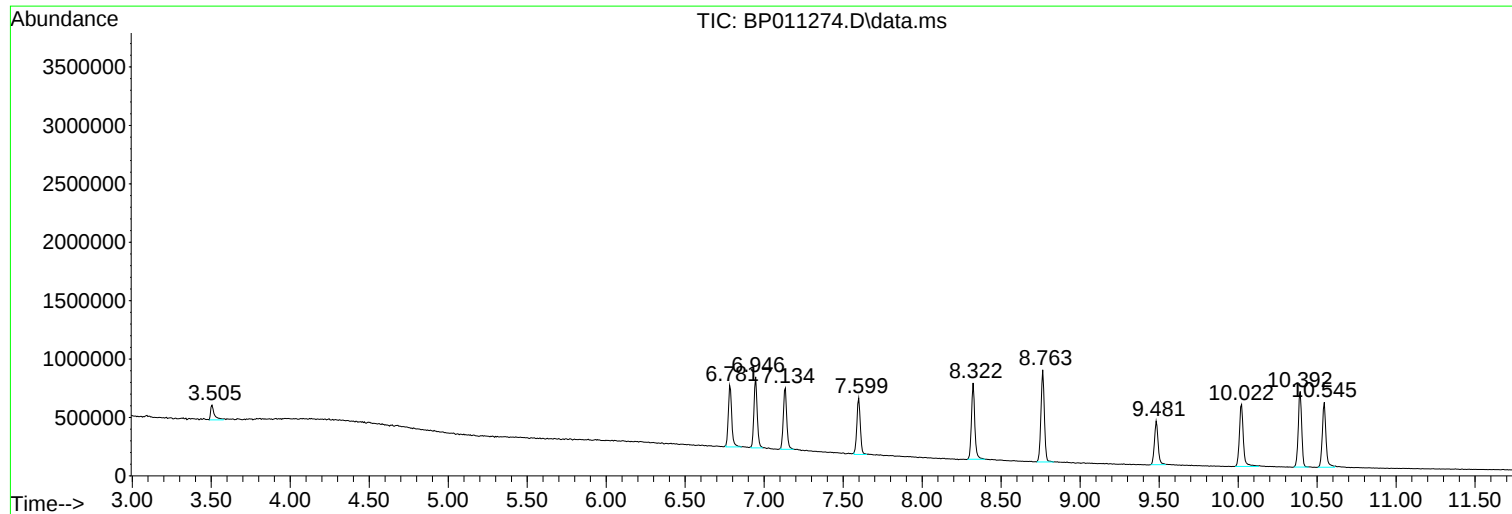

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011274.D
Acq On : 05 Aug 2022 11:58
Operator : CG/JU
Sample : PB146743BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK743

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011274.D
Acq On : 05 Aug 2022 11:58
Operator : CG/JU
Sample : PB146743BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK743

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------