

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011276.D
 Acq On : 05 Aug 2022 13:07
 Operator : CG/JU
 Sample : N4026-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	668	673	687	rVB	437472	679175	16.61%	2.425%
2	7.134	700	705	714	rVB	261701	416891	10.20%	1.488%
3	7.599	779	784	795	rVB	394802	616676	15.08%	2.202%
4	8.322	902	907	919	rVB	166765	288744	7.06%	1.031%
5	8.763	976	982	990	rVB	583360	893020	21.84%	3.188%
6	9.481	1098	1104	1116	rBV	259651	438174	10.72%	1.564%
7	10.016	1189	1195	1208	rBV	313002	563422	13.78%	2.011%
8	10.393	1252	1259	1270	rVB	536774	819464	20.04%	2.926%
9	10.546	1279	1285	1303	rVB	98329	207237	5.07%	0.740%
10	13.698	1814	1821	1834	rBV	771865	1100975	26.93%	3.931%
11	13.963	1859	1866	1880	rBV	1106619	1418933	34.71%	5.066%
12	14.275	1912	1919	1933	rBV	977022	1269681	31.06%	4.533%
13	14.504	1954	1958	1971	rBV4	20769	57127	1.40%	0.204%
14	15.092	2051	2058	2063	rBV2	8725	13835	0.34%	0.049%
15	15.275	2081	2089	2105	rBV	1921890	2296337	56.17%	8.198%
16	15.404	2105	2111	2127	rVV	380253	590580	14.45%	2.108%
17	15.516	2127	2130	2134	rVB4	9950	14881	0.36%	0.053%
18	16.528	2297	2302	2309	rBV9	3660	6592	0.16%	0.024%
19	16.822	2350	2352	2359	rVB5	2933	5066	0.12%	0.018%
20	17.045	2383	2390	2401	rBV	951287	1162467	28.43%	4.150%
21	17.145	2401	2407	2422	rVV	2572390	3206222	78.42%	11.447%
22	18.033	2552	2558	2562	rBV4	6270	9938	0.24%	0.035%
23	18.528	2640	2642	2645	rBV4	3753	4553	0.11%	0.016%
24	18.980	2716	2719	2723	rVB4	10554	13863	0.34%	0.049%
25	19.045	2728	2730	2734	rVB	8895	10986	0.27%	0.039%
26	19.404	2785	2791	2805	rBV	3411319	3666880	89.69%	13.091%
27	21.169	3087	3091	3099	rBV	1656738	1995189	48.80%	7.123%
28	23.339	3454	3460	3469	rBV	2274207	4088368	100.00%	14.596%
29	23.486	3479	3485	3497	rVB	1172714	2155225	52.72%	7.694%




Sum of corrected areas: 28010501

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011276.D
Acq On : 05 Aug 2022 13:07
Operator : CG/JU
Sample : N4026-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

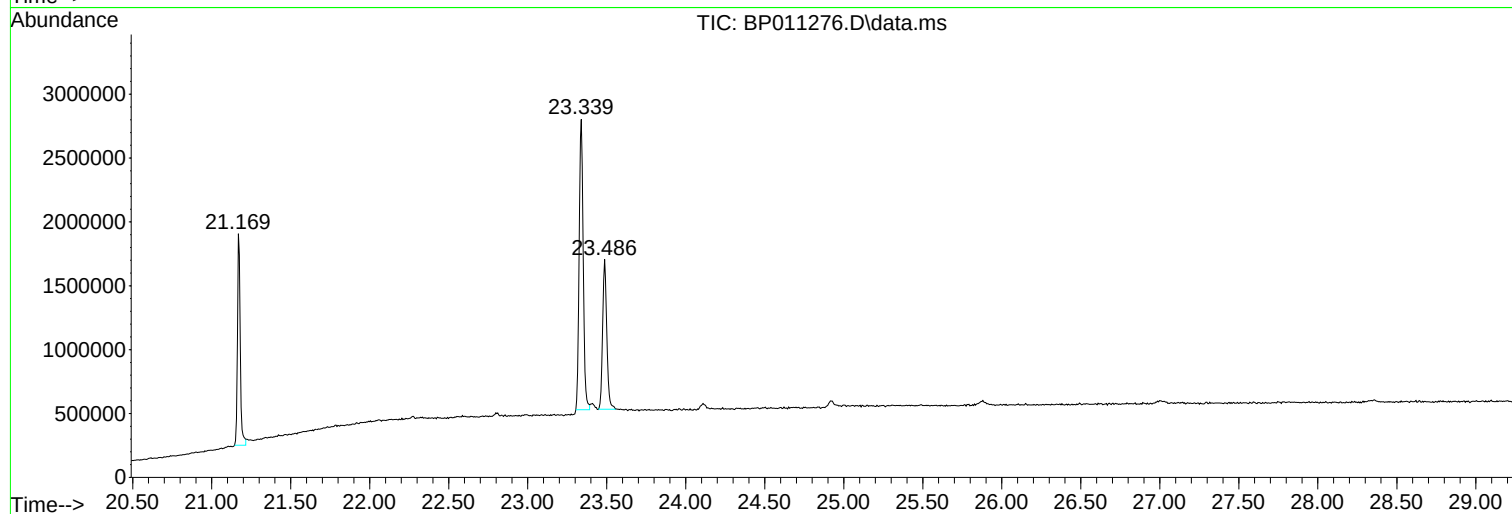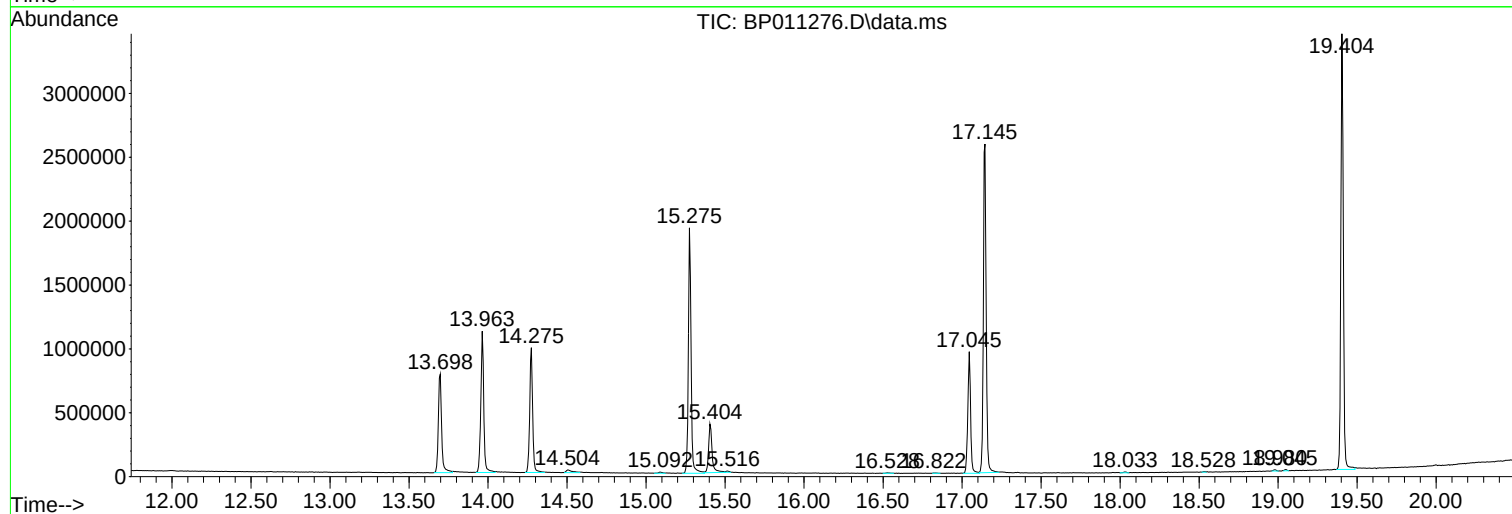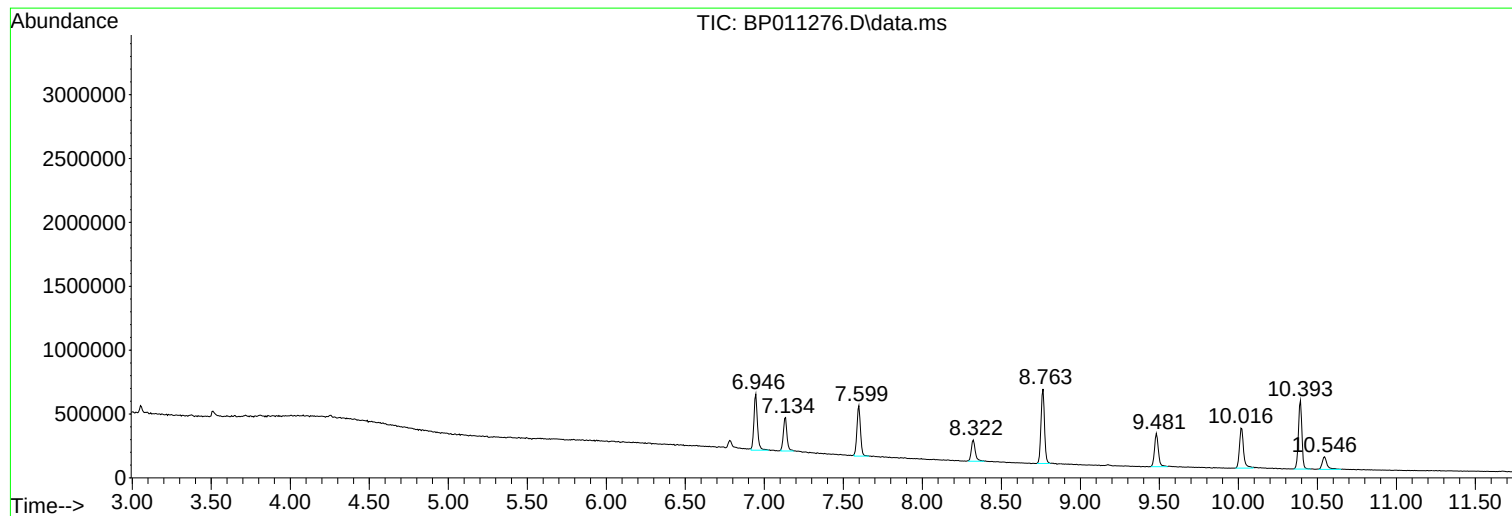

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011276.D
Acq On : 05 Aug 2022 13:07
Operator : CG/JU
Sample : N4026-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011276.D
Acq On : 05 Aug 2022 13:07
Operator : CG/JU
Sample : N4026-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
