

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011281.D
 Acq On : 05 Aug 2022 16:37
 Operator : CG/JU
 Sample : N4026-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	668	673	684	rVB	507845	770341	19.56%	2.759%
2	7.128	700	704	715	rVB	314403	503406	12.78%	1.803%
3	7.599	778	784	793	rVB	517453	806139	20.47%	2.887%
4	8.322	902	907	919	rVB	177500	318162	8.08%	1.139%
5	8.763	976	982	992	rVB	638615	996860	25.32%	3.570%
6	9.481	1098	1104	1116	rBV	286598	482404	12.25%	1.728%
7	10.016	1189	1195	1218	rVB	349093	633921	16.10%	2.270%
8	10.387	1252	1258	1265	rBV	666404	1008768	25.62%	3.613%
9	10.546	1279	1285	1297	rVB	88470	171038	4.34%	0.613%
10	13.693	1814	1820	1835	rBV	727045	1055843	26.81%	3.781%
11	13.963	1859	1866	1879	rBV	1029335	1325064	33.65%	4.746%
12	14.275	1911	1919	1928	rBV	1010270	1355019	34.41%	4.853%
13	14.510	1952	1959	1966	rBV4	19594	49138	1.25%	0.176%
14	15.087	2053	2057	2064	rBV5	7588	13645	0.35%	0.049%
15	15.275	2080	2089	2105	rBV	1768230	2101403	53.37%	7.526%
16	15.404	2105	2111	2126	rVV	352710	557742	14.16%	1.998%
17	15.516	2127	2130	2139	rVB7	10414	21589	0.55%	0.077%
18	15.898	2189	2195	2197	rBV5	4034	6359	0.16%	0.023%
19	16.057	2220	2222	2229	rVB7	3986	6236	0.16%	0.022%
20	16.522	2297	2301	2305	rVV5	3745	4354	0.11%	0.016%
21	16.822	2350	2352	2358	rVB7	2571	4083	0.10%	0.015%
22	17.045	2384	2390	2400	rBV	869246	1123973	28.54%	4.025%
23	17.140	2400	2406	2421	rVV	2252264	2752231	69.89%	9.857%
24	17.345	2436	2441	2444	rBV5	3433	4482	0.11%	0.016%
25	17.610	2482	2486	2489	rBV4	4202	6511	0.17%	0.023%
26	17.681	2491	2498	2503	rVV9	6859	13049	0.33%	0.047%
27	17.739	2503	2508	2509	rBV4	2822	4013	0.10%	0.014%
28	17.957	2541	2545	2550	rBV6	11182	15423	0.39%	0.055%
29	18.028	2552	2557	2560	rBV2	9737	11649	0.30%	0.042%
30	18.975	2715	2718	2722	rBV4	9825	12192	0.31%	0.044%
31	19.045	2727	2730	2734	rBV3	9377	10920	0.28%	0.039%
32	19.404	2785	2791	2807	rBV	3052274	3347698	85.02%	11.990%
33	20.904	3042	3046	3052	rBV7	79060	160073	4.07%	0.573%
34	21.169	3086	3091	3100	rBV	1754683	2110178	53.59%	7.557%
35	23.333	3453	3459	3468	rBV	2166930	3937685	100.00%	14.103%
36	23.480	3478	3484	3497	rVB	1217411	2220090	56.38%	7.951%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011281.D
Acq On : 05 Aug 2022 16:37
Operator : CG/JU
Sample : N4026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 27921681

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011281.D
Acq On : 05 Aug 2022 16:37
Operator : CG/JU
Sample : N4026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

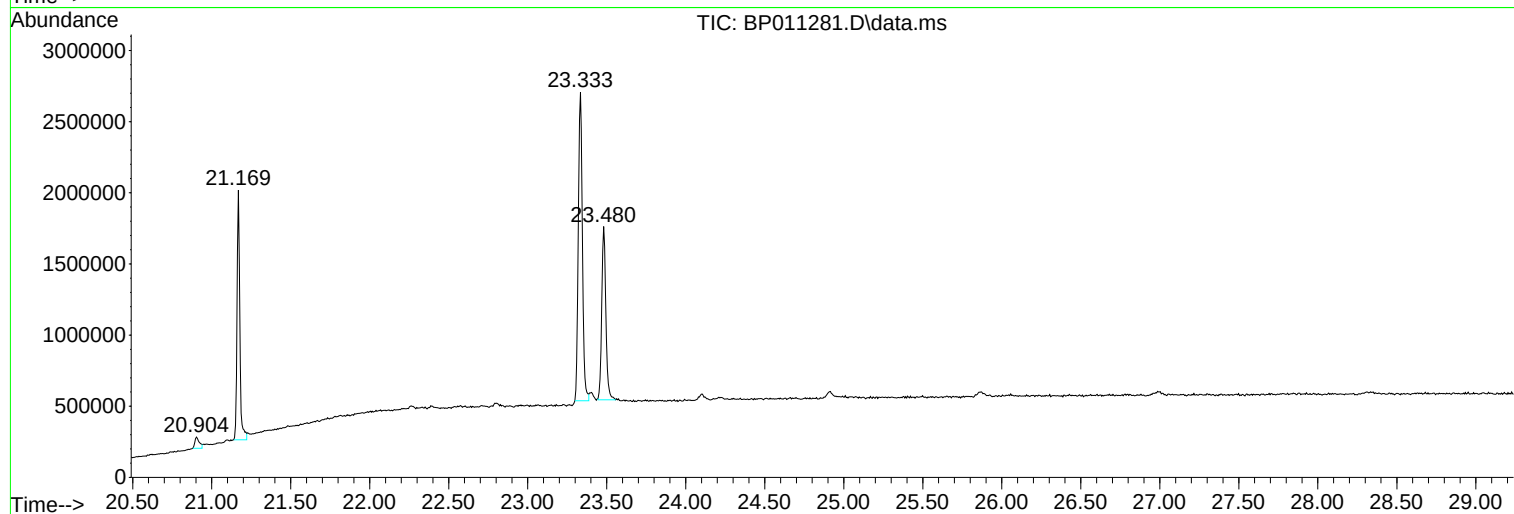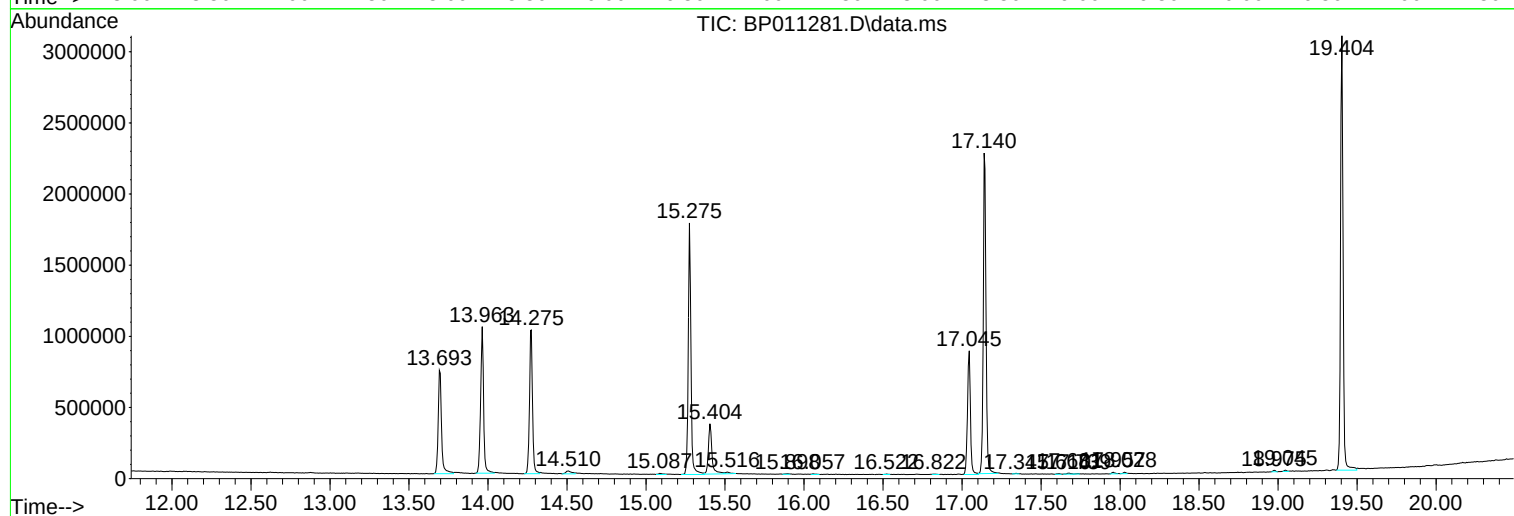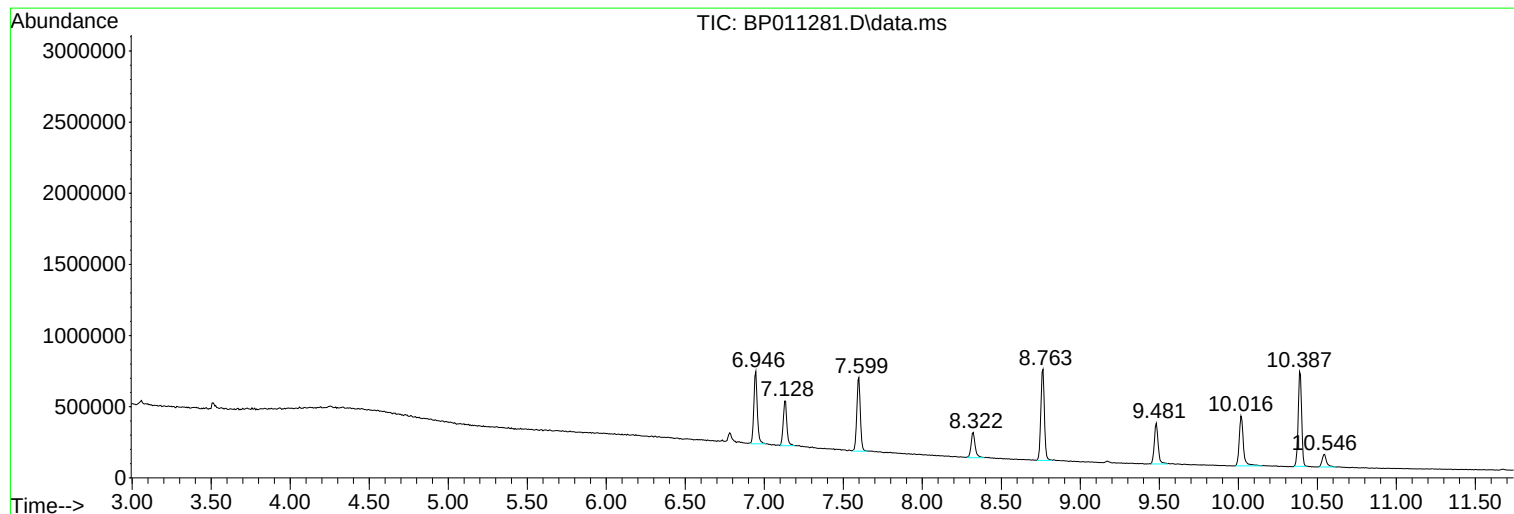

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011281.D
Acq On : 05 Aug 2022 16:37
Operator : CG/JU
Sample : N4026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011281.D
Acq On : 05 Aug 2022 16:37
Operator : CG/JU
Sample : N4026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc