

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011282.D
 Acq On : 05 Aug 2022 17:12
 Operator : CG/JU
 Sample : N4026-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	668	673	683	rVB	460699	697151	16.98%	2.602%
2	7.128	700	704	714	rVB	277549	452028	11.01%	1.687%
3	7.599	778	784	795	rVB	440056	702384	17.11%	2.621%
4	8.322	902	907	918	rVB	153374	265103	6.46%	0.989%
5	8.763	976	982	989	rVB	599644	940719	22.92%	3.511%
6	9.481	1098	1104	1118	rVB	277214	465709	11.35%	1.738%
7	10.016	1189	1195	1216	rVB	322642	580115	14.13%	2.165%
8	10.387	1252	1258	1266	rVB	576092	876984	21.36%	3.273%
9	10.540	1279	1284	1294	rBV	88496	172383	4.20%	0.643%
10	12.875	1679	1681	1686	rBV6	2766	4248	0.10%	0.016%
11	13.692	1814	1820	1843	rBV	689774	1020945	24.87%	3.810%
12	13.963	1858	1866	1879	rBV	985600	1285295	31.31%	4.797%
13	14.275	1911	1919	1930	rBV	916447	1238654	30.17%	4.623%
14	14.504	1953	1958	1967	rBV3	19462	53178	1.30%	0.198%
15	15.086	2054	2057	2061	rBV3	10055	13342	0.33%	0.050%
16	15.275	2079	2089	2105	rBV	1703143	2046975	49.87%	7.639%
17	15.404	2105	2111	2125	rVV	385603	580365	14.14%	2.166%
18	15.510	2127	2129	2136	rVB5	10994	18203	0.44%	0.068%
19	16.522	2296	2301	2307	rVB5	3747	7057	0.17%	0.026%
20	16.816	2348	2351	2355	rVB5	3312	4571	0.11%	0.017%
21	17.045	2382	2390	2400	rBV	761064	1022684	24.91%	3.817%
22	17.139	2400	2406	2425	rVB	2323208	2772997	67.55%	10.349%
23	17.345	2439	2441	2445	rBV3	5053	5344	0.13%	0.020%
24	17.610	2480	2486	2490	rBV9	3876	5808	0.14%	0.022%
25	17.951	2539	2544	2550	rBV8	6859	12771	0.31%	0.048%
26	18.027	2554	2557	2561	rVV2	7247	9921	0.24%	0.037%
27	18.427	2620	2625	2628	rBV7	4672	8458	0.21%	0.032%
28	18.974	2715	2718	2724	rBV7	9835	14353	0.35%	0.054%
29	19.045	2727	2730	2734	rVB3	8110	11485	0.28%	0.043%
30	19.404	2785	2791	2803	rBV	3180621	3381471	82.38%	12.620%
31	21.168	3086	3091	3100	rBV	1658864	1937887	47.21%	7.232%
32	23.333	3452	3459	3468	rBV	2277756	4104961	100.00%	15.320%
33	23.480	3478	3484	3498	rVB	1131654	2081514	50.71%	7.768%




Sum of corrected areas: 26795063

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011282.D
Acq On : 05 Aug 2022 17:12
Operator : CG/JU
Sample : N4026-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

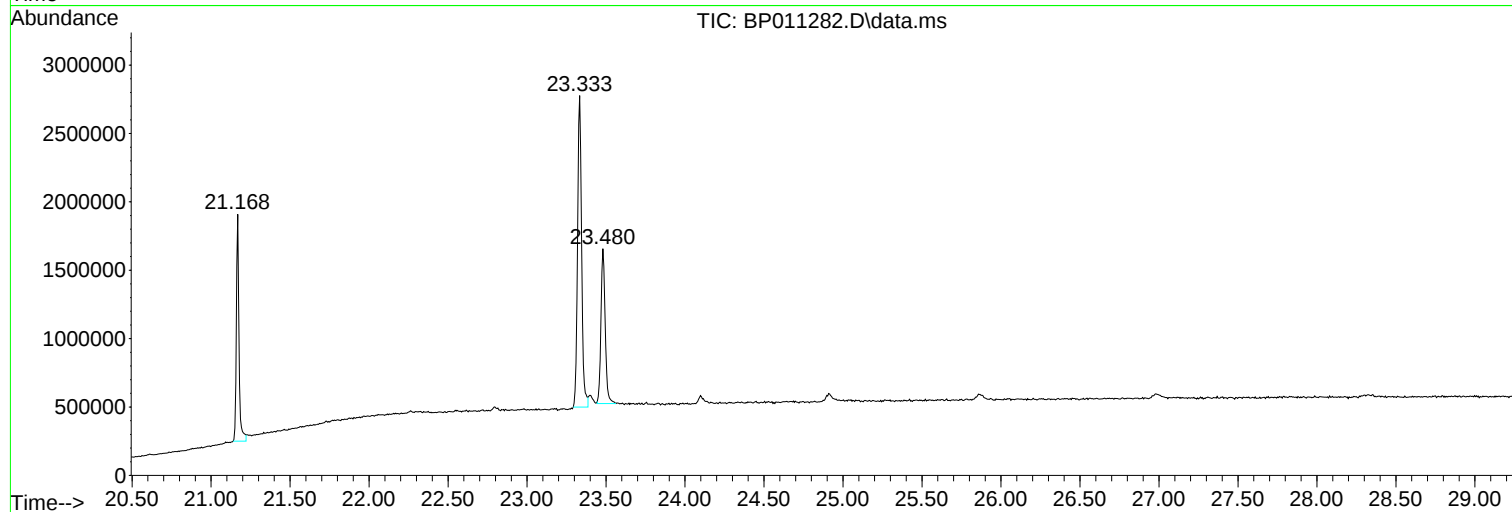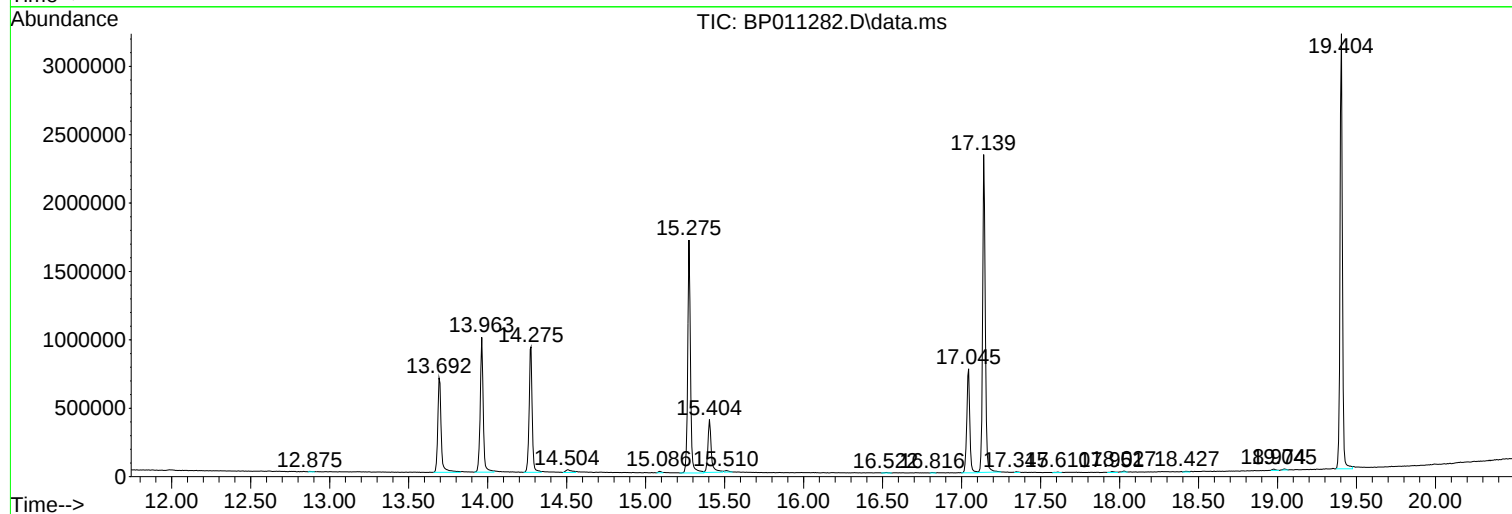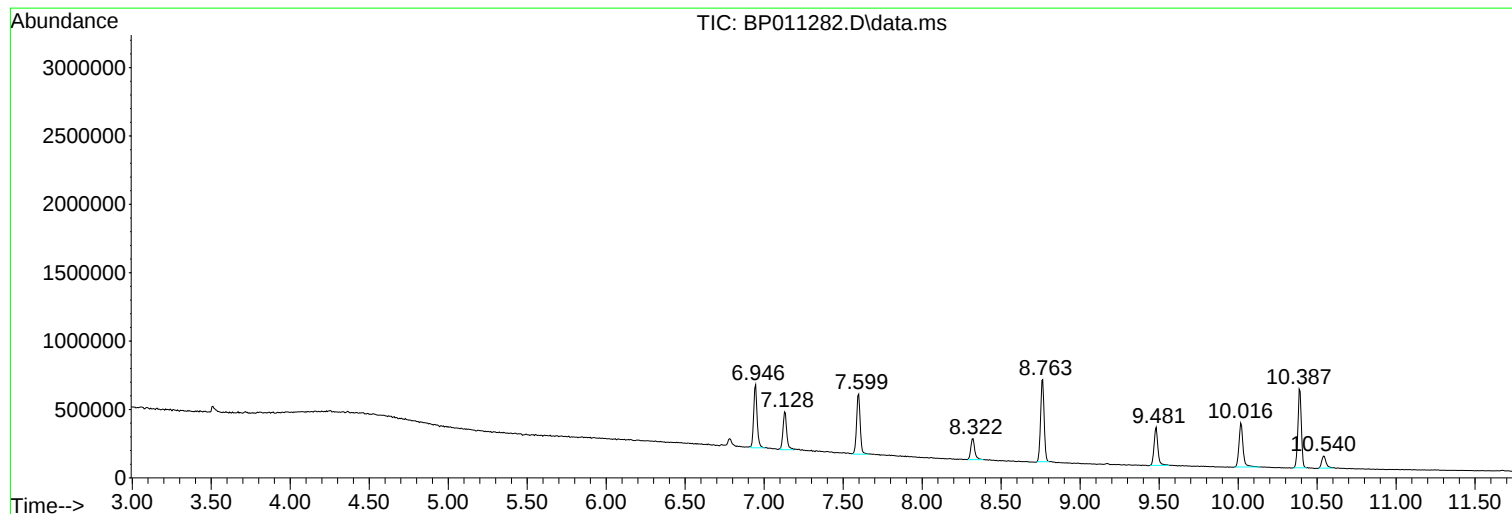

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011282.D
Acq On : 05 Aug 2022 17:12
Operator : CG/JU
Sample : N4026-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011282.D
Acq On : 05 Aug 2022 17:12
Operator : CG/JU
Sample : N4026-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc