

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011285.D
 Acq On : 05 Aug 2022 18:57
 Operator : CG/JU
 Sample : PB146767BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK767

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	85	88	99	rBV	145122	228572	5.62%	0.697%
2	6.781	640	645	665	rVB	430414	689039	16.93%	2.100%
3	6.946	668	673	684	rVB	495817	755116	18.56%	2.301%
4	7.128	699	704	715	rVB	432322	661999	16.27%	2.017%
5	7.593	779	783	795	rVB	390977	630053	15.48%	1.920%
6	8.322	901	907	929	rVB	500146	823843	20.24%	2.510%
7	8.764	976	982	991	rVB	657937	1018121	25.02%	3.103%
8	9.481	1098	1104	1112	rBV	326740	526989	12.95%	1.606%
9	10.016	1189	1195	1213	rBV	436995	752463	18.49%	2.293%
10	10.387	1252	1258	1267	rVB	521768	819604	20.14%	2.498%
11	10.540	1278	1284	1297	rBV	547299	885523	21.76%	2.698%
12	13.693	1814	1820	1832	rBV	929591	1276222	31.36%	3.889%
13	13.963	1859	1866	1891	rBV	1313073	1654993	40.67%	5.043%
14	14.269	1912	1918	1929	rBV	1071455	1363799	33.51%	4.156%
15	14.499	1951	1957	1977	rBV	306105	668395	16.42%	2.037%
16	15.275	2082	2089	2105	rBV	2140635	2622683	64.45%	7.992%
17	15.404	2105	2111	2125	rVV	522817	760205	18.68%	2.317%
18	15.510	2126	2129	2135	rVB4	12824	20617	0.51%	0.063%
19	16.822	2348	2352	2358	rBV7	2507	5495	0.14%	0.017%
20	17.040	2383	2389	2400	rBV	1018978	1302119	32.00%	3.968%
21	17.140	2400	2406	2421	rVV	2725937	3226938	79.30%	9.833%
22	17.722	2501	2505	2509	rBV6	2906	4733	0.12%	0.014%
23	18.975	2714	2718	2723	rBV4	11207	16321	0.40%	0.050%
24	19.045	2727	2730	2734	rVB3	9120	13192	0.32%	0.040%
25	19.398	2784	2790	2802	rBV	3302476	3608363	88.67%	10.996%
26	21.163	3086	3090	3101	rBV	1759158	2183531	53.66%	6.654%
27	23.328	3452	3458	3467	rBV2	2261036	4069475	100.00%	12.401%
28	23.475	3478	3483	3495	rVB	1188511	2227652	54.74%	6.788%




Sum of corrected areas: 32816055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011285.D
Acq On : 05 Aug 2022 18:57
Operator : CG/JU
Sample : PB146767BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

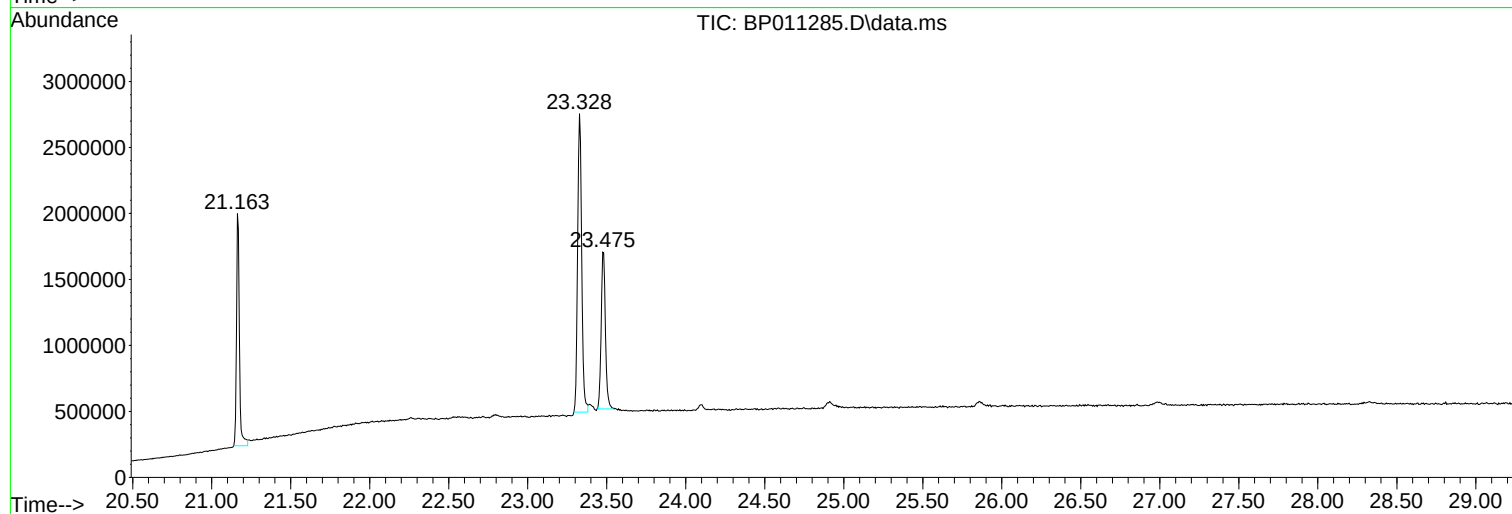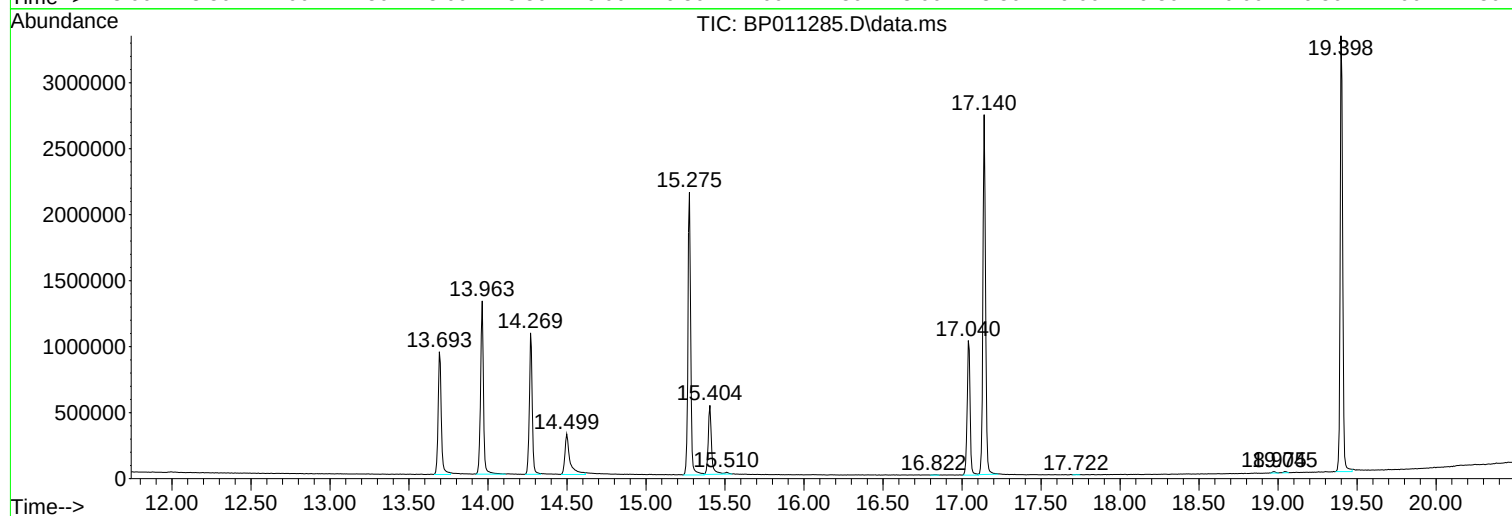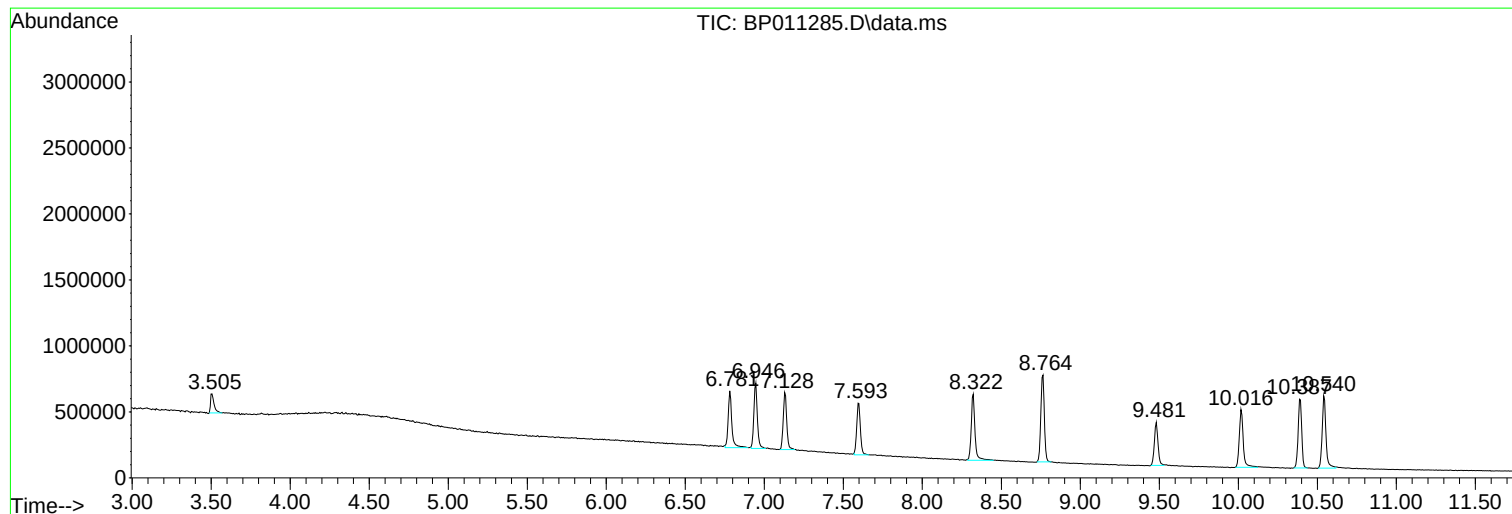

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011285.D
Acq On : 05 Aug 2022 18:57
Operator : CG/JU
Sample : PB146767BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011285.D
Acq On : 05 Aug 2022 18:57
Operator : CG/JU
Sample : PB146767BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------