

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011291.D
 Acq On : 05 Aug 2022 22:26
 Operator : CG/JU
 Sample : N4026-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	668	673	680	rVB	476626	721843	16.03%	2.344%
2	7.128	699	704	712	rBV	303652	454418	10.09%	1.476%
3	7.593	778	783	793	rVB	426894	651855	14.47%	2.117%
4	8.316	901	906	915	rBV	181727	297806	6.61%	0.967%
5	8.757	975	981	992	rVB	705439	1084114	24.07%	3.520%
6	9.481	1098	1104	1114	rBV	305343	513334	11.40%	1.667%
7	10.016	1189	1195	1210	rBV	384691	645491	14.33%	2.096%
8	10.387	1252	1258	1265	rBV	578284	856906	19.03%	2.782%
9	10.540	1278	1284	1293	rBV	131824	235714	5.23%	0.765%
10	11.669	1472	1476	1482	rBV4	27938	43653	0.97%	0.142%
11	12.557	1623	1627	1633	rVB5	7506	12320	0.27%	0.040%
12	13.692	1813	1820	1837	rBV	908168	1249391	27.74%	4.057%
13	13.828	1841	1843	1849	rVV6	14047	22261	0.49%	0.072%
14	13.957	1858	1865	1889	rVV	1285233	1694830	37.63%	5.503%
15	14.269	1910	1918	1935	rBV	1071285	1341665	29.79%	4.356%
16	14.504	1952	1958	1970	rBV4	22657	62602	1.39%	0.203%
17	14.710	1991	1993	1999	rVB6	3095	5279	0.12%	0.017%
18	15.086	2052	2057	2061	rBV5	5170	9408	0.21%	0.031%
19	15.269	2082	2088	2105	rBV	2128536	2638758	58.59%	8.568%
20	15.398	2105	2110	2125	rVV	471584	742271	16.48%	2.410%
21	15.510	2125	2129	2142	rVB7	15344	38849	0.86%	0.126%
22	16.639	2317	2321	2327	rBV3	14779	20087	0.45%	0.065%
23	17.039	2381	2389	2399	rBV	931326	1126032	25.00%	3.656%
24	17.139	2399	2406	2422	rVV	2957893	3588126	79.67%	11.651%
25	17.604	2482	2485	2491	rVB8	4623	8512	0.19%	0.028%
26	17.727	2501	2506	2508	rBV6	5342	7394	0.16%	0.024%
27	17.845	2523	2526	2529	rBV4	5646	6696	0.15%	0.022%
28	17.951	2540	2544	2548	rBV7	4964	7062	0.16%	0.023%
29	18.022	2554	2556	2562	rVB5	4073	7070	0.16%	0.023%
30	18.521	2636	2641	2646	rBV7	6762	12374	0.27%	0.040%
31	18.974	2714	2718	2722	rBV5	10377	15824	0.35%	0.051%
32	19.039	2726	2729	2732	rVV3	8958	11534	0.26%	0.037%
33	19.398	2784	2790	2807	rBV	3739944	4085551	90.72%	13.266%
34	21.163	3085	3090	3102	rBV	1618283	2027136	45.01%	6.582%
35	23.321	3451	3457	3466	rBV	2453353	4503701	100.00%	14.624%
36	23.468	3477	3482	3494	rVB	1122837	2047553	45.46%	6.648%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011291.D
Acq On : 05 Aug 2022 22:26
Operator : CG/JU
Sample : N4026-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 30797420

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011291.D
Acq On : 05 Aug 2022 22:26
Operator : CG/JU
Sample : N4026-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

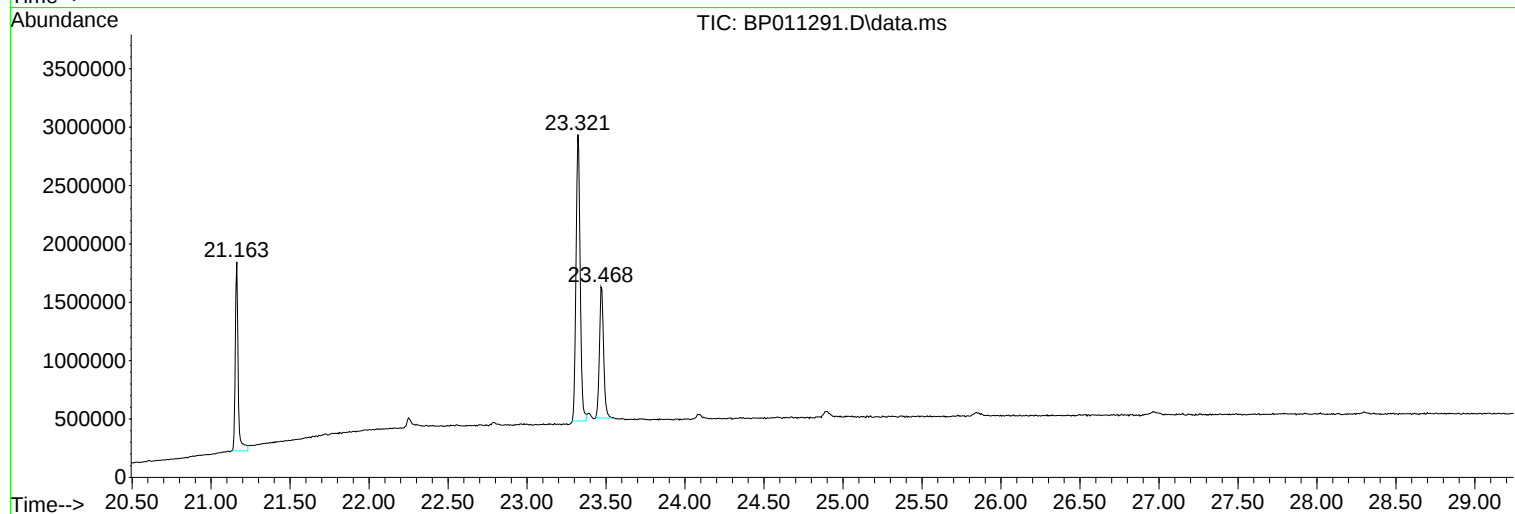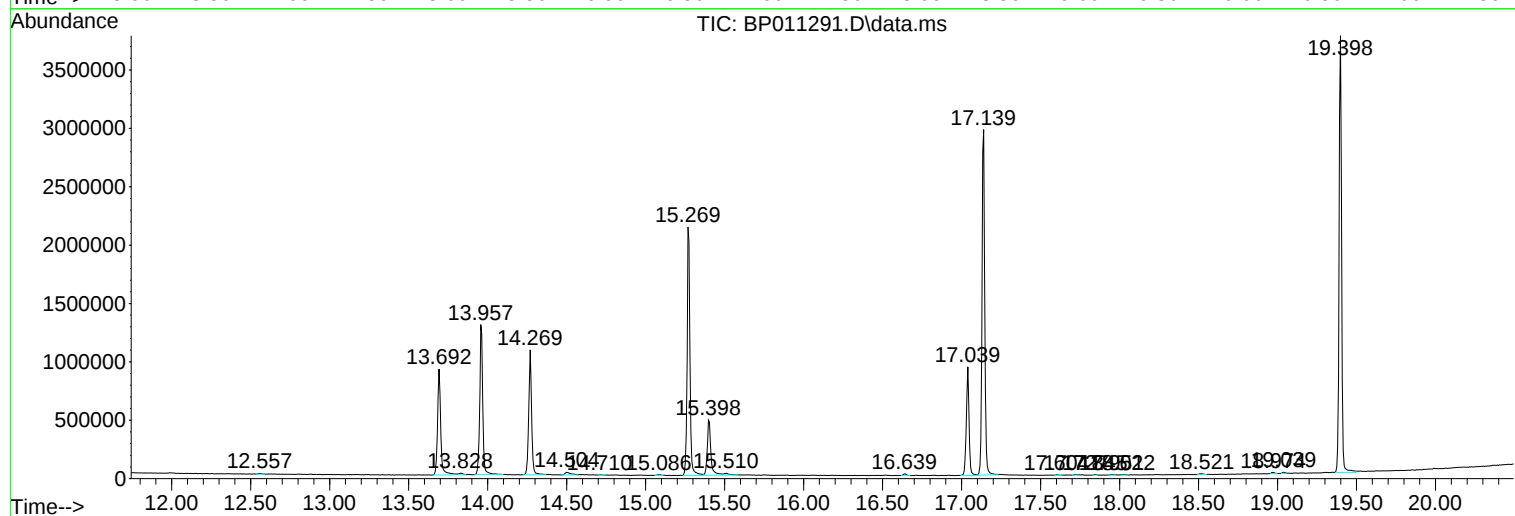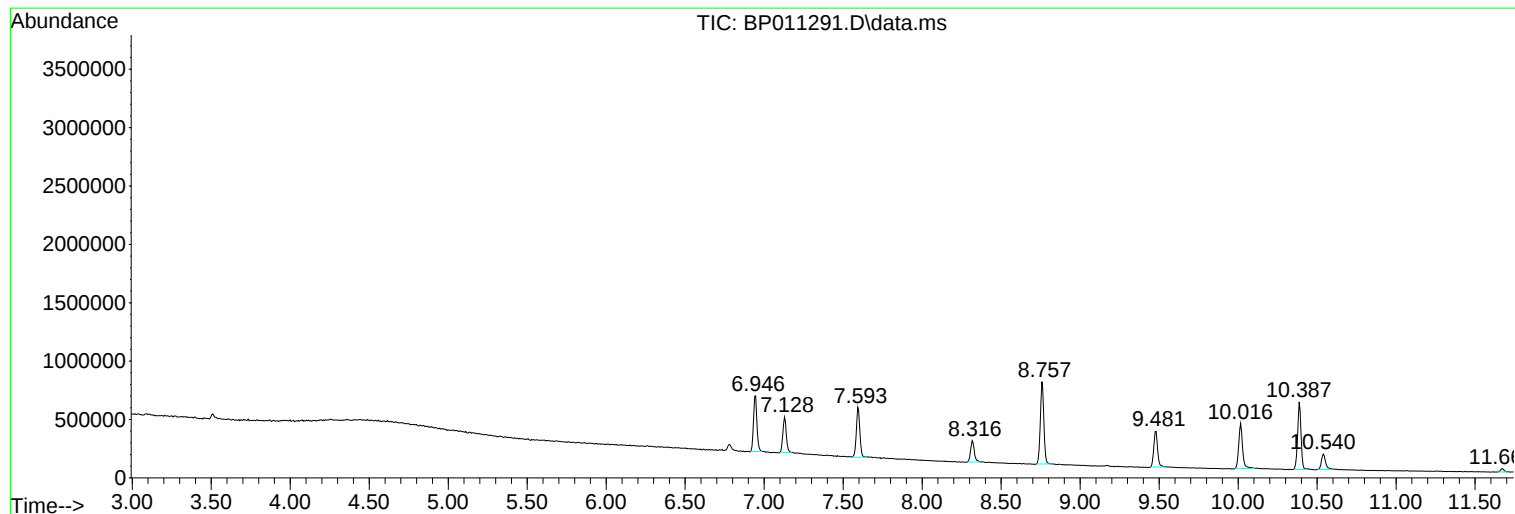

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011291.D
Acq On : 05 Aug 2022 22:26
Operator : CG/JU
Sample : N4026-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011291.D
Acq On : 05 Aug 2022 22:26
Operator : CG/JU
Sample : N4026-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc