

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011295.D
 Acq On : 06 Aug 2022 00:45
 Operator : CG/JU
 Sample : N4026-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.940	668	672	681	rVB	393361	588894	16.05%	2.303%
2	7.128	699	704	716	rVB	239295	385824	10.52%	1.509%
3	7.593	778	783	793	rVB	371828	574879	15.67%	2.248%
4	8.316	901	906	914	rVB2	134470	227583	6.20%	0.890%
5	8.757	975	981	990	rBV	565155	869621	23.71%	3.400%
6	9.475	1098	1103	1116	rVB	250217	423401	11.54%	1.656%
7	10.016	1188	1195	1206	rBV	283269	517612	14.11%	2.024%
8	10.387	1252	1258	1265	rBV	472676	711023	19.38%	2.780%
9	10.540	1279	1284	1293	rBV2	72468	130638	3.56%	0.511%
10	11.669	1472	1476	1485	rBV3	36105	60870	1.66%	0.238%
11	12.557	1623	1627	1634	rBV6	9620	14771	0.40%	0.058%
12	13.439	1773	1777	1781	rVB2	3078	3736	0.10%	0.015%
13	13.692	1813	1820	1837	rBV	732614	1027876	28.02%	4.019%
14	13.828	1840	1843	1852	rVB4	17063	31307	0.85%	0.122%
15	13.957	1859	1865	1878	rBV	952639	1271071	34.65%	4.970%
16	14.181	1902	1903	1909	rVB5	3200	3898	0.11%	0.015%
17	14.269	1909	1918	1929	rBV	911820	1176927	32.08%	4.602%
18	14.504	1953	1958	1965	rBV4	16743	37142	1.01%	0.145%
19	15.086	2052	2057	2061	rBV4	9498	16221	0.44%	0.063%
20	15.269	2081	2088	2104	rBV	1630924	2062027	56.21%	8.063%
21	15.398	2104	2110	2124	rVV	394699	612772	16.70%	2.396%
22	15.504	2126	2128	2134	rVB5	11889	18923	0.52%	0.074%
23	15.751	2164	2170	2174	rVB7	6078	10220	0.28%	0.040%
24	16.186	2239	2244	2247	rVB6	3564	5472	0.15%	0.021%
25	16.522	2296	2301	2305	rBV8	4328	5961	0.16%	0.023%
26	16.639	2316	2321	2326	rBV2	21923	28970	0.79%	0.113%
27	17.039	2378	2389	2399	rBV	797162	1037344	28.28%	4.056%
28	17.133	2399	2405	2418	rVV	2341302	2856331	77.86%	11.169%
29	17.345	2439	2441	2445	rVB5	3520	4052	0.11%	0.016%
30	17.439	2455	2457	2462	rVB6	2461	3869	0.11%	0.015%
31	17.598	2482	2484	2488	rVB5	3992	4631	0.13%	0.018%
32	17.727	2501	2506	2509	rBV7	6326	8690	0.24%	0.034%
33	17.839	2519	2525	2531	rBV7	5955	10717	0.29%	0.042%
34	17.951	2538	2544	2547	rBV7	10041	15455	0.42%	0.060%
35	18.022	2553	2556	2560	rBV2	6779	8745	0.24%	0.034%
36	18.227	2589	2591	2595	rVB5	3365	3723	0.10%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011295.D
Acq On : 06 Aug 2022 00:45
Operator : CG/JU
Sample : N4026-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Title : SVOA CALIBRATION

37	18.510	2636	2639	2645	rBV6	9961	16659	0.45%	0.065%
38	18.969	2713	2717	2721	rBV4	11807	18206	0.50%	0.071%
39	19.039	2726	2729	2733	rVB3	8241	10631	0.29%	0.042%
40	19.345	2779	2781	2784	rBV4	4893	5746	0.16%	0.022%
41	19.398	2784	2790	2798	rBV	3151437	3344958	91.18%	13.080%
42	21.163	3085	3090	3102	rBV	1540284	1892760	51.60%	7.401%
43	23.321	3451	3457	3465	rBV2	1994894	3668335	100.00%	14.344%
44	23.468	3477	3482	3495	rVB	989159	1844911	50.29%	7.214%




Sum of corrected areas: 25573402

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011295.D
Acq On : 06 Aug 2022 00:45
Operator : CG/JU
Sample : N4026-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

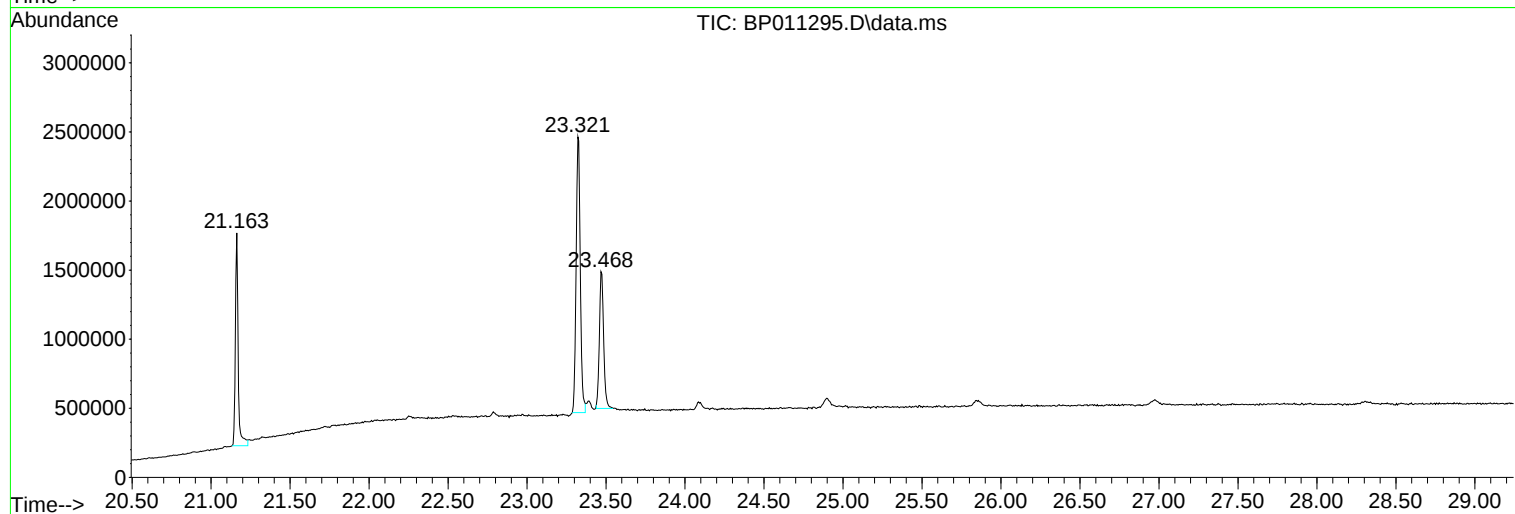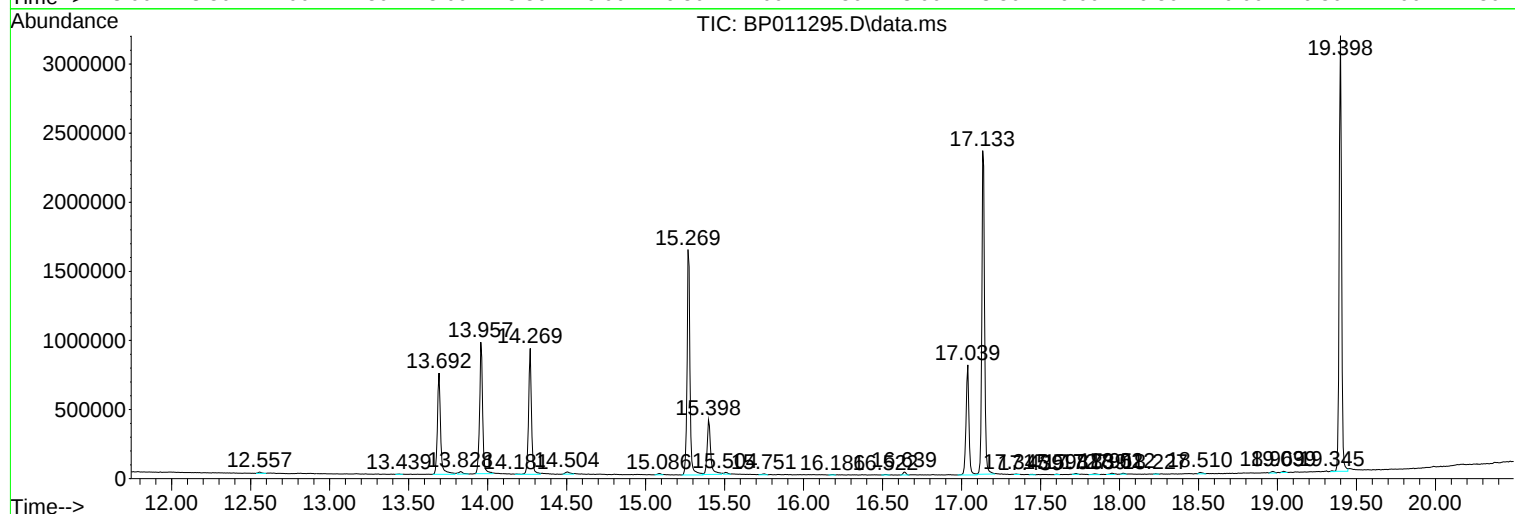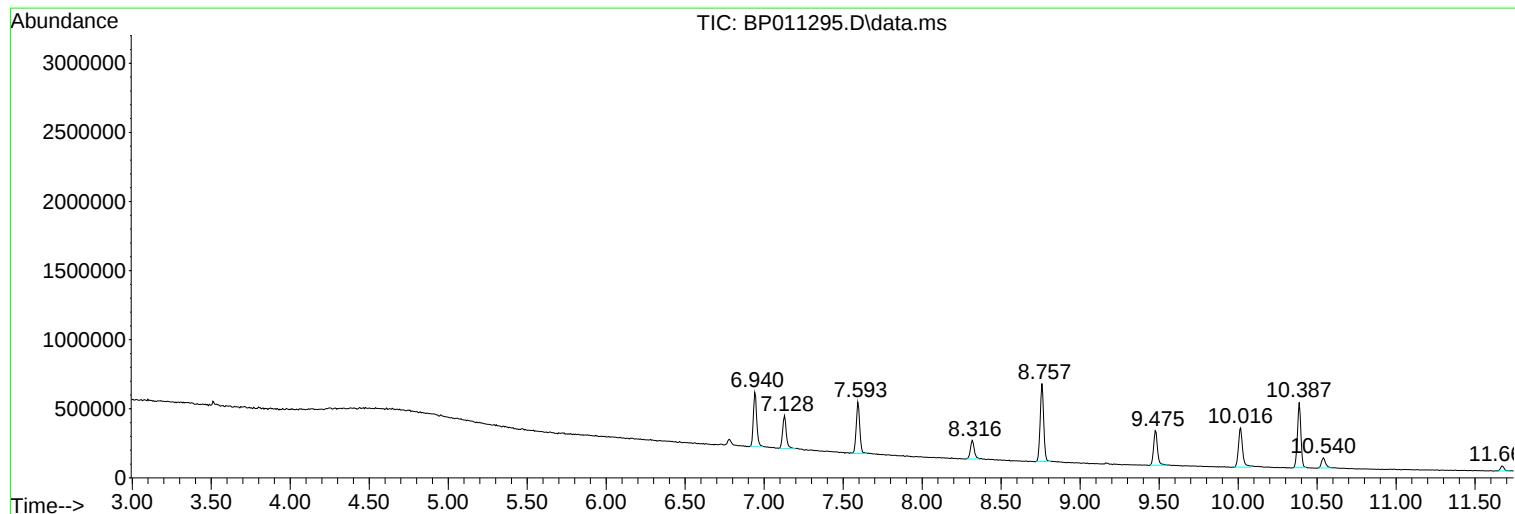

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011295.D
Acq On : 06 Aug 2022 00:45
Operator : CG/JU
Sample : N4026-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011295.D
Acq On : 06 Aug 2022 00:45
Operator : CG/JU
Sample : N4026-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
