

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011301.D
 Acq On : 06 Aug 2022 05:31
 Operator : CG/JU
 Sample : PB146785BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK785

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.775	640	644	656	rVB	407966	616864	15.62%	1.692%
2	6.940	667	672	681	rVB	508882	756557	19.16%	2.075%
3	7.128	699	704	713	rVB	425926	656274	16.62%	1.800%
4	7.593	778	783	793	rVB	544036	826189	20.93%	2.266%
5	8.316	900	906	919	rVB	506237	791990	20.06%	2.173%
6	8.757	975	981	995	rVB	689752	1079761	27.35%	2.962%
7	9.475	1097	1103	1113	rBV	342256	544038	13.78%	1.492%
8	10.010	1188	1194	1209	rBV	462071	782689	19.82%	2.147%
9	10.387	1251	1258	1266	rVB	764665	1166312	29.54%	3.199%
10	10.534	1277	1283	1295	rBV	339875	618427	15.66%	1.696%
11	13.692	1813	1820	1833	rBV	1019670	1379996	34.95%	3.786%
12	13.957	1858	1865	1881	rBV	1514679	1823334	46.18%	5.002%
13	14.263	1911	1917	1930	rBV	1574450	2022525	51.23%	5.548%
14	14.492	1950	1956	1973	rBV	337281	685043	17.35%	1.879%
15	15.269	2079	2088	2102	rBV	2567130	2883621	73.04%	7.910%
16	15.398	2104	2110	2121	rVV	566953	815605	20.66%	2.237%
17	15.510	2125	2129	2135	rVB5	12943	25394	0.64%	0.070%
18	16.828	2347	2353	2356	rBV5	3055	5349	0.14%	0.015%
19	17.039	2382	2389	2399	rBV	1627636	1927066	48.81%	5.286%
20	17.133	2399	2405	2428	rVV	2949852	3632736	92.01%	9.965%
21	17.716	2501	2504	2512	rBV4	3145	5826	0.15%	0.016%
22	18.969	2713	2717	2723	rBV5	12327	19402	0.49%	0.053%
23	19.039	2725	2729	2732	rBV3	10013	12999	0.33%	0.036%
24	19.398	2784	2790	2805	rBV	3376252	3894898	98.65%	10.684%
25	21.157	3085	3089	3101	rBV	2334964	2884910	73.07%	7.914%
26	23.321	3450	3457	3465	rBV2	2164612	3948041	100.00%	10.830%
27	23.468	3476	3482	3492	rVB	1478132	2648863	67.09%	7.266%




Sum of corrected areas: 36454709

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011301.D
Acq On : 06 Aug 2022 05:31
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

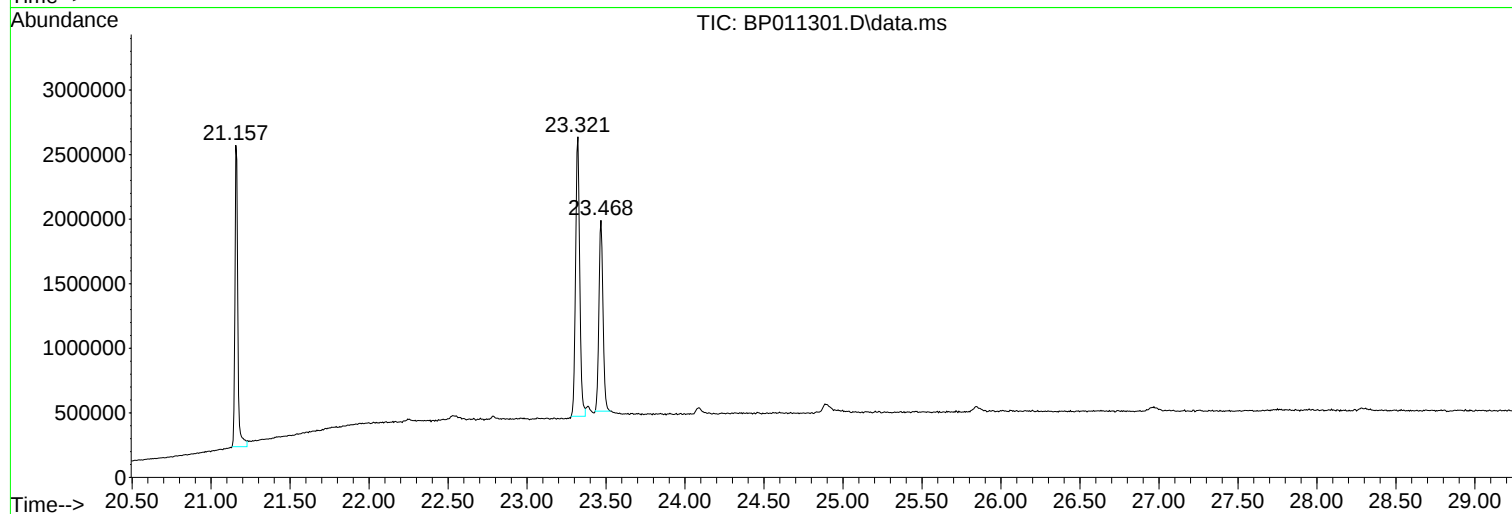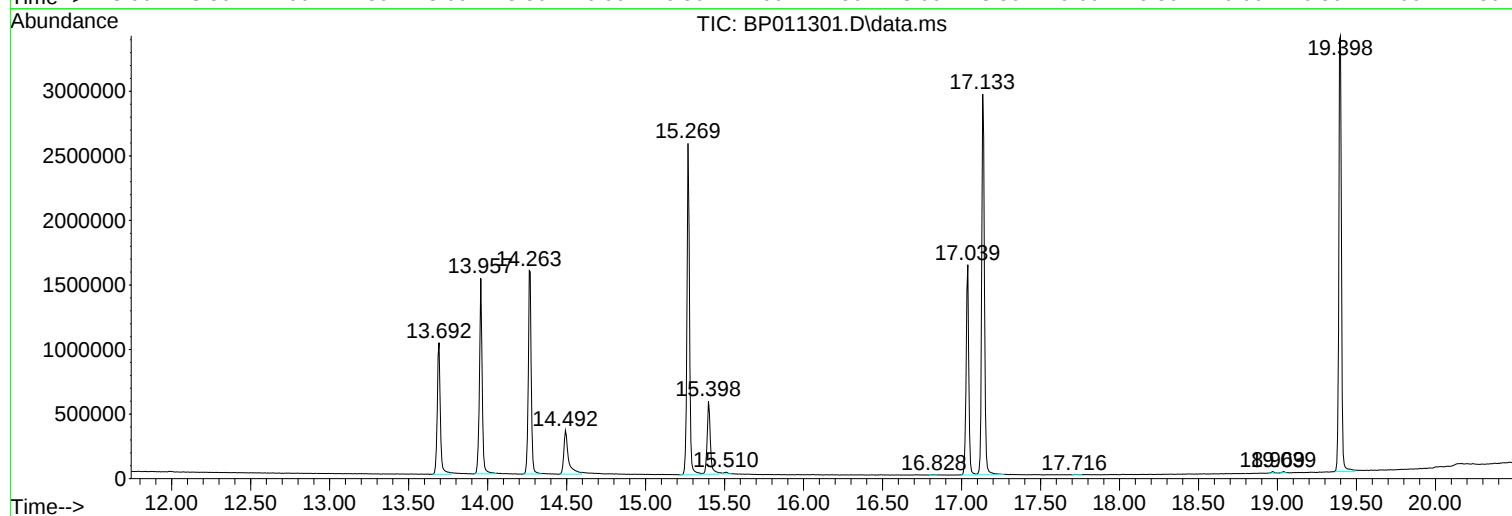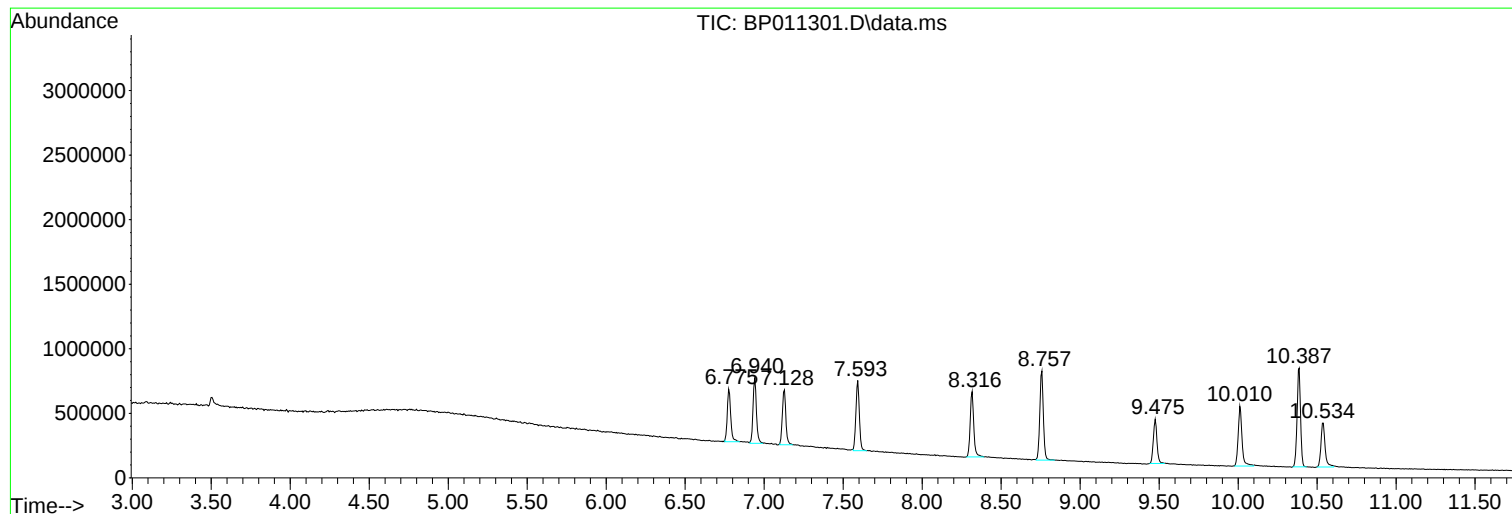

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011301.D
Acq On : 06 Aug 2022 05:31
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011301.D
Acq On : 06 Aug 2022 05:31
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------