

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011303.D
 Acq On : 06 Aug 2022 06:40
 Operator : CG/JU
 Sample : N4026-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.940	667	672	684	rVB	430817	655286	15.94%	1.977%
2	7.128	699	704	712	rVB	240434	376717	9.17%	1.137%
3	7.593	778	783	792	rVB	415320	628842	15.30%	1.897%
4	8.316	901	906	915	rVB2	145680	252833	6.15%	0.763%
5	8.758	975	981	988	rVB	603297	945682	23.01%	2.853%
6	9.475	1097	1103	1114	rBV2	294981	483511	11.76%	1.459%
7	10.010	1188	1194	1208	rBV	374220	644144	15.67%	1.943%
8	10.387	1251	1258	1266	rVB	595503	912880	22.21%	2.754%
9	10.534	1278	1283	1293	rBV	94625	180808	4.40%	0.545%
10	12.604	1631	1635	1636	rBV3	4494	5623	0.14%	0.017%
11	13.093	1713	1718	1723	rVB7	2715	4496	0.11%	0.014%
12	13.687	1812	1819	1836	rBV	974506	1395123	33.95%	4.209%
13	13.957	1857	1865	1883	rBV	1437660	1823049	44.36%	5.500%
14	14.175	1898	1902	1910	rVB9	6308	10074	0.25%	0.030%
15	14.263	1911	1917	1937	rVV	1305624	1684708	40.99%	5.083%
16	14.498	1951	1957	1968	rBV5	26416	65627	1.60%	0.198%
17	14.710	1989	1993	1997	rVB7	4420	6790	0.17%	0.020%
18	15.081	2051	2056	2059	rVV6	3590	4351	0.11%	0.013%
19	15.134	2063	2065	2074	rVB10	3257	4690	0.11%	0.014%
20	15.269	2081	2088	2104	rBV	2344845	2868996	69.81%	8.656%
21	15.398	2104	2110	2124	rVV	486107	704884	17.15%	2.127%
22	15.510	2125	2129	2133	rVB7	11293	19160	0.47%	0.058%
23	15.857	2178	2188	2190	rBV7	3520	9467	0.23%	0.029%
24	16.004	2208	2213	2220	rBV4	19775	28770	0.70%	0.087%
25	16.057	2220	2222	2227	rVB6	2868	4285	0.10%	0.013%
26	16.451	2281	2289	2292	rBV7	7945	12891	0.31%	0.039%
27	16.522	2297	2301	2304	rVV4	5598	6553	0.16%	0.020%
28	16.704	2329	2332	2337	rVB7	3435	6472	0.16%	0.020%
29	16.810	2346	2350	2353	rBV6	5835	8772	0.21%	0.026%
30	17.034	2381	2388	2395	rBV	1408877	1700909	41.39%	5.132%
31	17.092	2395	2398	2400	rVV2	33395	45526	1.11%	0.137%
32	17.134	2400	2405	2418	rVB	2875439	3453612	84.03%	10.419%
33	17.269	2425	2428	2436	rVB10	7388	12726	0.31%	0.038%
34	17.422	2449	2454	2457	rBV6	13528	19303	0.47%	0.058%
35	17.598	2482	2484	2488	rVB5	4482	4565	0.11%	0.014%
36	17.663	2492	2495	2498	rBV5	4836	6420	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
 Data File : BP011303.D
 Acq On : 06 Aug 2022 06:40
 Operator : CG/JU
 Sample : N4026-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

37	17.733	2502	2507	2514	rVV3	34992	48389	1.18%	0.146%
38	17.828	2518	2523	2529	rVB9	5167	9592	0.23%	0.029%
39	17.951	2539	2544	2550	rBV2	98373	146973	3.58%	0.443%
40	18.416	2621	2623	2625	rVB3	5982	4521	0.11%	0.014%
41	18.528	2639	2642	2646	rBV6	4678	6370	0.15%	0.019%
42	18.592	2650	2653	2656	rBV4	5190	6822	0.17%	0.021%
43	18.875	2698	2701	2709	rVB4	35823	46464	1.13%	0.140%
44	18.969	2713	2717	2722	rBV6	17371	27051	0.66%	0.082%
45	19.010	2722	2724	2726	rBV3	5951	6095	0.15%	0.018%
46	19.033	2726	2728	2732	rVB2	11129	14323	0.35%	0.043%
47	19.198	2753	2756	2759	rBV4	14411	15920	0.39%	0.048%
48	19.392	2784	2789	2798	rBV	3641162	4109839	100.00%	12.399%
49	19.922	2875	2879	2886	rBV6	75135	127916	3.11%	0.386%
50	20.898	3040	3045	3053	rBV2	324298	624905	15.21%	1.885%
51	21.157	3085	3089	3100	rBV	2032065	2549684	62.04%	7.692%
52	23.316	3450	3456	3465	rBV2	2071607	3957725	96.30%	11.940%
53	23.468	3476	3482	3498	rVB	1329802	2444555	59.48%	7.375%




Sum of corrected areas: 33145689

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011303.D
Acq On : 06 Aug 2022 06:40
Operator : CG/JU
Sample : N4026-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

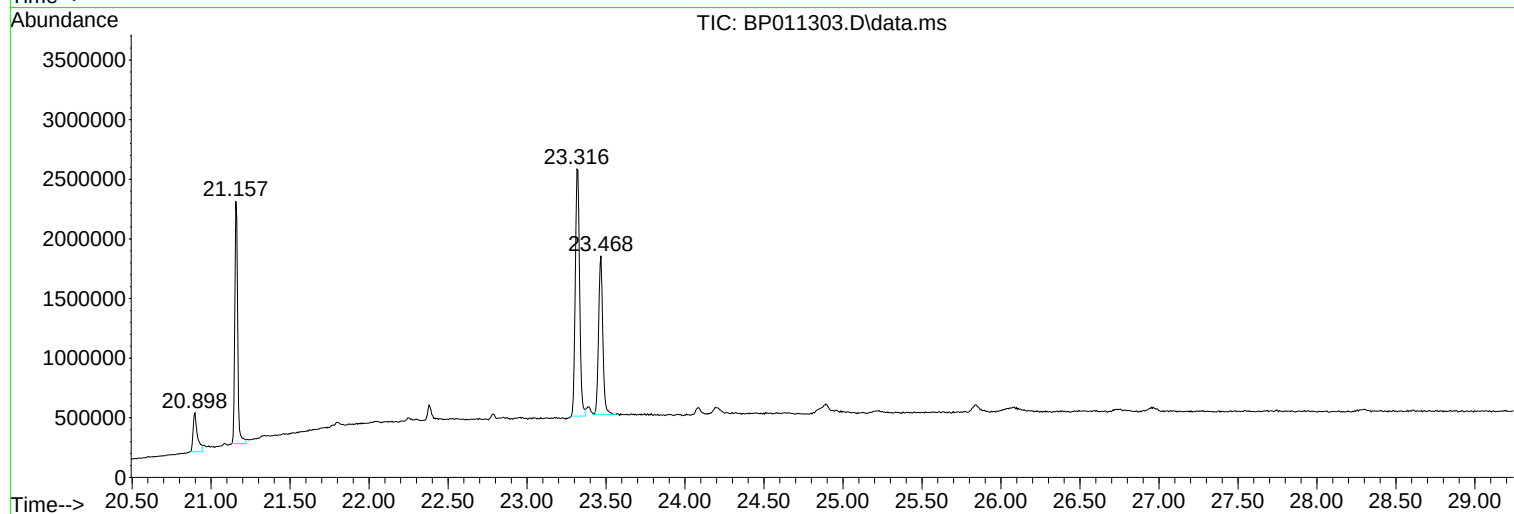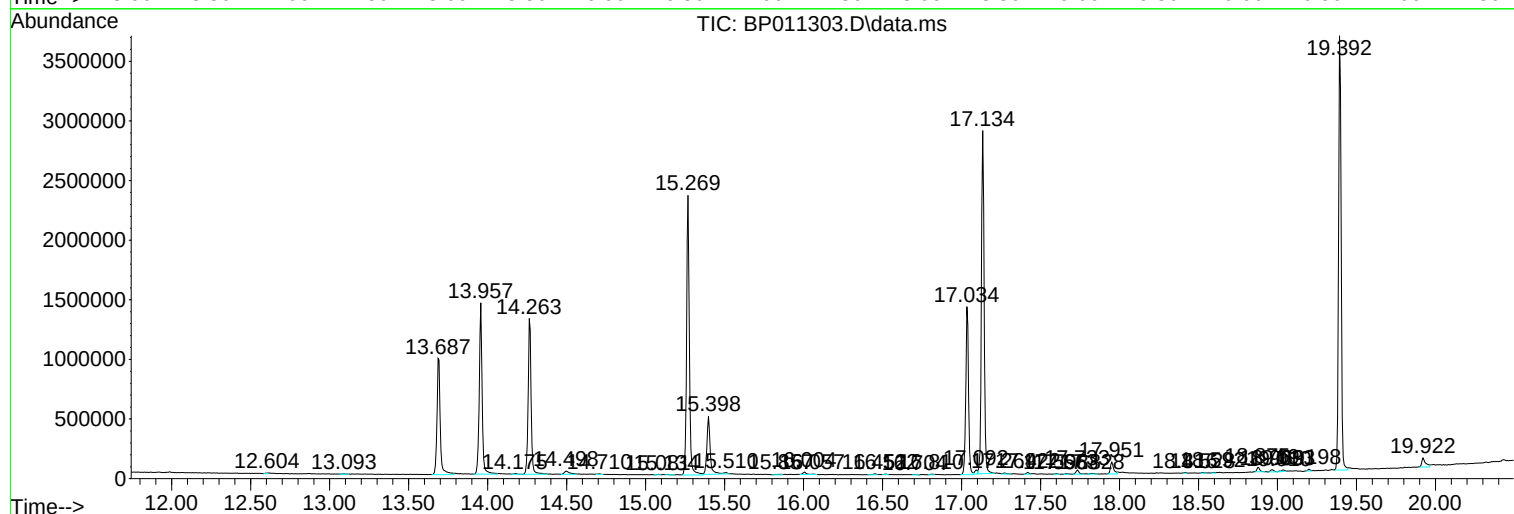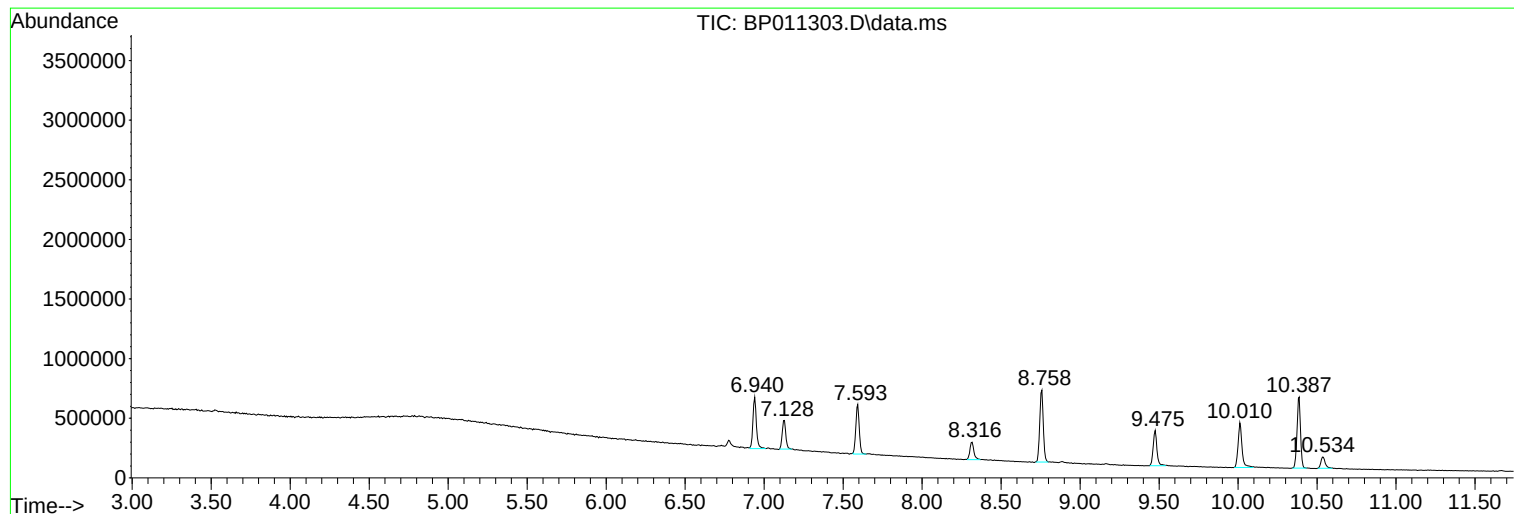

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011303.D
Acq On : 06 Aug 2022 06:40
Operator : CG/JU
Sample : N4026-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic20.898 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.898	4.90 ng/ul	624905	Chrysene-d12	21.157

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	96
2			Bromoacetic acid, pentadecyl ester	348	C17H33BrO2	131143-01-6	89
3			Cyclopentane, 1,1'-[3-(2-cyclope...	304	C22H40	055255-85-1	83
4			n-Nonadecanol-1	284	C19H40O	001454-84-8	81
5			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	81

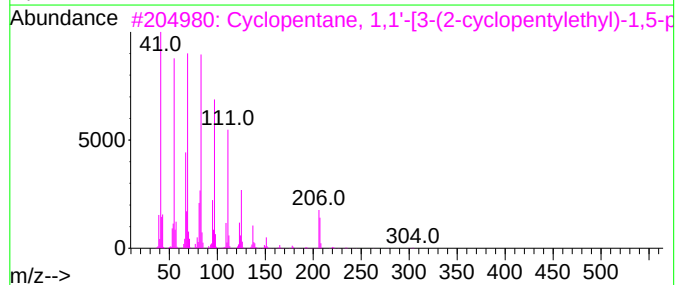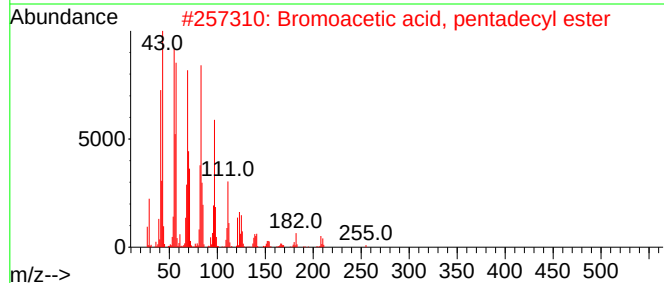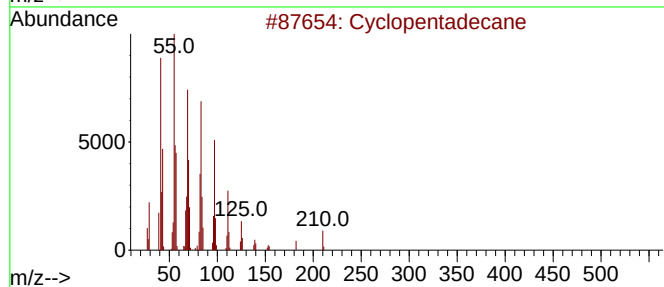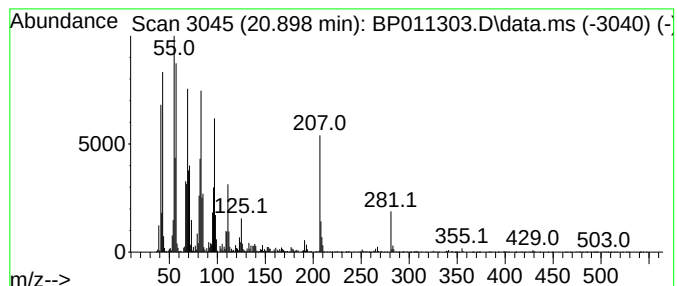

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080522\
Data File : BP011303.D
Acq On : 06 Aug 2022 06:40
Operator : CG/JU
Sample : N4026-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	20.898	4.9	ng/u1	624905	5	21.157	2549680	20.0