

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080524\
 Data File : BP021372.D
 Acq On : 05 Aug 2024 14:37
 Operator : CG/JU
 Sample : P3300-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1GA5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/07/2024

Quant Time: Aug 05 15:34:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.610	152	184390	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.375	136	740700	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.251	164	482977	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.075	188	1053804	20.000	ng/u1	-0.02
79) Chrysene-d12	21.527	240	1067923	20.000	ng/u1	0.00
88) Perylene-d12	24.827	264	1326594	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	17695	4.367	ng/uL	-0.01
4) Pyridine-d5	3.593	84	94994	8.098	ng/u1	0.00
7) Phenol-d5	6.863	99	87896	5.847	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.969	67	198718	21.813	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.169	132	256601	20.717	ng/u1	-0.01
15) 4-Methylphenol-d8	8.352	113	174060	13.941	ng/u1	-0.01
21) Nitrobenzene-d5	8.781	128	119794	20.822	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.493	143	132601	20.138	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.051	165	232485	19.525	ng/u1	0.00
31) 4-Chloroaniline-d4	10.551	131	276137	17.506	ng/u1	0.00
46) Dimethylphthalate-d6	13.675	166	792785	22.580	ng/u1	0.00
49) Acenaphthylene-d8	13.945	160	895449	22.714	ng/u1	-0.02
54) 4-Nitrophenol-d4	14.663	143	25838m	5.172	ng/u1	0.08
60) Fluorene-d10	15.275	176	722097	25.069	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.463	200	104676	16.417	ng/u1	0.00
73) Anthracene-d10	17.180	188	1182351	25.261	ng/u1	-0.01
81) Pyrene-d10	19.569	212	1481829	22.444	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.586	264	1666441	25.470	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.410	149	114401	2.352	ng/u1	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080524\
Data File : BP021372.D
Acq On : 05 Aug 2024 14:37
Operator : CG/JU
Sample : P3300-09
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
E1GA5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/07/2024


Quant Time: Aug 05 15:34:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

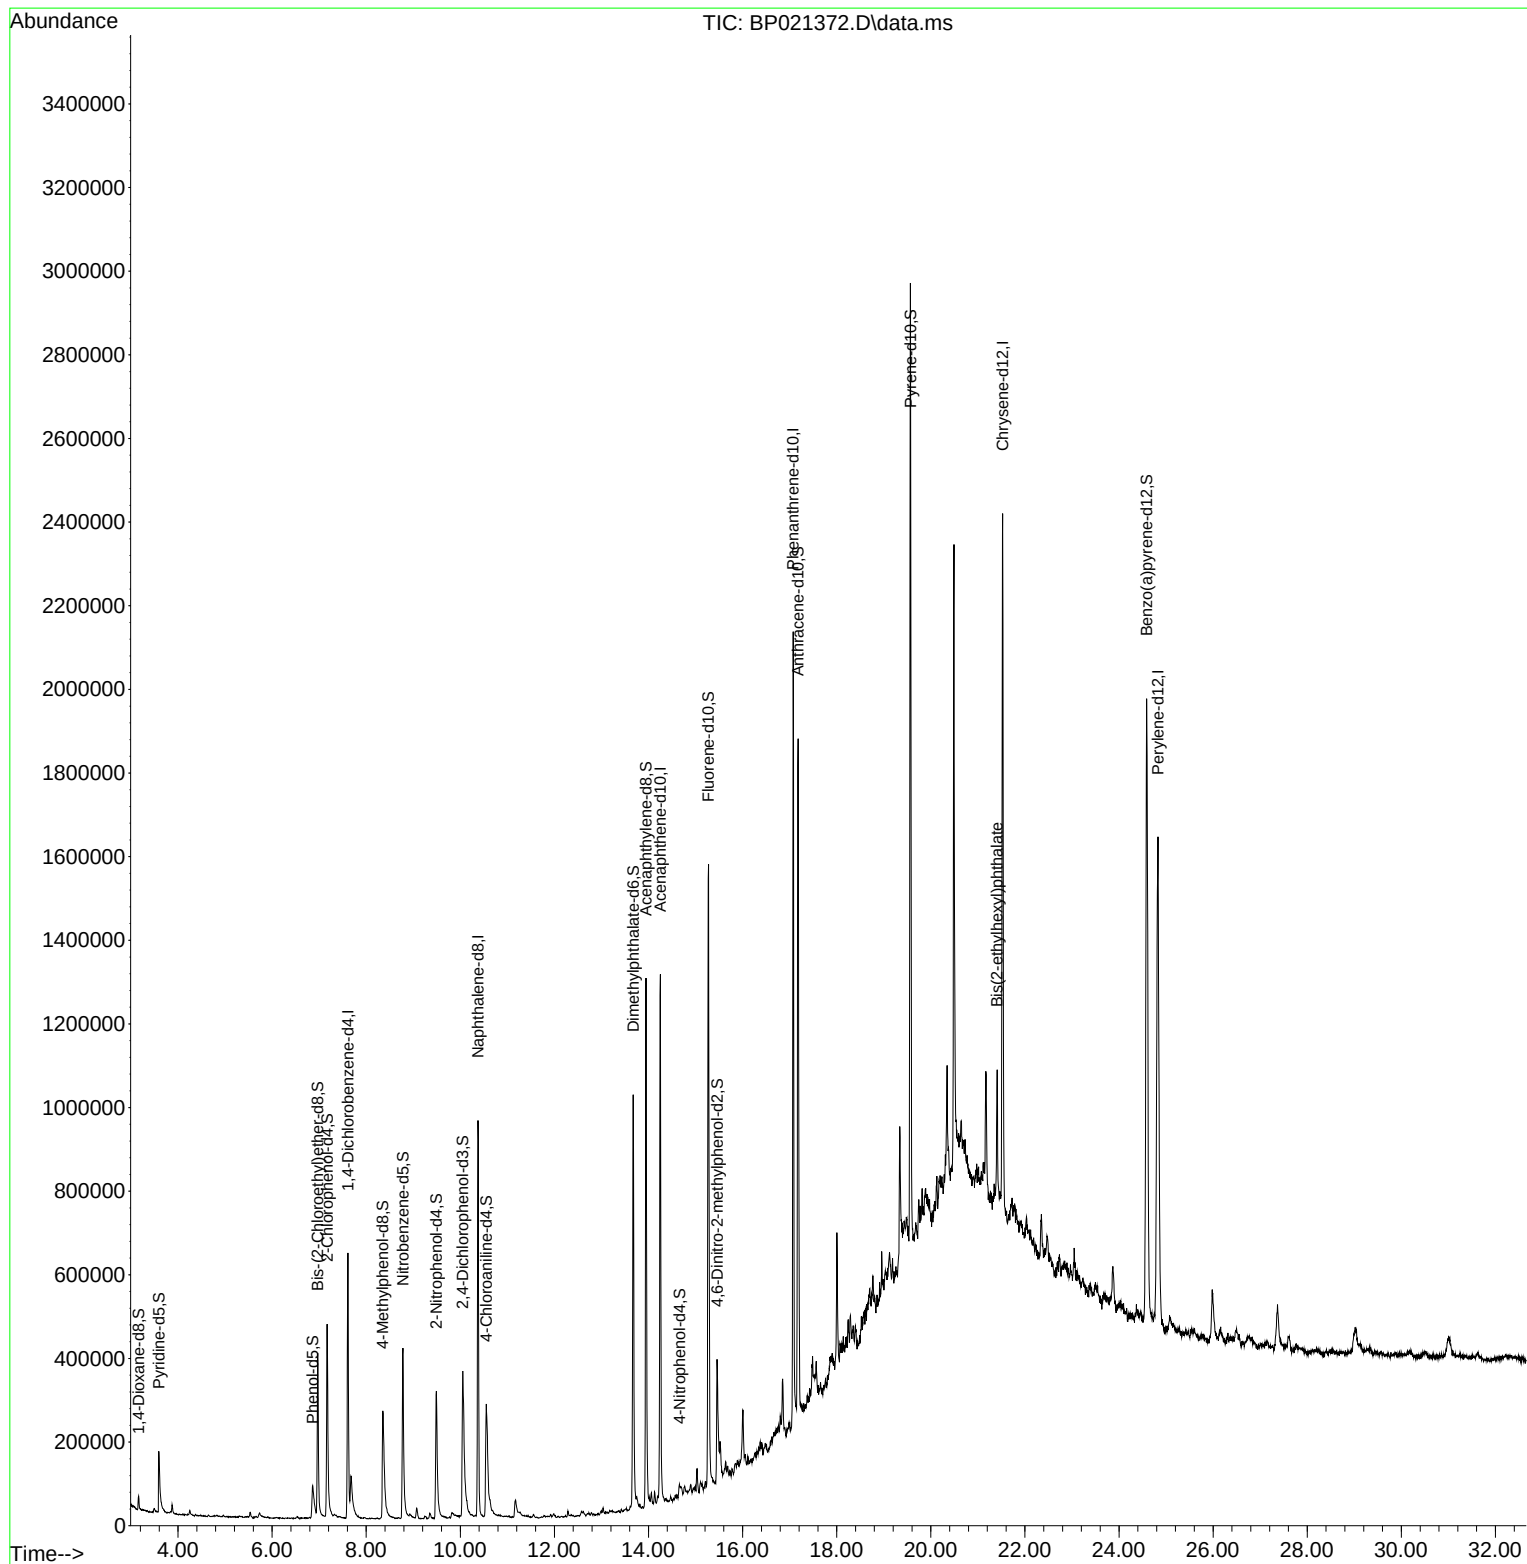

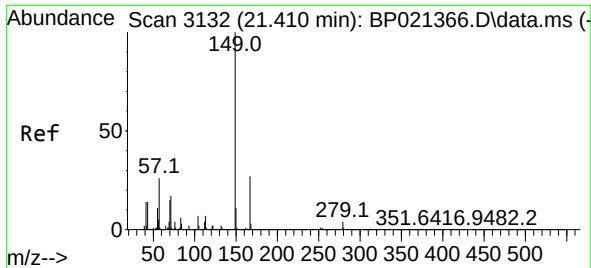

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.352 ng/ul
 RT: 21.410 min Scan# 31
 Delta R.T. -0.011 min
 Lab File: BP021372.D
 Acq: 05 Aug 2024 14:37

Instrument :
 BNA_P
 ClientSampleId :
 E1GA5

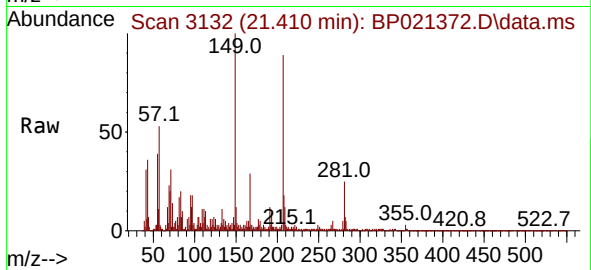

Tgt Ion:149 Resp: 11440
 Ion Ratio Lower Upper
 149 100
 167 28.6 22.1 33.1
 279 5.2 3.7 5.5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/07/2024

