

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080524\
 Data File : BP021367.D
 Acq On : 05 Aug 2024 10:04
 Operator : CG/JU
 Sample : PB162175BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	39	rBV	41775	59123	1.37%	0.140%
2	3.593	100	103	123	rBV	416624	802115	18.52%	1.895%
3	3.887	150	153	159	rVB2	10263	13856	0.32%	0.033%
4	6.852	651	657	672	rBV	328906	964382	22.27%	2.279%
5	6.975	673	678	695	rVB	442300	793111	18.31%	1.874%
6	7.181	706	713	729	rBV	562425	1040355	24.02%	2.458%
7	7.622	781	788	806	rBV	531122	988374	22.82%	2.335%
8	8.357	907	913	939	rBV	459500	1260999	29.12%	2.980%
9	8.787	979	986	1006	rBV	491019	1008905	23.30%	2.384%
10	9.493	1098	1106	1129	rBV	375108	859955	19.86%	2.032%
11	10.063	1196	1203	1226	rBV	357996	1188136	27.44%	2.807%
12	10.393	1251	1259	1276	rVB	788828	1415888	32.69%	3.346%
13	10.557	1279	1287	1311	rBV	436354	1233034	28.47%	2.914%
14	12.028	1528	1537	1543	rBV7	7361	21004	0.49%	0.050%
15	13.669	1808	1816	1843	rBV	937311	1970206	45.49%	4.655%
16	13.951	1856	1864	1888	rBV	1436207	2333035	53.87%	5.513%
17	14.257	1907	1916	1933	rBV	1179128	1958402	45.22%	4.628%
18	14.616	1969	1977	1980	rBV3	131097	287493	6.64%	0.679%
19	15.004	2039	2043	2047	rVB7	4165	5981	0.14%	0.014%
20	15.275	2082	2089	2106	rBV	1805066	2985246	68.93%	7.054%
21	15.463	2114	2121	2142	rBV	348221	849989	19.63%	2.008%
22	16.075	2222	2225	2231	rVB6	7566	10439	0.24%	0.025%
23	16.745	2335	2339	2343	rBV7	3569	5554	0.13%	0.013%
24	16.863	2356	2359	2364	rBV3	3951	5794	0.13%	0.014%
25	17.081	2389	2396	2407	rBV	1820402	2458972	56.78%	5.810%
26	17.175	2407	2412	2436	rVB2	1744897	3350433	77.36%	7.917%
27	19.110	2737	2741	2747	rBV6	27585	42269	0.98%	0.100%
28	19.198	2753	2756	2762	rBV	21488	32488	0.75%	0.077%
29	19.569	2812	2819	2834	rBV	2254574	4154606	95.93%	9.817%
30	21.533	3147	3153	3170	rBV2	1442280	2738877	63.24%	6.472%
31	24.598	3665	3674	3697	rVB2	1550439	4330707	100.00%	10.233%
32	24.833	3705	3714	3731	rVB	965605	3150438	72.75%	7.444%




Sum of corrected areas: 42320166

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080524\
Data File : BP021367.D
Acq On : 05 Aug 2024 10:04
Operator : CG/JU
Sample : PB162175BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK175

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

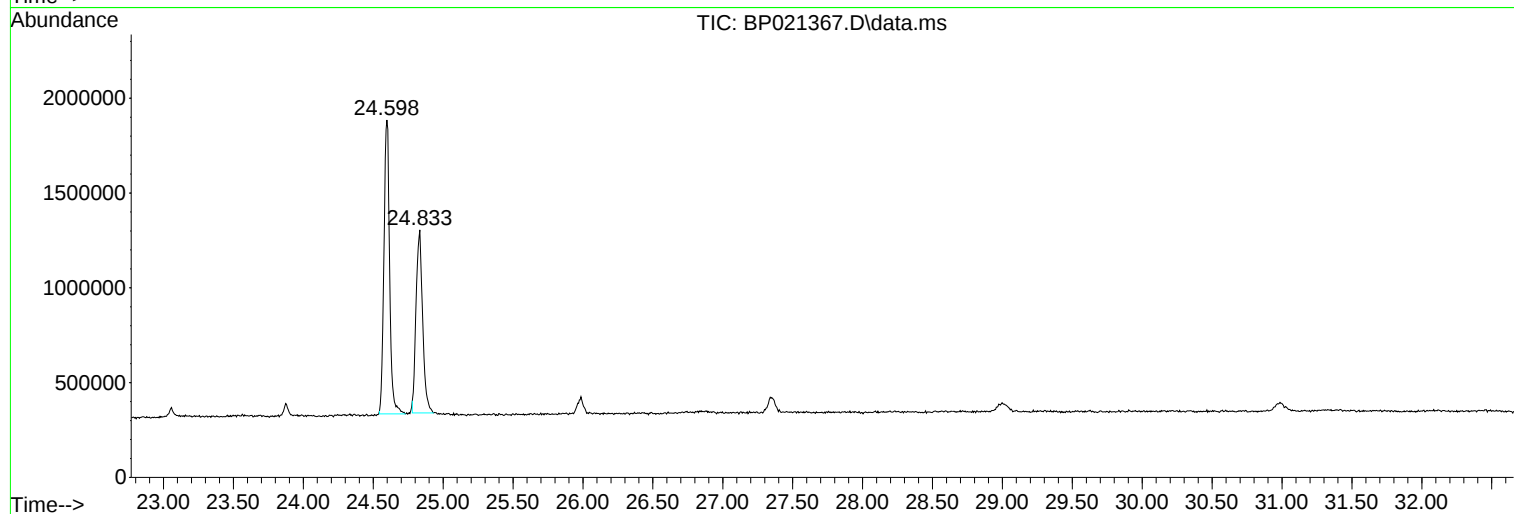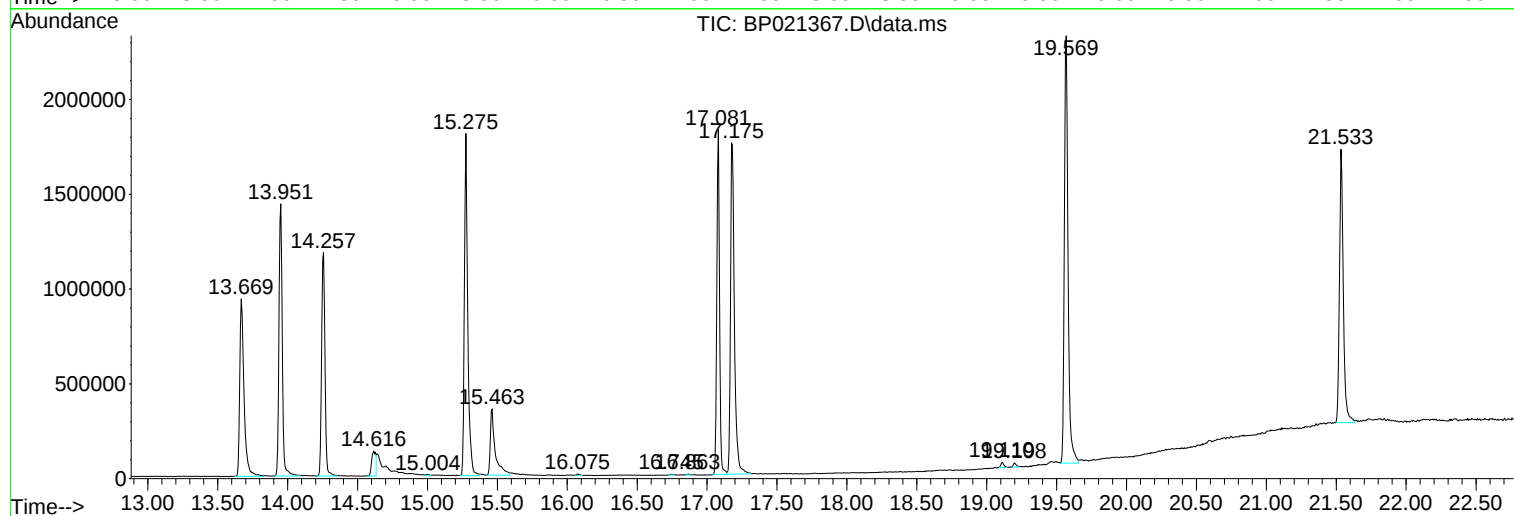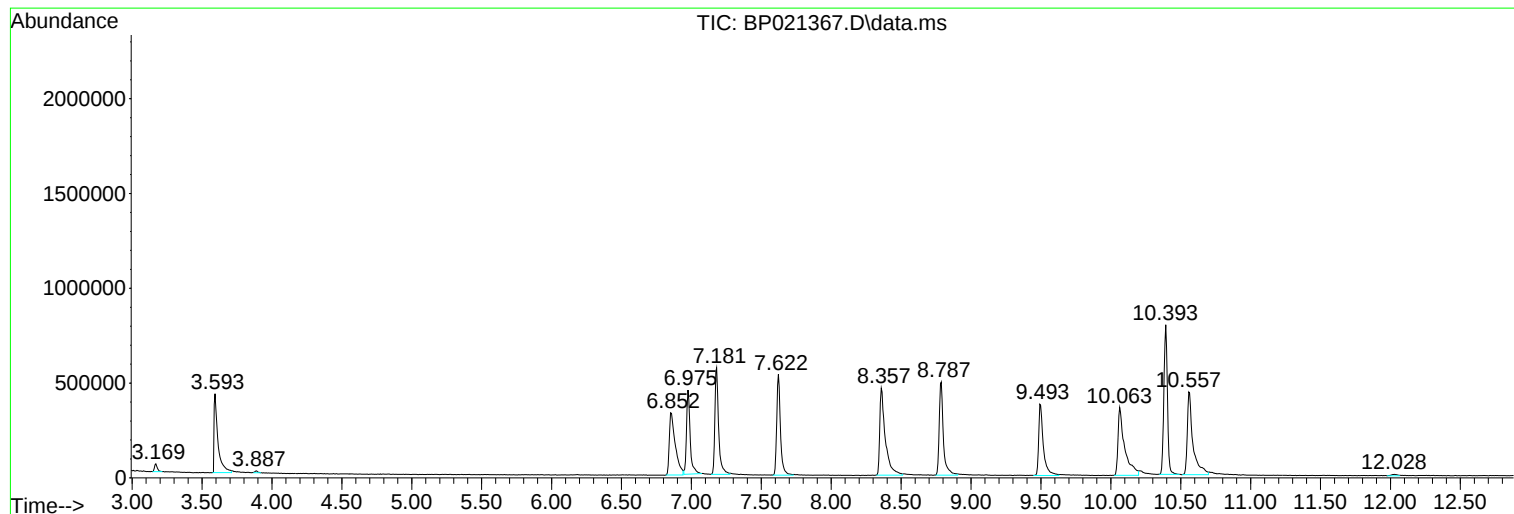

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080524\
Data File : BP021367.D
Acq On : 05 Aug 2024 10:04
Operator : CG/JU
Sample : PB162175BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK175

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080524\
Data File : BP021367.D
Acq On : 05 Aug 2024 10:04
Operator : CG/JU
Sample : PB162175BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK175

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc