

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016510.D
 Acq On : 07 Aug 2023 10:27
 Operator : MA/JU
 Sample : PB154583BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK583

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	16	20	29	rVB	143229	206522	2.46%	0.204%
2	3.840	89	94	111	rBV	1762350	2795195	33.27%	2.765%
3	4.164	145	149	153	rBV	28385	38668	0.46%	0.038%
4	7.205	659	666	674	rBV	2121410	3276140	39.00%	3.241%
5	7.405	693	700	709	rVB	1759184	2713956	32.30%	2.685%
6	7.587	723	731	741	rBV	2111990	3333722	39.68%	3.298%
7	8.069	805	813	821	rBV	1895940	2968862	35.34%	2.937%
8	8.763	923	931	946	rBV	2351058	3861374	45.96%	3.820%
9	9.263	1008	1016	1027	rBV	1781547	2910730	34.65%	2.880%
10	9.981	1127	1138	1149	rBV	1314609	2136091	25.43%	2.113%
11	10.504	1219	1227	1239	rBV	2167068	3634205	43.26%	3.595%
12	10.899	1285	1294	1302	rBV	2414111	3974663	47.31%	3.932%
13	11.051	1309	1320	1334	rBV	2227575	3725274	44.34%	3.685%
14	12.475	1556	1562	1568	rBV	42806	65517	0.78%	0.065%
15	13.498	1733	1736	1741	rVB5	5224	8416	0.10%	0.008%
16	13.563	1741	1747	1754	rBV	20636	39533	0.47%	0.039%
17	13.681	1761	1767	1773	rVB7	6444	9805	0.12%	0.010%
18	14.128	1836	1843	1856	rBV	3208053	4491116	53.46%	4.443%
19	14.222	1856	1859	1865	rVB7	6034	12965	0.15%	0.013%
20	14.416	1885	1892	1905	rBV	4044755	5906213	70.30%	5.843%
21	14.716	1936	1943	1951	rBV	3158968	4596336	54.71%	4.547%
22	14.904	1969	1975	1996	rBV	1262291	2063785	24.56%	2.042%
23	15.710	2105	2112	2124	rBV	4908262	7088153	84.37%	7.012%
24	15.822	2125	2131	2147	rVV	930933	1314810	15.65%	1.301%
25	15.945	2148	2152	2157	rVB3	24420	37424	0.45%	0.037%
26	16.281	2204	2209	2216	rBV9	4861	12038	0.14%	0.012%
27	17.145	2353	2356	2361	rVB7	7607	10402	0.12%	0.010%
28	17.269	2373	2377	2379	rBV4	9925	12077	0.14%	0.012%
29	17.481	2407	2413	2423	rBV	3641695	5140060	61.18%	5.085%
30	17.581	2424	2430	2446	rVB	5238909	7256817	86.38%	7.179%
31	18.328	2553	2557	2561	rBV7	16361	25857	0.31%	0.026%
32	19.386	2733	2737	2743	rBV4	63823	89465	1.06%	0.089%
33	19.451	2745	2748	2754	rVB2	56833	74015	0.88%	0.073%
34	19.810	2804	2809	2818	rBV	6205182	8085684	96.24%	7.999%
35	21.574	3104	3109	3120	rBV	3878401	5243037	62.41%	5.187%
36	23.998	3514	3521	3532	rVB2	4000114	8401325	100.00%	8.311%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016510.D
Acq On : 07 Aug 2023 10:27
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Title : SVOA CALIBRATION

37	24.168	3543	3550	3562	rVB	2576912	5523586	65.75%	5.464%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 101083838

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016510.D
Acq On : 07 Aug 2023 10:27
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

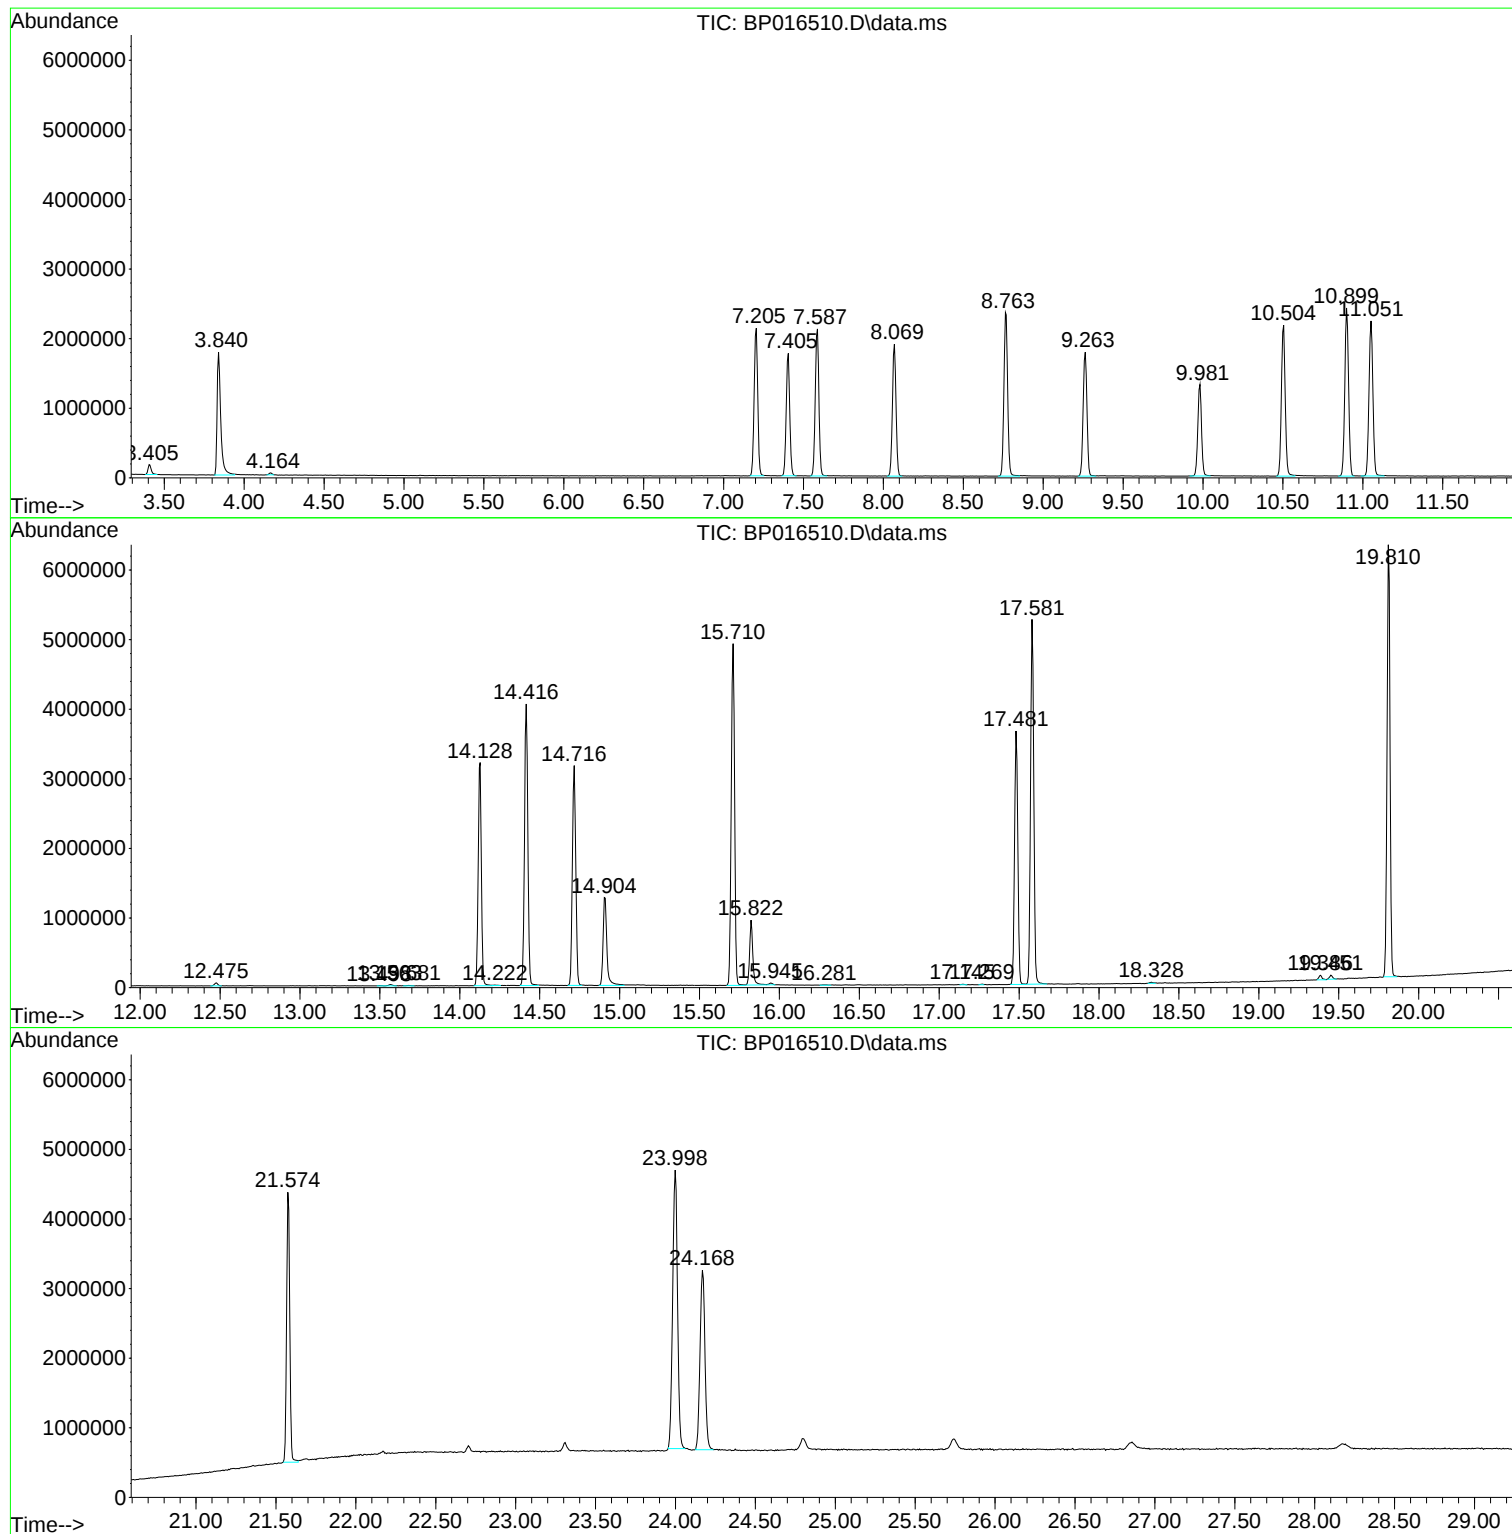

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016510.D
Acq On : 07 Aug 2023 10:27
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016510.D
Acq On : 07 Aug 2023 10:27
Operator : MA/JU
Sample : PB154583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------