

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016514.D
 Acq On : 07 Aug 2023 12:44
 Operator : MA/JU
 Sample : PB154581BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK581

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	16	20	34	rVB	157560	238610	2.70%	0.229%
2	3.840	90	94	114	rBV	1814879	2909507	32.95%	2.798%
3	4.164	145	149	156	rVB	28542	44276	0.50%	0.043%
4	7.199	656	665	678	rBV	2154557	3438935	38.95%	3.307%
5	7.399	693	699	709	rVB	1781425	2818746	31.93%	2.711%
6	7.587	723	731	739	rBV	2152651	3466630	39.26%	3.334%
7	8.069	805	813	821	rBV	1917935	3095687	35.06%	2.977%
8	8.763	923	931	947	rBV	2544298	4009989	45.42%	3.856%
9	9.263	1008	1016	1023	rBV	1837425	3039516	34.43%	2.923%
10	9.975	1128	1137	1156	rBV	1356177	2256061	25.55%	2.170%
11	10.499	1219	1226	1239	rBV	2228301	3774651	42.75%	3.630%
12	10.899	1283	1294	1302	rBV	2535831	4124962	46.72%	3.967%
13	11.052	1310	1320	1336	rBV	2289362	3861897	43.74%	3.714%
14	12.475	1555	1562	1569	rBV2	43723	71794	0.81%	0.069%
15	13.569	1742	1748	1753	rBV3	19630	34862	0.39%	0.034%
16	13.681	1760	1767	1774	rVB7	7315	14177	0.16%	0.014%
17	14.128	1836	1843	1855	rBV	3222554	4583085	51.91%	4.408%
18	14.216	1855	1858	1864	rVB8	5984	13428	0.15%	0.013%
19	14.416	1884	1892	1912	rBV	4210947	6057392	68.61%	5.825%
20	14.716	1936	1943	1952	rBV	3195253	4712143	53.37%	4.532%
21	14.904	1968	1975	1998	rBV	1354046	2142012	24.26%	2.060%
22	15.710	2105	2112	2120	rBV	5198226	7230798	81.90%	6.954%
23	15.822	2125	2131	2146	rVV	970434	1382052	15.65%	1.329%
24	15.945	2148	2152	2158	rVB2	26503	40333	0.46%	0.039%
25	17.263	2373	2376	2381	rVB2	7172	11062	0.13%	0.011%
26	17.481	2406	2413	2423	rBV	3705998	5220089	59.12%	5.020%
27	17.581	2423	2430	2442	rBV2	5169926	7358219	83.34%	7.076%
28	18.322	2553	2556	2560	rBV6	15921	25090	0.28%	0.024%
29	19.386	2733	2737	2743	rBV2	61391	83101	0.94%	0.080%
30	19.451	2745	2748	2753	rVB	53120	71184	0.81%	0.068%
31	19.810	2803	2809	2818	rBV	6493143	8260274	93.56%	7.944%
32	21.575	3104	3109	3115	rBV	4026445	5208060	58.99%	5.009%
33	23.998	3513	3521	3531	rBV2	4255668	8828926	100.00%	8.491%
34	24.168	3543	3550	3566	rVB	2672486	5554217	62.91%	5.342%

Sum of corrected areas: 103981765




Instrument :
BNA_P
ClientSampleId :
SBLK581

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016514.D
Acq On : 07 Aug 2023 12:44
Operator : MA/JU
Sample : PB154581BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

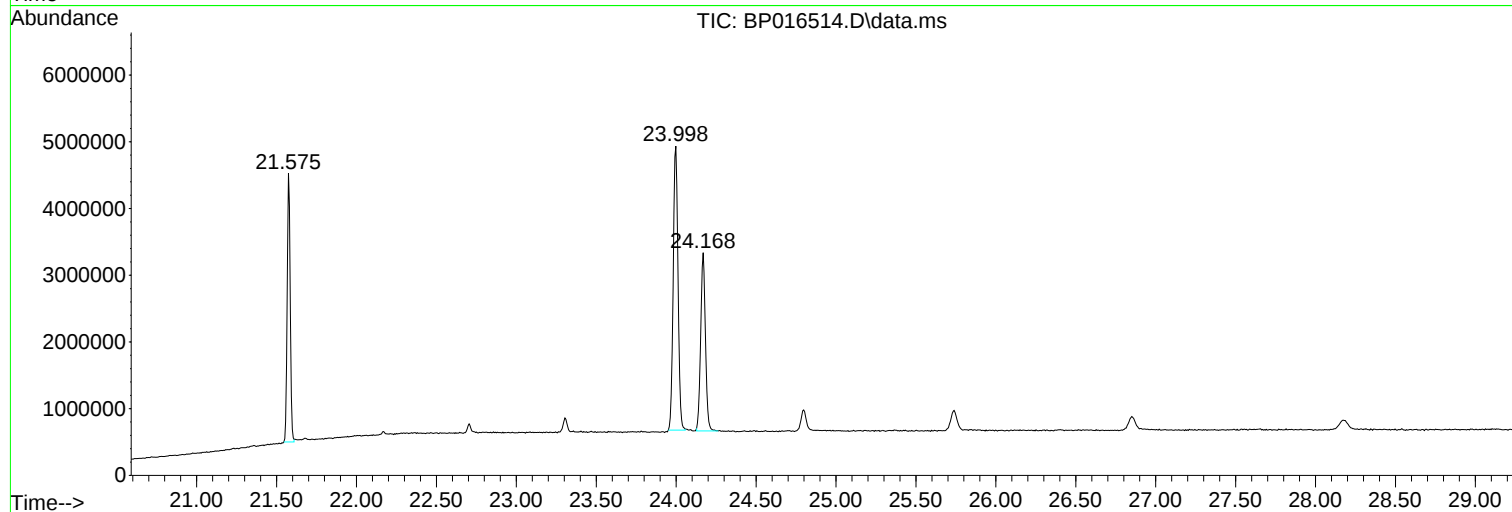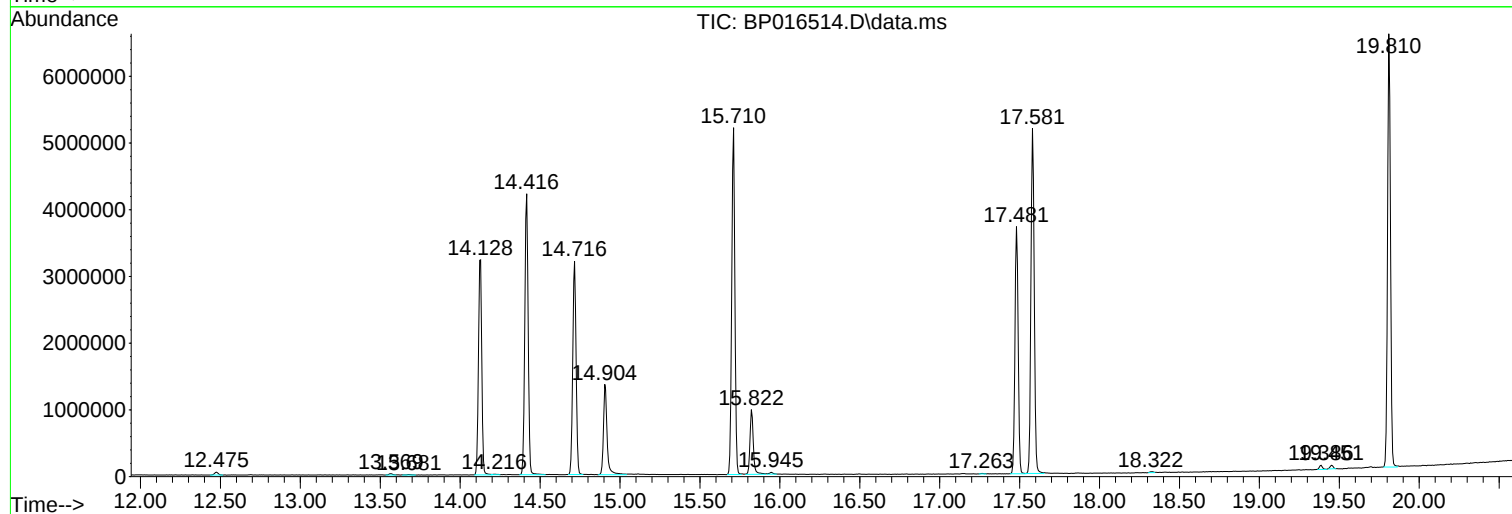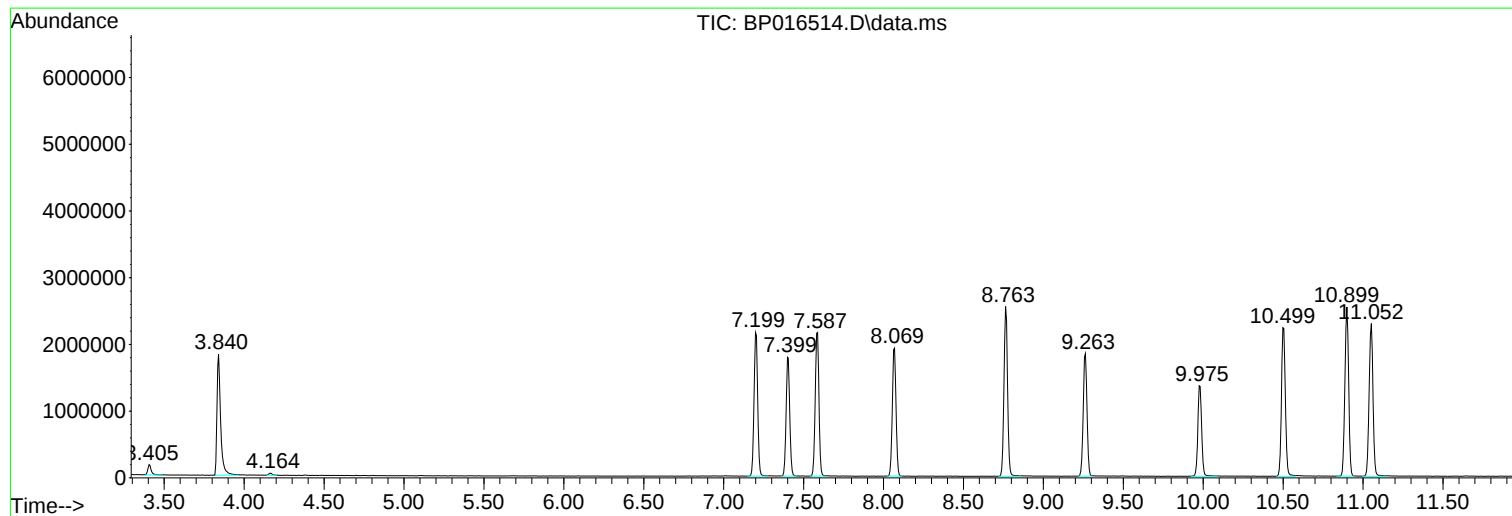

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016514.D
Acq On : 07 Aug 2023 12:44
Operator : MA/JU
Sample : PB154581BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016514.D
Acq On : 07 Aug 2023 12:44
Operator : MA/JU
Sample : PB154581BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc