

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016519.D
 Acq On : 07 Aug 2023 15:42
 Operator : MA/JU
 Sample : PB154647BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK647

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	15	20	30	rVB	119614	179755	2.53%	0.190%
2	3.834	88	93	111	rBV	1492387	2369308	33.36%	2.500%
3	4.158	143	148	158	rVB	37312	60633	0.85%	0.064%
4	4.581	216	220	223	rBV5	5966	12101	0.17%	0.013%
5	7.199	657	665	675	rBV	1764178	2816857	39.66%	2.972%
6	7.399	692	699	708	rBV	1493968	2329352	32.80%	2.457%
7	7.581	723	730	739	rBV	1783736	2854245	40.19%	3.011%
8	8.063	804	812	820	rBV	2325459	3622063	51.00%	3.821%
9	8.763	923	931	941	rBV	2058806	3293878	46.38%	3.475%
10	9.258	1007	1015	1029	rBV	1572987	2531425	35.64%	2.671%
11	9.975	1129	1137	1148	rBV	1133330	1831970	25.79%	1.933%
12	10.499	1215	1226	1242	rBV	1912846	3134241	44.13%	3.307%
13	10.899	1282	1294	1302	rBV	2863934	4815154	67.80%	5.080%
14	11.052	1312	1320	1336	rBV	1856948	3195231	44.99%	3.371%
15	12.475	1555	1562	1569	rBV2	36592	59208	0.83%	0.062%
16	13.563	1742	1747	1753	rBV3	19176	34294	0.48%	0.036%
17	13.681	1762	1767	1772	rVB8	6298	11673	0.16%	0.012%
18	14.128	1836	1843	1856	rBV	2753738	3858119	54.32%	4.070%
19	14.222	1856	1859	1864	rVB7	5297	8386	0.12%	0.009%
20	14.416	1885	1892	1900	rBV	3497221	4959001	69.82%	5.232%
21	14.716	1936	1943	1957	rBV	3654875	5429009	76.44%	5.728%
22	14.910	1969	1976	1997	rBV	1151330	1787626	25.17%	1.886%
23	15.710	2105	2112	2125	rBV	4231213	5968724	84.04%	6.297%
24	15.828	2126	2132	2142	rBV	815364	1145200	16.12%	1.208%
25	15.951	2150	2153	2157	rVB	20491	24640	0.35%	0.026%
26	16.504	2242	2247	2249	rVB6	6154	8920	0.13%	0.009%
27	17.151	2353	2357	2361	rBV6	5786	9181	0.13%	0.010%
28	17.263	2374	2376	2382	rVB4	10229	13337	0.19%	0.014%
29	17.487	2407	2414	2424	rBV	3969331	5858101	82.48%	6.180%
30	17.587	2424	2431	2443	rBV	4219624	6173717	86.93%	6.513%
31	18.322	2553	2556	2563	rBV4	32207	58572	0.82%	0.062%
32	19.386	2734	2737	2741	rVB3	50485	59127	0.83%	0.062%
33	19.457	2746	2749	2753	rVB	39800	48357	0.68%	0.051%
34	19.816	2804	2810	2816	rBV	5510911	6980801	98.29%	7.365%
35	21.580	3105	3110	3120	rBV	4372906	5862991	82.55%	6.185%
36	24.004	3515	3522	3532	rVB2	3441633	7102336	100.00%	7.493%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016519.D
Acq On : 07 Aug 2023 15:42
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Title : SVOA CALIBRATION

37	24.174	3544	3551	3564	rVB	2924328	6280538	88.43%	6.626%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 94788071

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016519.D
Acq On : 07 Aug 2023 15:42
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

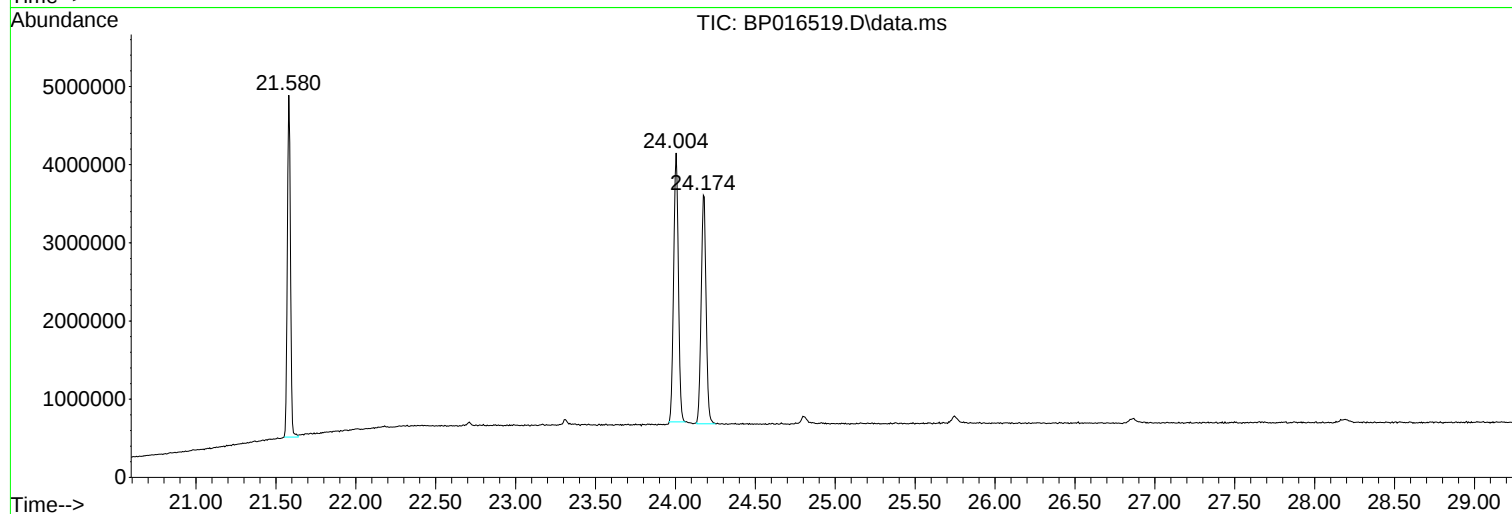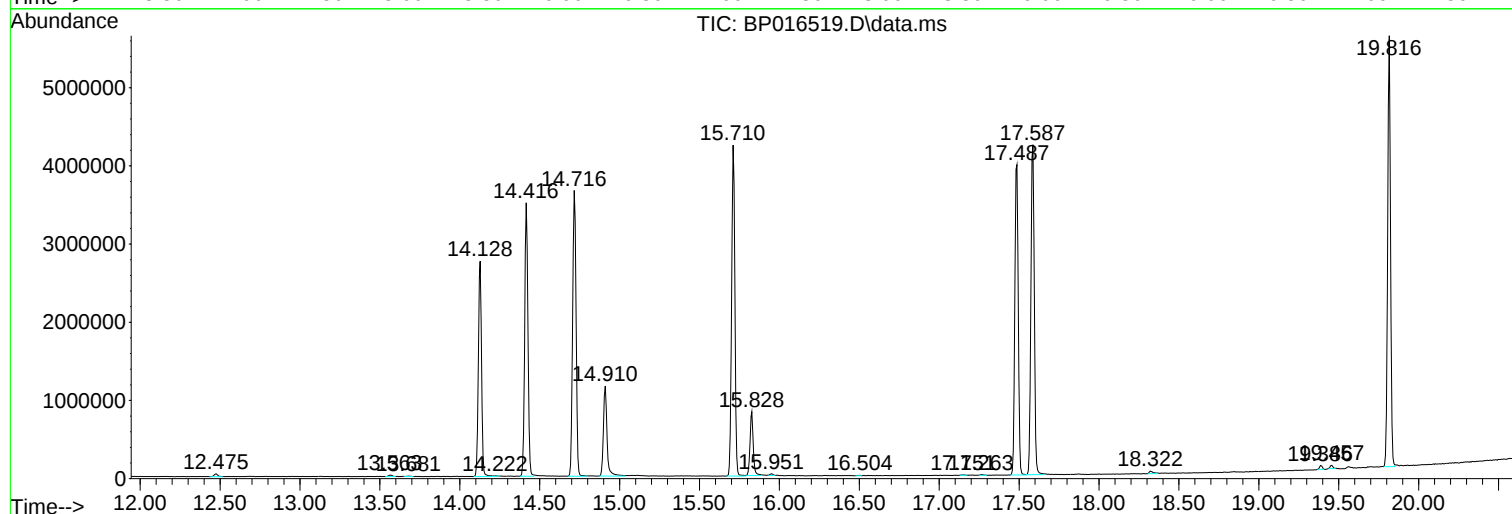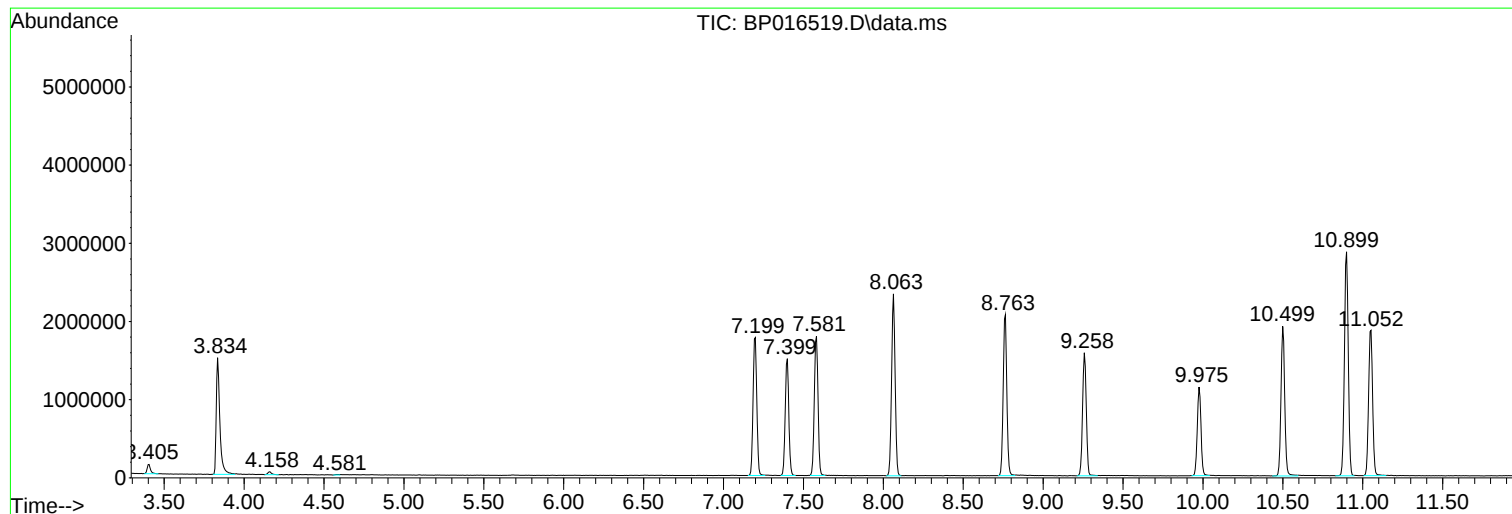

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016519.D
Acq On : 07 Aug 2023 15:42
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016519.D
Acq On : 07 Aug 2023 15:42
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc