

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016521.D
 Acq On : 07 Aug 2023 16:51
 Operator : MA/JU
 Sample : 03901-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH315

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	16	20	24	rBV	72244	95610	1.18%	0.119%
2	3.440	24	26	32	rVB	20564	27952	0.35%	0.035%
3	3.699	67	70	74	rVB3	7442	8836	0.11%	0.011%
4	3.840	90	94	109	rBV	305048	522470	6.46%	0.653%
5	4.011	119	123	125	rBV3	12136	17037	0.21%	0.021%
6	4.052	125	130	137	rVB	61276	101486	1.25%	0.127%
7	4.164	145	149	154	rVB	24976	35736	0.44%	0.045%
8	5.105	305	309	316	rVB3	12135	18916	0.23%	0.024%
9	5.693	407	409	418	rVB7	7966	13709	0.17%	0.017%
10	7.199	658	665	673	rBV	378821	599830	7.42%	0.749%
11	7.399	693	699	710	rVB	1606852	2511386	31.05%	3.138%
12	7.581	723	730	741	rBV	1472241	2329278	28.80%	2.910%
13	8.064	805	812	823	rBV	1418859	2295167	28.38%	2.868%
14	8.763	923	931	947	rBV	1077511	1681798	20.80%	2.101%
15	9.263	1006	1016	1027	rBV	1650860	2747993	33.98%	3.433%
16	9.975	1128	1137	1148	rBV	1148034	1903821	23.54%	2.379%
17	10.499	1219	1226	1239	rBV	1768204	2968576	36.71%	3.709%
18	10.899	1286	1294	1302	rBV	1813104	3014634	37.28%	3.766%
19	11.052	1312	1320	1334	rBV	1719376	2838035	35.09%	3.546%
20	12.475	1555	1562	1568	rBV2	38876	63086	0.78%	0.079%
21	12.681	1592	1597	1605	rBV10	4914	11444	0.14%	0.014%
22	13.563	1740	1747	1754	rBV5	17761	30921	0.38%	0.039%
23	13.681	1759	1767	1771	rVV9	5632	11376	0.14%	0.014%
24	14.122	1836	1842	1854	rBV	2884090	4126001	51.02%	5.155%
25	14.416	1885	1892	1908	rBV	3701686	5424089	67.07%	6.777%
26	14.716	1936	1943	1957	rBV	2391585	3444554	42.59%	4.304%
27	14.910	1969	1976	1985	rBV	161168	294319	3.64%	0.368%
28	15.140	2013	2015	2019	rVB5	12043	13929	0.17%	0.017%
29	15.710	2105	2112	2125	rBV	4593602	6583976	81.41%	8.226%
30	15.822	2125	2131	2145	rVV	920729	1300733	16.08%	1.625%
31	15.945	2148	2152	2161	rVB3	24993	42561	0.53%	0.053%
32	16.498	2241	2246	2251	rVB9	8223	14575	0.18%	0.018%
33	17.269	2372	2377	2383	rVB7	7567	13491	0.17%	0.017%
34	17.481	2406	2413	2423	rBV	2705048	3797537	46.96%	4.745%
35	17.581	2423	2430	2451	rVV	4923895	6978484	86.29%	8.719%
36	18.316	2552	2555	2564	rBV4	34466	67274	0.83%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016521.D
Acq On : 07 Aug 2023 16:51
Operator : MA/JU
Sample : 03901-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH315

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Title : SVOA CALIBRATION

37	19.381	2733	2736	2741	rBV4	57092	77954	0.96%	0.097%
38	19.451	2744	2748	2752	rVB	44295	65887	0.81%	0.082%
39	19.557	2762	2766	2770	rBV6	32297	58122	0.72%	0.073%
40	19.810	2803	2809	2818	rBV	6147677	7897573	97.65%	9.867%
41	21.575	3104	3109	3117	rBV	2980839	3853386	47.65%	4.814%
42	23.998	3513	3521	3531	rVB2	3877073	8087390	100.00%	10.104%
43	24.163	3543	3549	3563	rVB	1852266	4049531	50.07%	5.059%




Sum of corrected areas: 80040463

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016521.D
Acq On : 07 Aug 2023 16:51
Operator : MA/JU
Sample : 03901-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH315

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

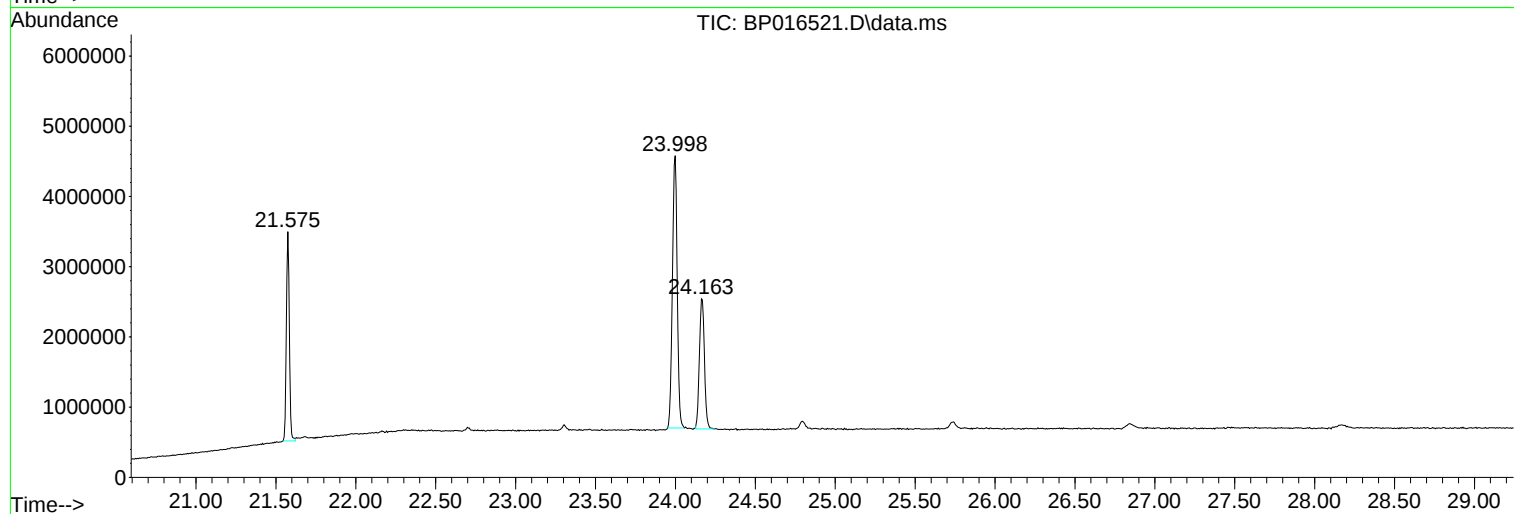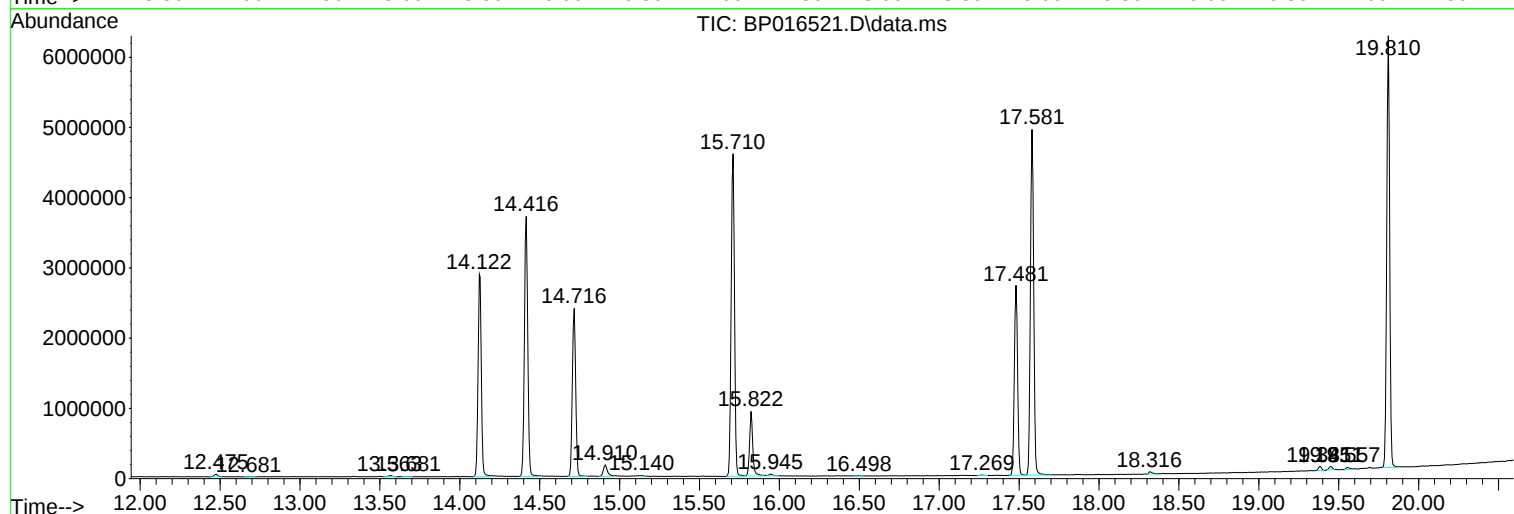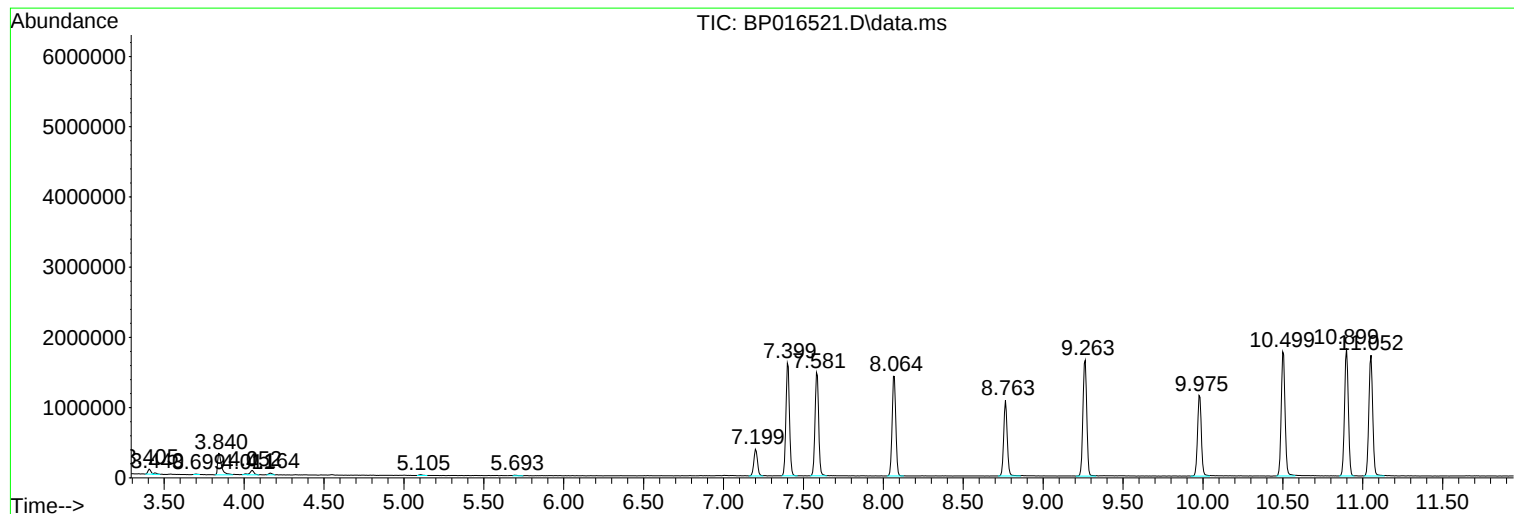

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016521.D
Acq On : 07 Aug 2023 16:51
Operator : MA/JU
Sample : 03901-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH315

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016521.D
Acq On : 07 Aug 2023 16:51
Operator : MA/JU
Sample : 03901-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH315

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------