

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016523.D
 Acq On : 07 Aug 2023 17:59
 Operator : MA/JU
 Sample : PB154677BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK677

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	15	20	29	rVB	142153	193289	2.60%	0.209%
2	3.840	90	94	115	rBV	1624662	2596663	34.91%	2.809%
3	4.164	145	149	155	rVB	33173	49900	0.67%	0.054%
4	7.199	658	665	678	rBV	1930352	3050166	41.00%	3.299%
5	7.399	692	699	710	rVB	1605350	2531682	34.03%	2.738%
6	7.581	721	730	741	rBV	1920931	3071322	41.29%	3.322%
7	8.069	805	813	823	rVB	1828154	2957850	39.76%	3.199%
8	8.763	924	931	945	rBV	2226148	3557227	47.82%	3.848%
9	9.263	1008	1016	1027	rBV	1667652	2703259	36.34%	2.924%
10	9.981	1125	1138	1149	rBV	1198791	1981918	26.64%	2.144%
11	10.504	1218	1227	1243	rBV	1986575	3333028	44.80%	3.605%
12	10.898	1285	1294	1302	rBV	2355752	3917151	52.66%	4.237%
13	11.051	1312	1320	1335	rBV	2037323	3431179	46.12%	3.711%
14	12.475	1556	1562	1570	rVB2	37677	66647	0.90%	0.072%
15	13.563	1740	1747	1752	rBV3	27161	45869	0.62%	0.050%
16	13.681	1762	1767	1772	rVB5	6954	10035	0.13%	0.011%
17	14.122	1836	1842	1852	rBV	2919541	4101369	55.13%	4.436%
18	14.416	1884	1892	1909	rBV	3648213	5350842	71.93%	5.788%
19	14.716	1936	1943	1951	rBV	3026530	4382207	58.91%	4.740%
20	14.904	1967	1975	1987	rBV	1190364	1881070	25.29%	2.035%
21	15.386	2052	2057	2060	rBV7	3557	8266	0.11%	0.009%
22	15.710	2105	2112	2123	rBV	4469212	6398604	86.01%	6.921%
23	15.822	2125	2131	2149	rVV	896598	1295996	17.42%	1.402%
24	15.945	2149	2152	2159	rVB3	20513	35410	0.48%	0.038%
25	17.145	2354	2356	2361	rVB5	5982	7541	0.10%	0.008%
26	17.263	2372	2376	2382	rBV7	8218	14937	0.20%	0.016%
27	17.480	2406	2413	2420	rBV	3328692	4689826	63.04%	5.073%
28	17.580	2424	2430	2443	rVV	4713025	6555293	88.12%	7.090%
29	18.328	2552	2557	2562	rBV8	16722	32345	0.43%	0.035%
30	19.386	2733	2737	2742	rBV2	55756	72349	0.97%	0.078%
31	19.451	2745	2748	2752	rVB	46172	60717	0.82%	0.066%
32	19.810	2803	2809	2817	rBV	5671336	7283481	97.91%	7.878%
33	21.574	3104	3109	3119	rBV	3442368	4564113	61.35%	4.937%
34	23.992	3513	3520	3532	rVB2	3542511	7439070	100.00%	8.046%
35	24.168	3543	3550	3560	rVB	2241978	4783331	64.30%	5.174%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016523.D
Acq On : 07 Aug 2023 17:59
Operator : MA/JU
Sample : PB154677BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 92453952

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016523.D
Acq On : 07 Aug 2023 17:59
Operator : MA/JU
Sample : PB154677BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

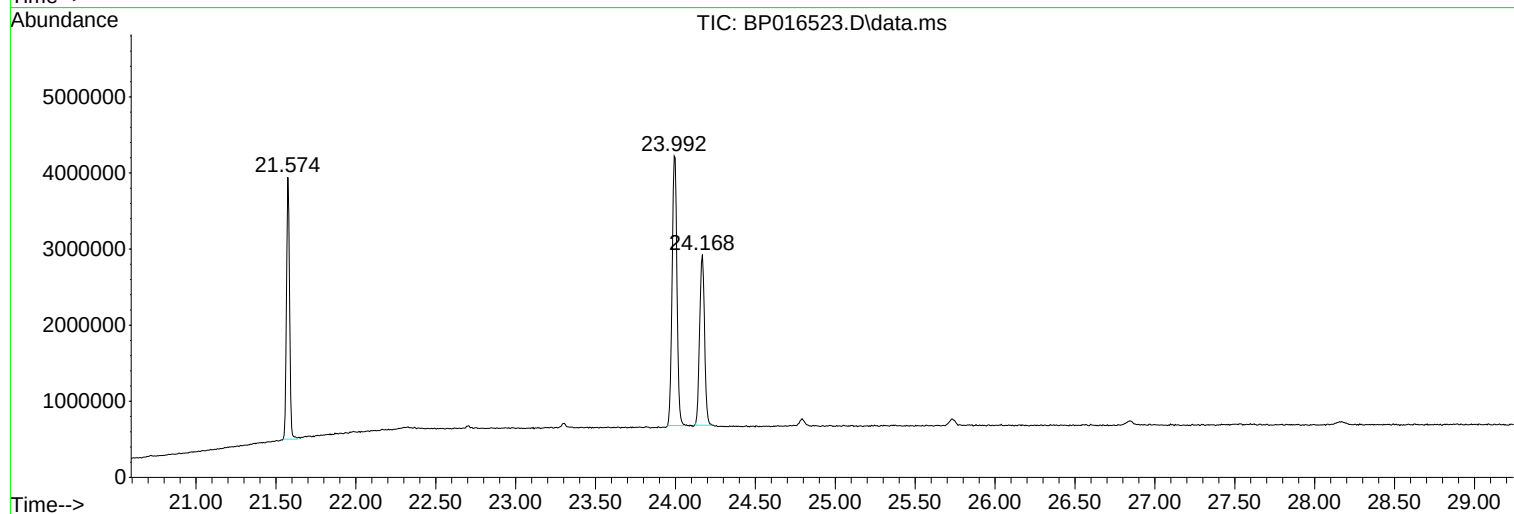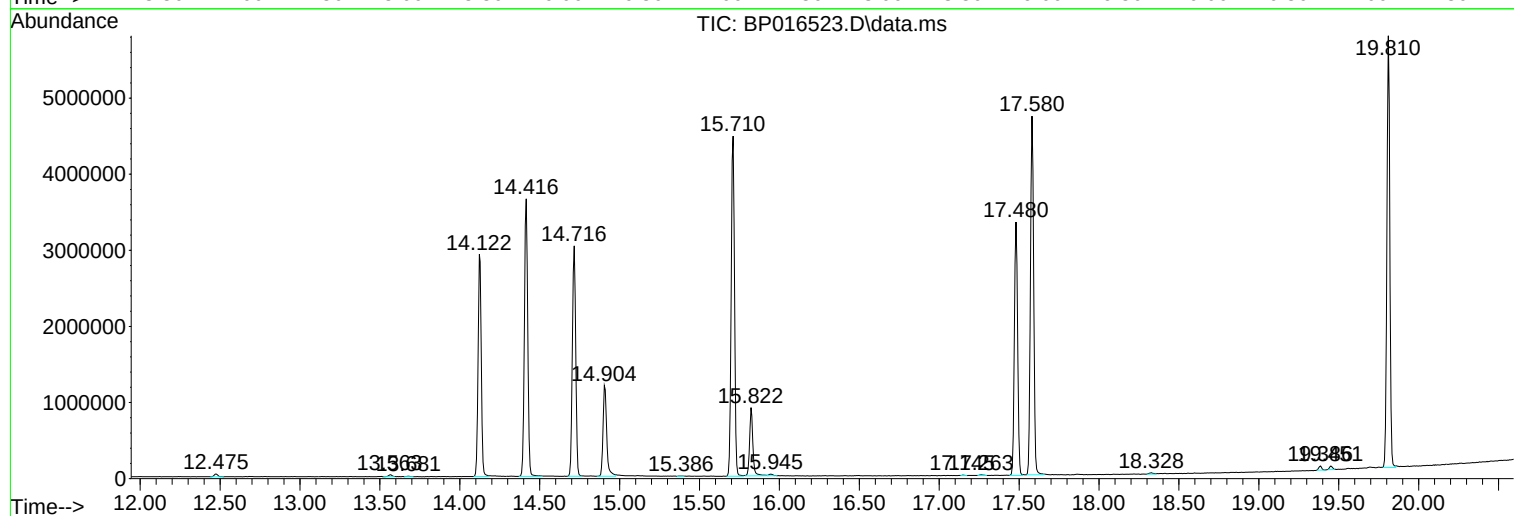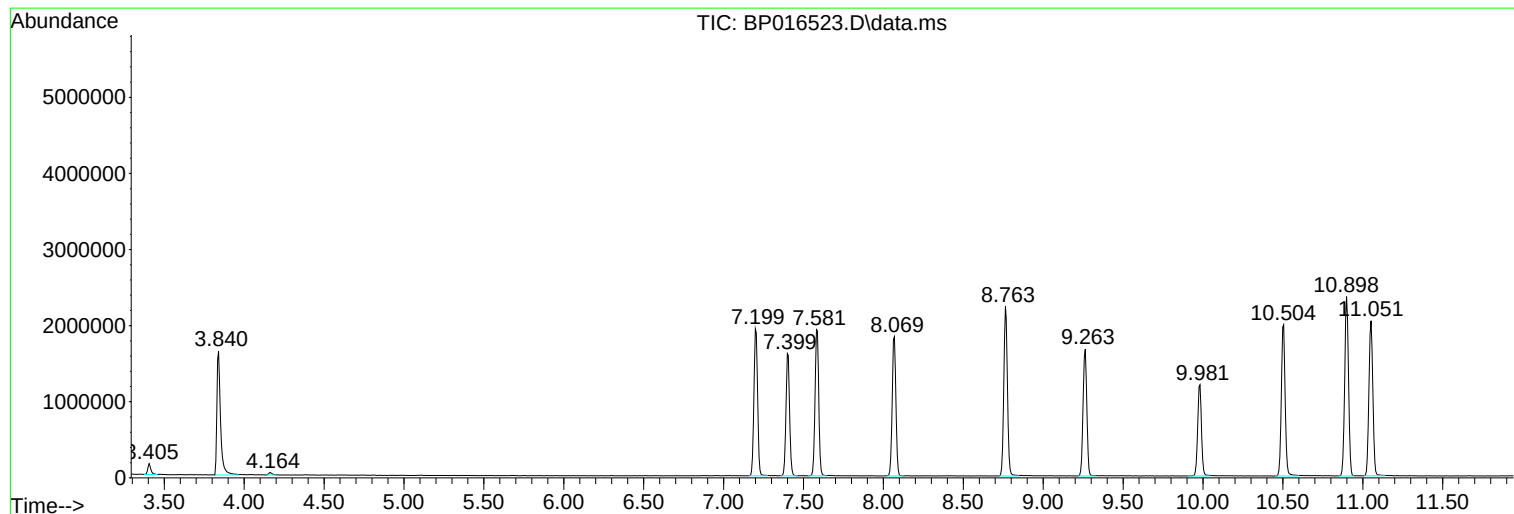

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016523.D
Acq On : 07 Aug 2023 17:59
Operator : MA/JU
Sample : PB154677BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016523.D
Acq On : 07 Aug 2023 17:59
Operator : MA/JU
Sample : PB154677BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------