

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016525.D
 Acq On : 07 Aug 2023 19:08
 Operator : MA/JU
 Sample : 03889-01DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.852	93	96	104	rBV	48170	79422	1.74%	0.219%
2	4.046	125	129	134	rBV3	6865	10691	0.23%	0.029%
3	4.164	144	149	157	rVB	31012	49261	1.08%	0.136%
4	5.375	350	355	359	rBV5	18806	29523	0.65%	0.081%
5	5.675	404	406	412	rVB7	5327	8395	0.18%	0.023%
6	6.511	543	548	553	rVB5	13616	19779	0.43%	0.054%
7	6.993	625	630	632	rBV6	5423	8922	0.19%	0.025%
8	7.205	658	666	674	rBV	34551	62737	1.37%	0.173%
9	7.399	694	699	707	rBV	152737	244015	5.33%	0.672%
10	7.581	723	730	738	rBV	117319	197700	4.32%	0.545%
11	8.069	805	813	824	rVB	1626732	2620336	57.26%	7.218%
12	8.605	898	904	909	rBV4	8259	17145	0.37%	0.047%
13	8.764	921	931	939	rBV	89200	157191	3.43%	0.433%
14	9.264	1008	1016	1027	rVB	139618	247463	5.41%	0.682%
15	9.428	1040	1044	1048	rVB7	5155	8526	0.19%	0.023%
16	9.546	1058	1064	1073	rVV7	9914	27095	0.59%	0.075%
17	9.828	1106	1112	1114	rBV7	5099	8463	0.18%	0.023%
18	9.975	1131	1137	1145	rBV	84520	138341	3.02%	0.381%
19	10.140	1162	1165	1170	rVB7	5486	8658	0.19%	0.024%
20	10.293	1181	1191	1197	rBV7	13615	35142	0.77%	0.097%
21	10.375	1200	1205	1208	rVV7	5302	9307	0.20%	0.026%
22	10.505	1219	1227	1234	rBV	138373	242633	5.30%	0.668%
23	10.563	1234	1237	1248	rVB	5848	16323	0.36%	0.045%
24	10.816	1276	1280	1284	rBV6	6910	10507	0.23%	0.029%
25	10.899	1286	1294	1300	rVV	2112274	3455581	75.51%	9.519%
26	10.952	1300	1303	1310	rVB	37351	59287	1.30%	0.163%
27	11.052	1310	1320	1329	rBV	137602	264170	5.77%	0.728%
28	11.263	1351	1356	1357	rVV5	5248	9069	0.20%	0.025%
29	11.299	1357	1362	1368	rVV6	11157	21824	0.48%	0.060%
30	11.363	1368	1373	1376	rVB7	6287	10927	0.24%	0.030%
31	11.481	1386	1393	1400	rVB	37525	68167	1.49%	0.188%
32	11.652	1415	1422	1427	rBV10	8726	18555	0.41%	0.051%
33	11.716	1427	1433	1436	rBV8	5673	9191	0.20%	0.025%
34	11.922	1459	1468	1469	rBV9	5495	12608	0.28%	0.035%
35	11.963	1469	1475	1478	rVV7	6873	13084	0.29%	0.036%
36	12.022	1478	1485	1493	rVV	40847	72683	1.59%	0.200%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016525.D
 Acq On : 07 Aug 2023 19:08
 Operator : MA/JU
 Sample : 03889-01DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

37	12.287	1522	1530	1537	rBV6	11027	23098	0.50%	0.064%
38	12.393	1543	1548	1551	rBV5	11203	19147	0.42%	0.053%
39	12.446	1551	1557	1564	rVB5	15067	39253	0.86%	0.108%
40	12.581	1577	1580	1585	rVB4	6920	8686	0.19%	0.024%
41	12.681	1593	1597	1602	rBV6	23228	42700	0.93%	0.118%
42	12.734	1603	1606	1611	rVV2	8661	11677	0.26%	0.032%
43	12.869	1622	1629	1633	rBV4	21606	40839	0.89%	0.112%
44	12.940	1638	1641	1645	rVV4	7471	9714	0.21%	0.027%
45	13.046	1656	1659	1663	rBV5	6743	9478	0.21%	0.026%
46	13.116	1668	1671	1677	rVB4	12806	18492	0.40%	0.051%
47	13.222	1685	1689	1693	rVB7	10028	15349	0.34%	0.042%
48	13.499	1734	1736	1743	rVV6	7117	11091	0.24%	0.031%
49	13.569	1743	1748	1753	rVB7	20666	36594	0.80%	0.101%
50	13.746	1768	1778	1788	rVB3	48043	136314	2.98%	0.375%
51	13.852	1791	1796	1797	rBV5	16386	20116	0.44%	0.055%
52	13.881	1798	1801	1808	rVB4	26186	51993	1.14%	0.143%
53	13.969	1812	1816	1822	rBV9	3890	8583	0.19%	0.024%
54	14.034	1822	1827	1835	rBV9	24139	49129	1.07%	0.135%
55	14.122	1836	1842	1848	rBV	276306	393783	8.60%	1.085%
56	14.263	1859	1866	1869	rBV	46474	76564	1.67%	0.211%
57	14.299	1869	1872	1877	rVB2	40195	54732	1.20%	0.151%
58	14.416	1886	1892	1901	rBV	337730	573009	12.52%	1.578%
59	14.499	1902	1906	1913	rVB10	12322	24519	0.54%	0.068%
60	14.640	1926	1930	1932	rBV5	6843	9791	0.21%	0.027%
61	14.716	1933	1943	1948	rBV	2645434	3828467	83.66%	10.546%
62	14.781	1948	1954	1966	rVB	2285318	3377752	73.81%	9.304%
63	14.904	1973	1975	1983	rVB8	19486	39018	0.85%	0.107%
64	15.022	1991	1995	1999	rVB	48799	65807	1.44%	0.181%
65	15.316	2040	2045	2051	rBV4	28541	59156	1.29%	0.163%
66	15.593	2087	2092	2097	rVB2	17905	28622	0.63%	0.079%
67	15.710	2106	2112	2116	rBV	421038	603965	13.20%	1.664%
68	15.763	2116	2121	2127	rVV	518831	770413	16.83%	2.122%
69	15.822	2127	2131	2134	rVV	55369	79229	1.73%	0.218%
70	15.887	2138	2142	2151	rVV6	48664	133039	2.91%	0.366%
71	15.969	2152	2156	2160	rVV3	27596	42082	0.92%	0.116%
72	16.081	2172	2175	2181	rVB4	34082	50382	1.10%	0.139%
73	16.157	2183	2188	2189	rBV5	12025	16184	0.35%	0.045%
74	16.204	2191	2196	2204	rVB2	71673	153606	3.36%	0.423%
75	16.457	2233	2239	2245	rVB3	58239	102106	2.23%	0.281%
76	16.563	2252	2257	2264	rBV	49160	76387	1.67%	0.210%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
 Data File : BP016525.D
 Acq On : 07 Aug 2023 19:08
 Operator : MA/JU
 Sample : 03889-01DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
 Title : SVOA CALIBRATION

77	16.645	2267	2271	2276	rVV3	28731	41889	0.92%	0.115%
78	16.769	2289	2292	2296	rVB4	27409	39451	0.86%	0.109%
79	16.922	2315	2318	2321	rVB2	15490	18482	0.40%	0.051%
80	17.193	2362	2364	2369	rVB6	9525	12752	0.28%	0.035%
81	17.251	2371	2374	2377	rBV2	24870	40409	0.88%	0.111%
82	17.293	2378	2381	2388	rVB2	46842	76080	1.66%	0.210%
83	17.363	2390	2393	2396	rBV5	12807	18623	0.41%	0.051%
84	17.481	2407	2413	2420	rBV	2993537	4265322	93.20%	11.749%
85	17.581	2425	2430	2434	rBV	431183	611018	13.35%	1.683%
86	17.681	2444	2447	2453	rVB4	22230	35611	0.78%	0.098%
87	17.845	2471	2475	2478	rBV2	32500	45711	1.00%	0.126%
88	17.892	2479	2483	2488	rVB	58086	80348	1.76%	0.221%
89	18.316	2550	2555	2559	rBV2	76401	126693	2.77%	0.349%
90	18.387	2564	2567	2574	rVB3	48384	88549	1.93%	0.244%
91	18.463	2575	2580	2585	rVB3	64772	104627	2.29%	0.288%
92	18.534	2587	2592	2598	rVB2	120101	161671	3.53%	0.445%
93	18.769	2628	2632	2636	rBV2	43483	53728	1.17%	0.148%
94	19.481	2749	2753	2760	rVB	263668	340404	7.44%	0.938%
95	19.551	2763	2765	2769	rBV4	39441	48993	1.07%	0.135%
96	19.810	2804	2809	2812	rBV	581947	784728	17.15%	2.162%
97	20.281	2885	2889	2897	rBV	100265	175201	3.83%	0.483%
98	21.575	3104	3109	3117	rBV	3153445	4333423	94.69%	11.937%
99	23.992	3516	3520	3531	rVB	422455	838955	18.33%	2.311%
100	24.169	3543	3550	3562	rVB	2143608	4576460	100.00%	12.606%




Sum of corrected areas: 36302715

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016525.D
Acq On : 07 Aug 2023 19:08
Operator : MA/JU
Sample : 03889-01DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

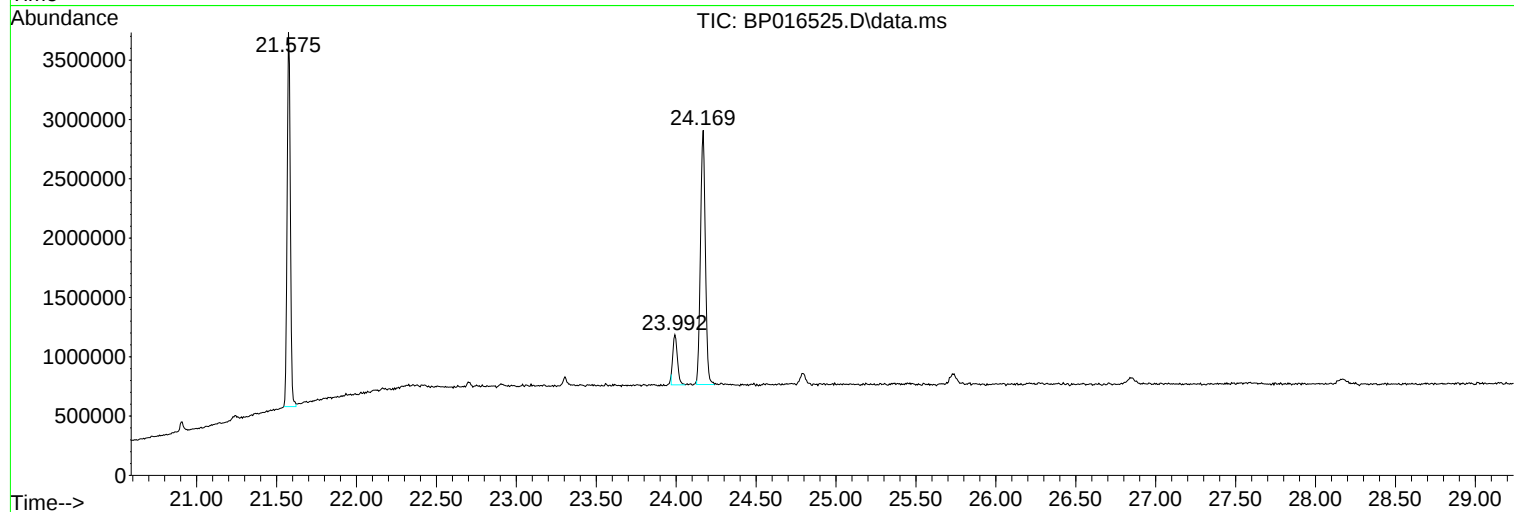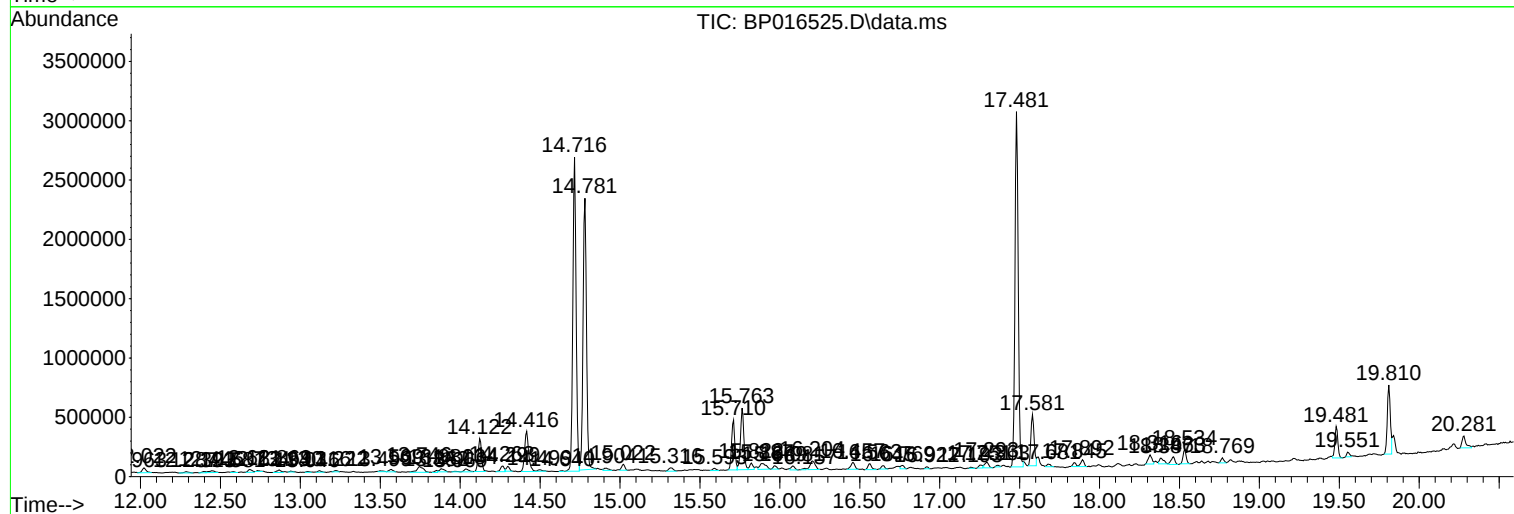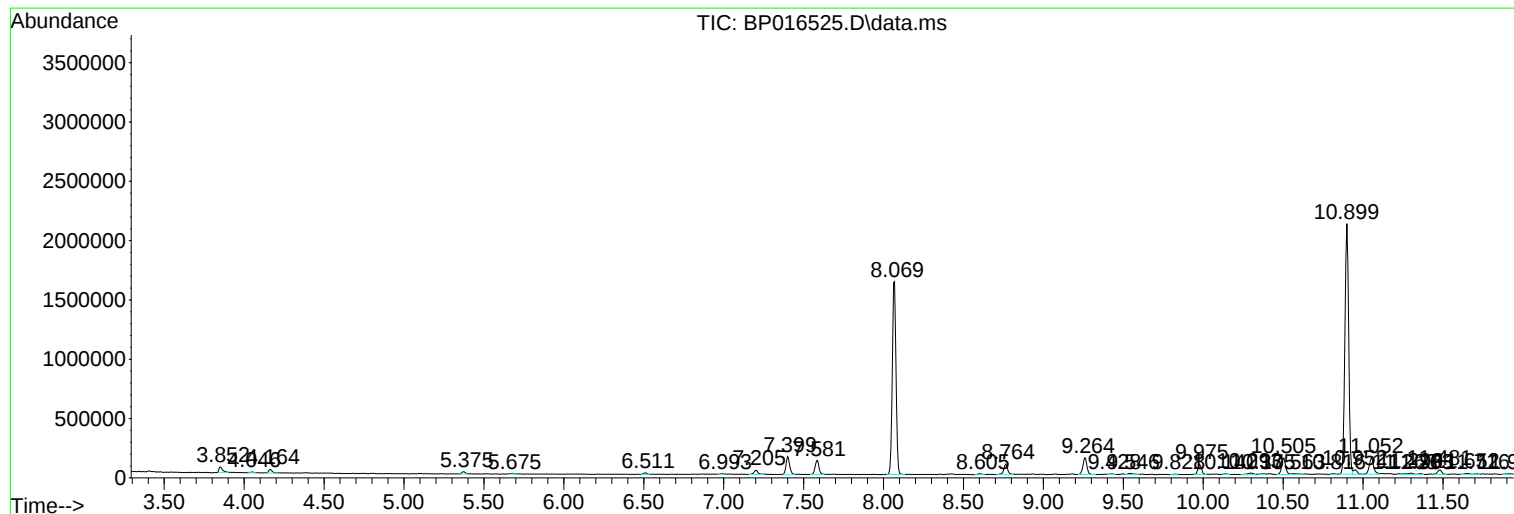

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016525.D
Acq On : 07 Aug 2023 19:08
Operator : MA/JU
Sample : 03889-01DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080723\
Data File : BP016525.D
Acq On : 07 Aug 2023 19:08
Operator : MA/JU
Sample : 03889-01DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------